
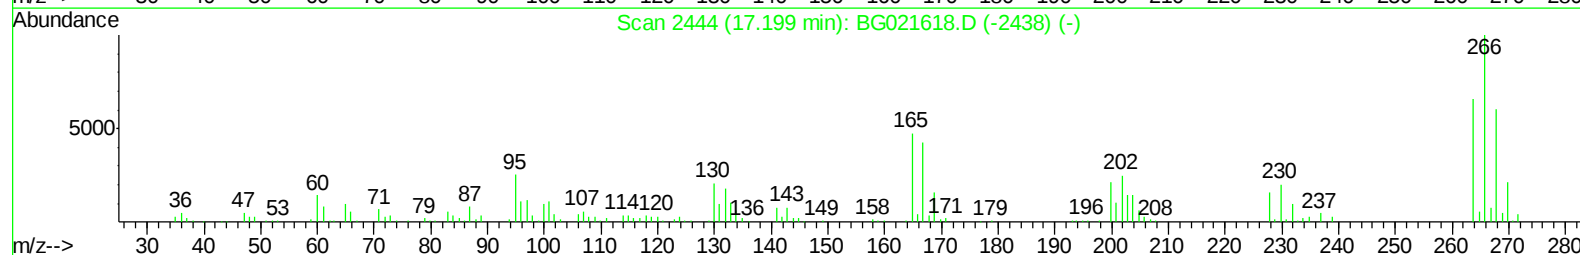
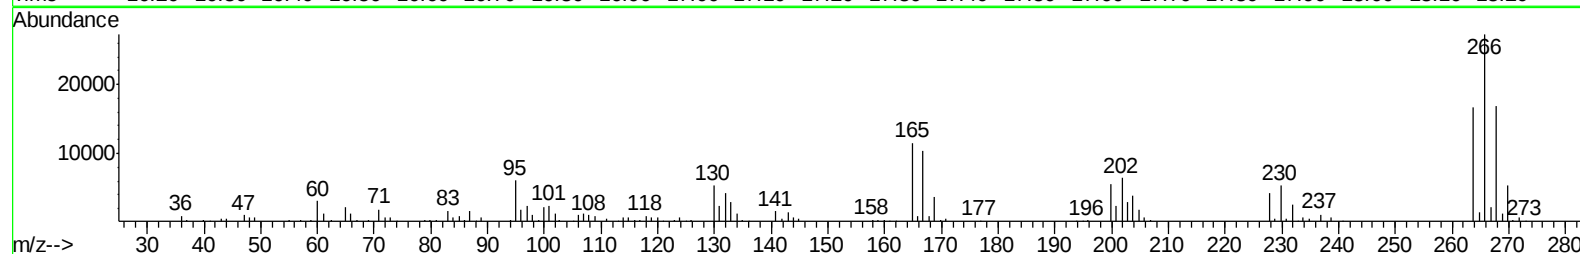


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041916\
Data File : BG021753.D
Acq On : 19 Apr 2016 3:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 04:38:05 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

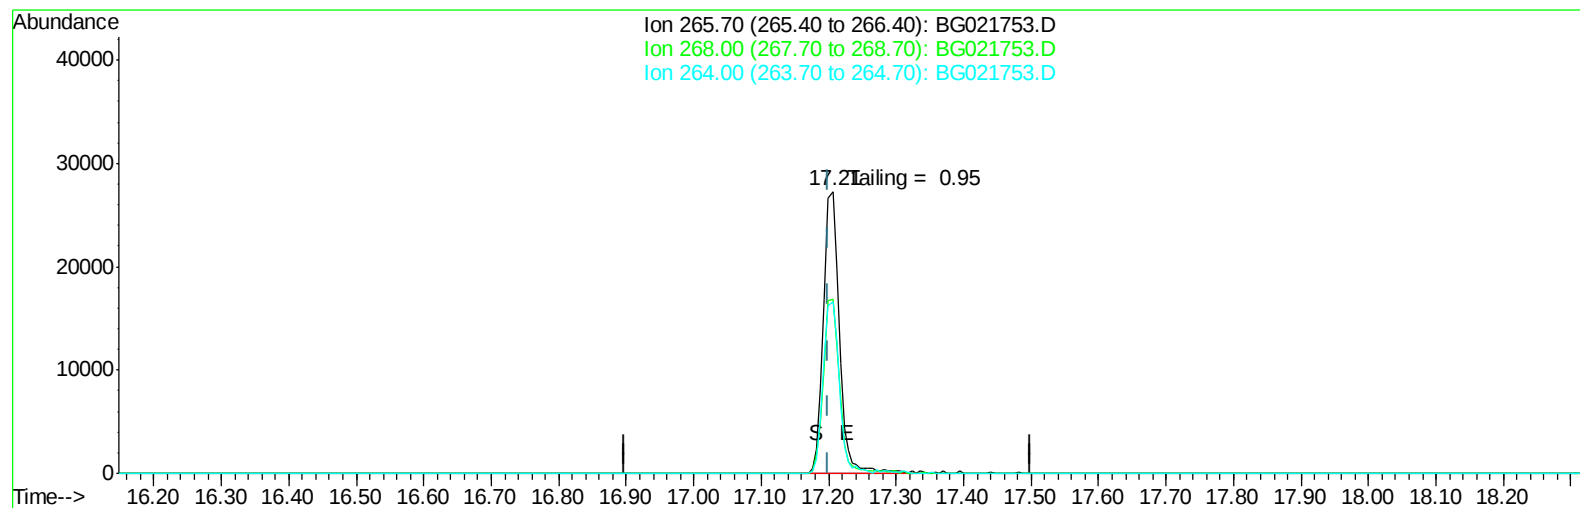

TIC: BG021753.D

(69) Pentachlorophenol (C)




17.206min (+0.007) 0.00ng

response 43860

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	61.71
264.00	67.20	61.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041916\
Data File : BG021753.D
Acq On : 19 Apr 2016 3:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 04:38:05 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

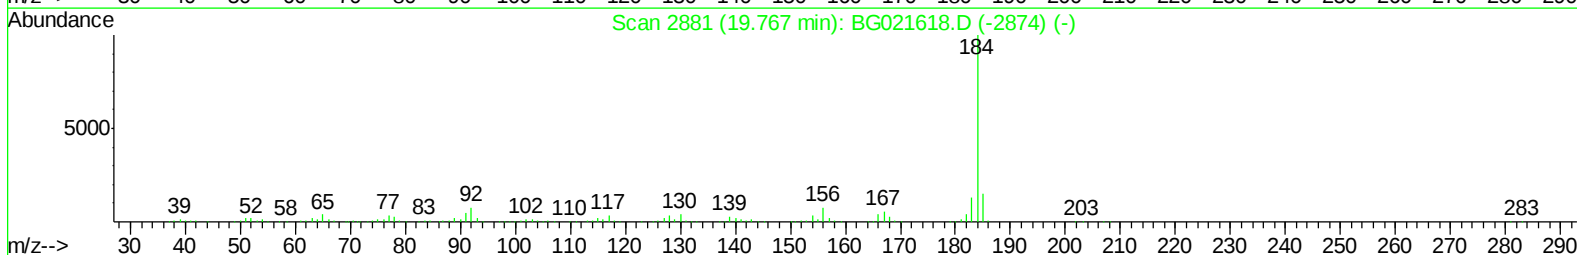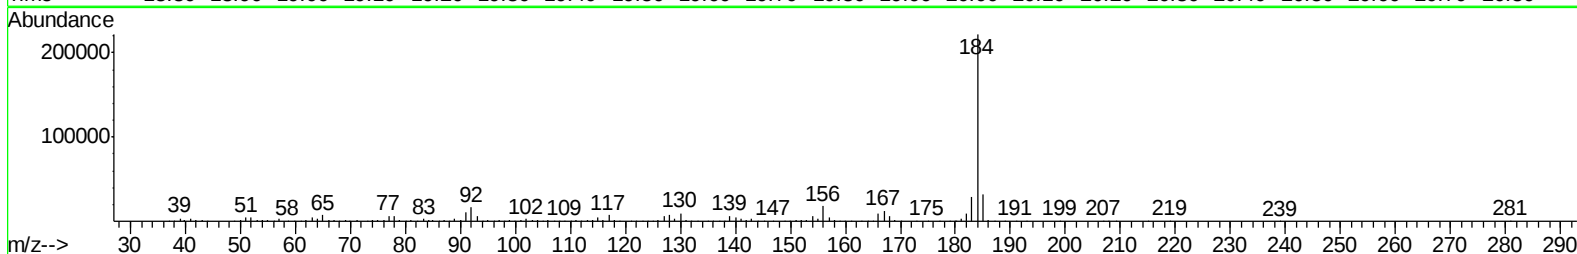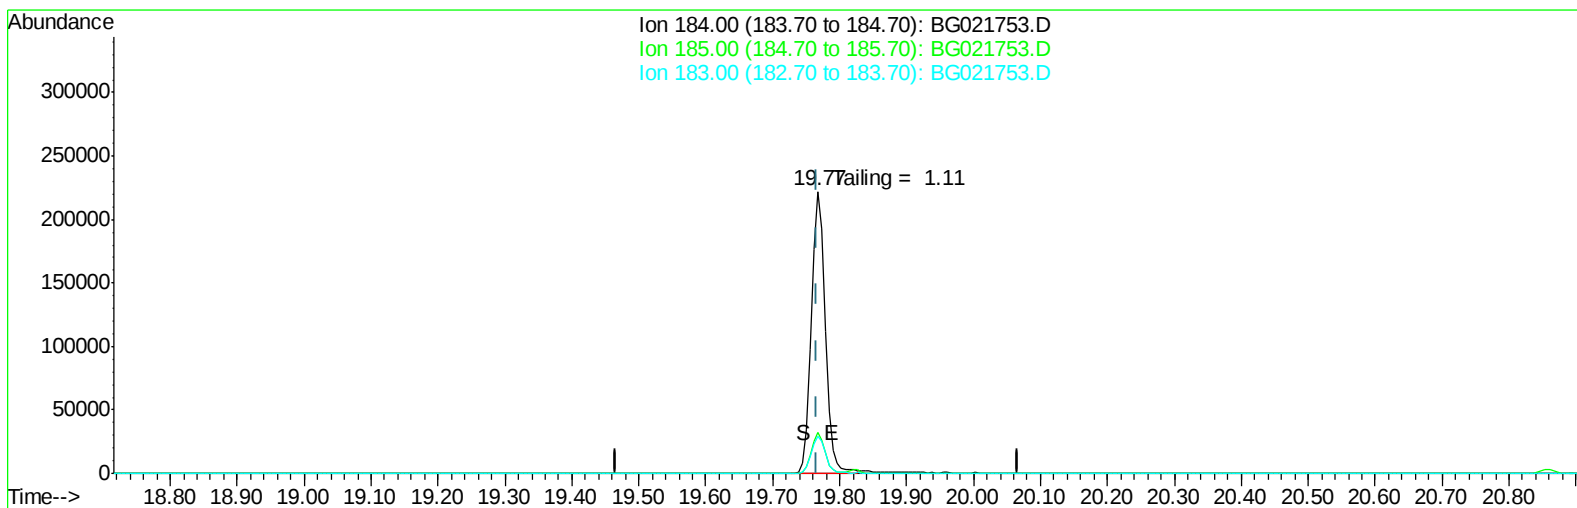

TIC: BG021753.D

(76) Benzidine

19.767min (+0.001) 75631.43ng

response 334384

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.78
183.00	12.80	13.36
0.00	0.00	0.00