


Data Path : Z:\HPCHEM1\BNA G\Data\BG041916\
 Data File : BG021738.D
 Acq On : 18 Apr 2016 15:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

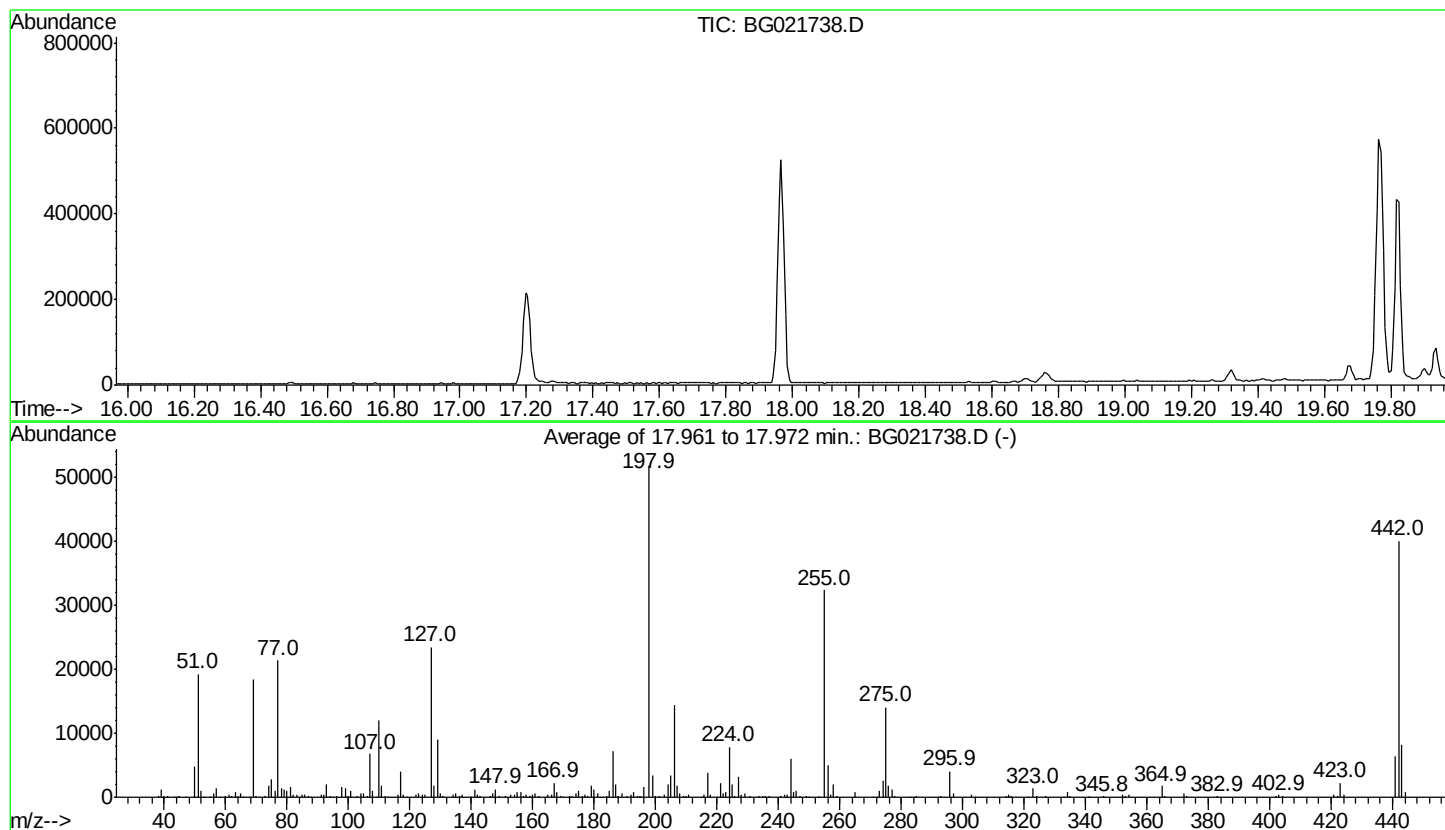

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	19271	PASS
68	69	0.00	2	0.5	98	PASS
69	198	0.00	100	35.4	18367	PASS
70	69	0.00	2	0.7	133	PASS
127	198	10	80	45.3	23498	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51869	PASS
199	198	5	9	6.7	3485	PASS
275	198	10	60	27.2	14105	PASS
365	198	1	100	3.4	1775	PASS
441	442	0.01	24	16.0	6411	PASS
442	198	50	100	77.3	40093	PASS
443	442	15	24	20.2	8116	PASS