


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041916\
 Data File : BG021753.D
 Acq On : 19 Apr 2016 3:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

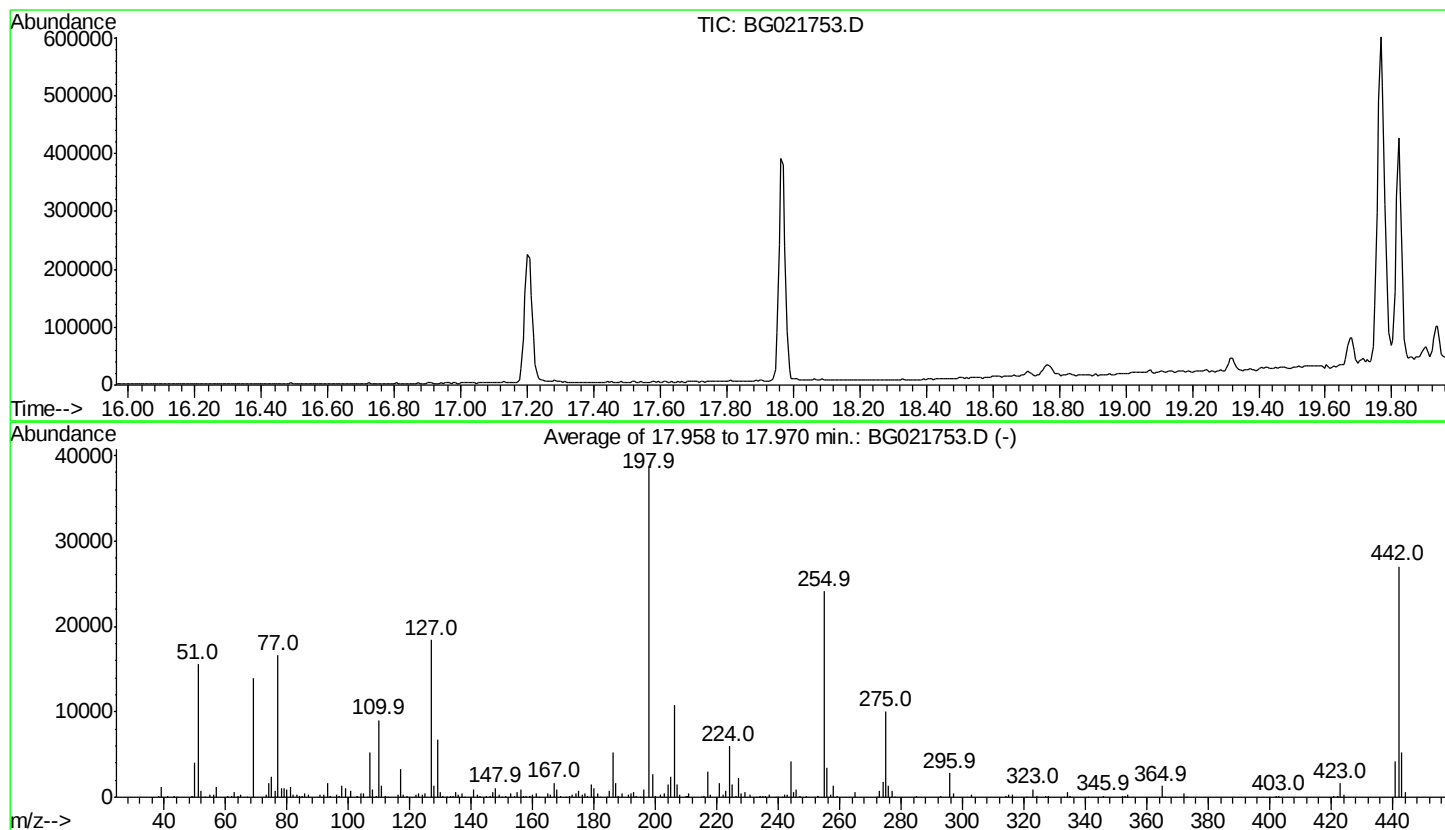

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	15566	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.9	13913	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	18362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38800	PASS
199	198	5	9	7.0	2730	PASS
275	198	10	60	25.7	9975	PASS
365	198	1	100	3.4	1306	PASS
441	442	0.01	24	15.8	4257	PASS
442	198	50	100	69.6	27009	PASS
443	442	15	24	19.5	5278	PASS