
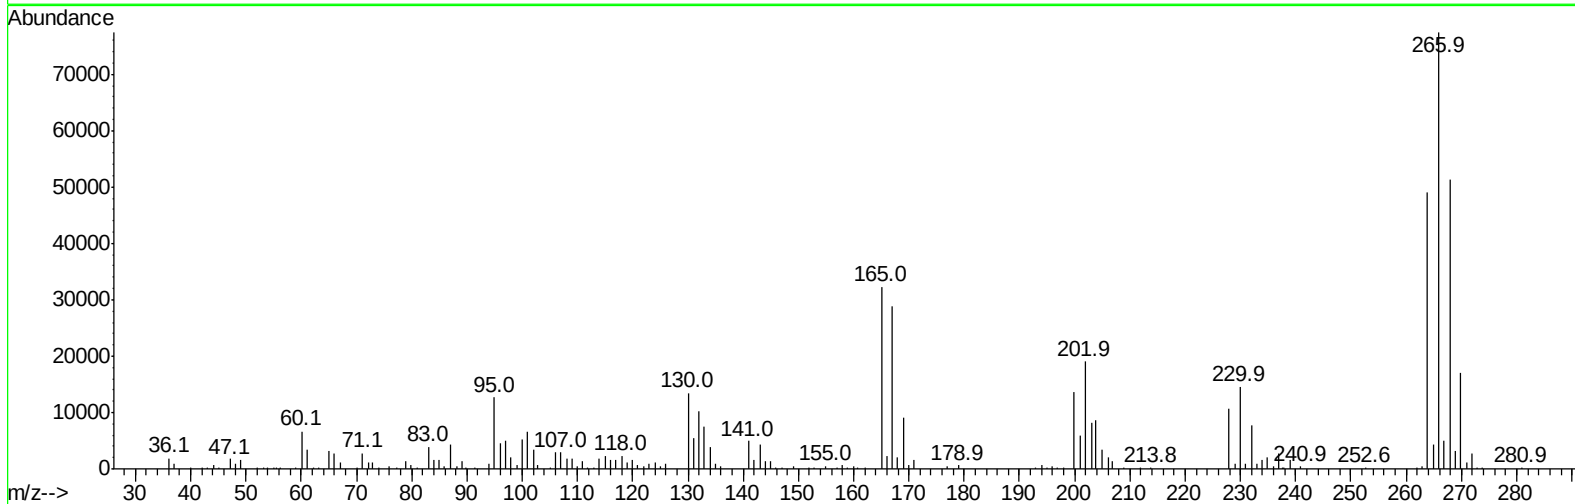


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041917\
Data File : BG026654.D
Acq On : 19 Apr 2017 13:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 08:13:09 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

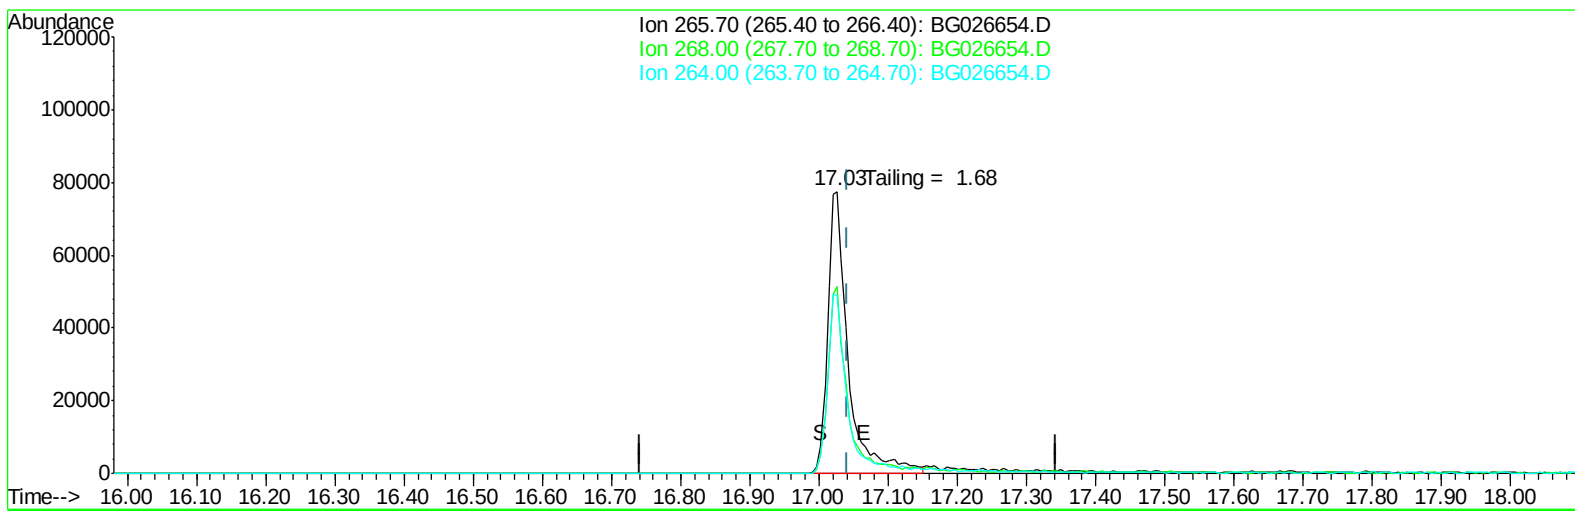

TIC: BG026654.D

(69) Pentachlorophenol (C)



17.026min (-0.016) 0.00ng

response 149993

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	66.19
264.00	62.60	63.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041917\
Data File : BG026654.D
Acq On : 19 Apr 2017 13:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 08:13:09 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

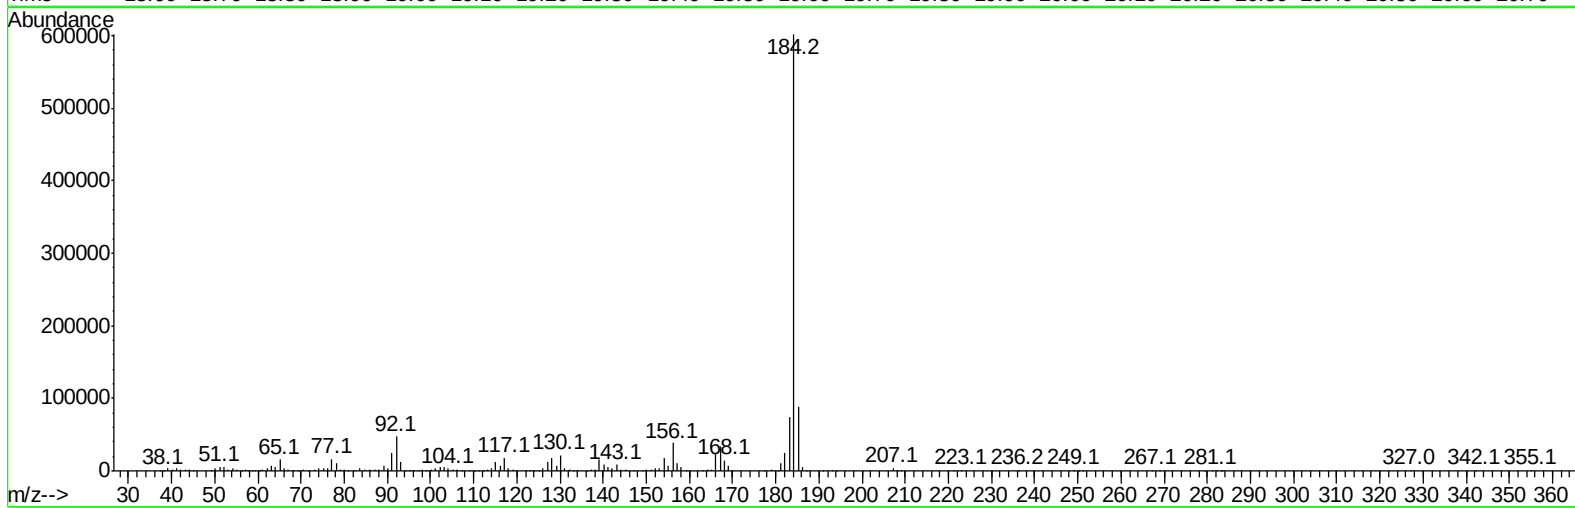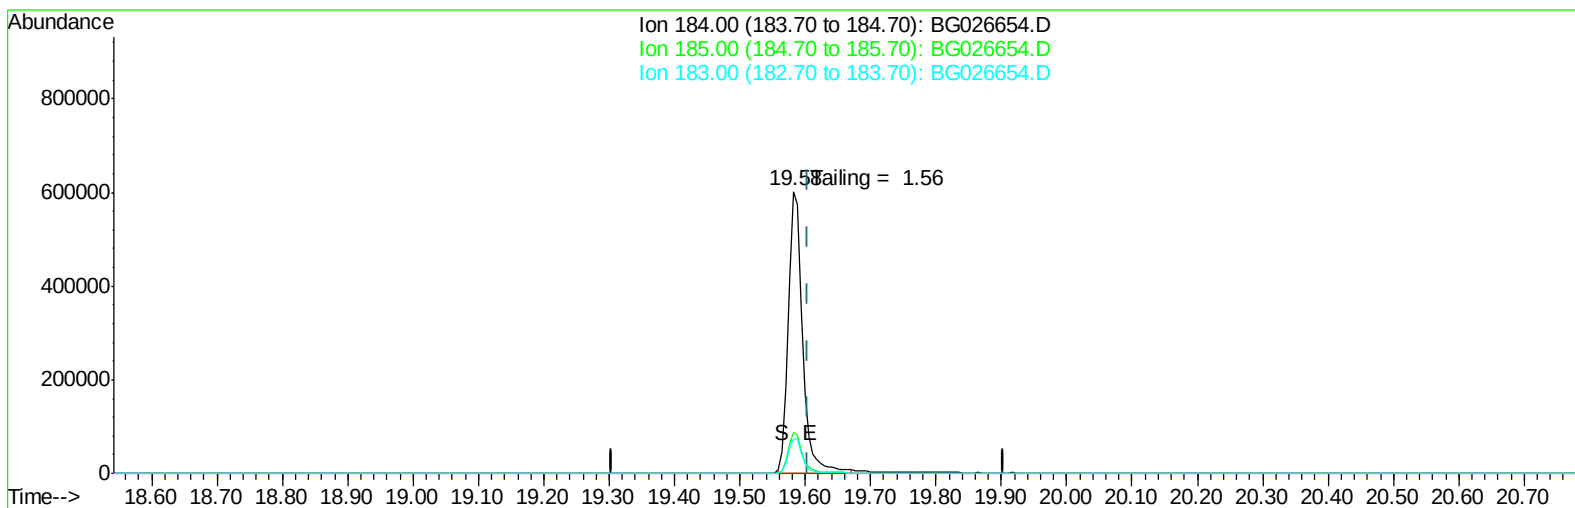

TIC: BG026654.D

(76) Benzidine

19.582min (-0.022) 488149.89ng

response 946788

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.65
183.00	13.80	12.25
0.00	0.00	0.00