
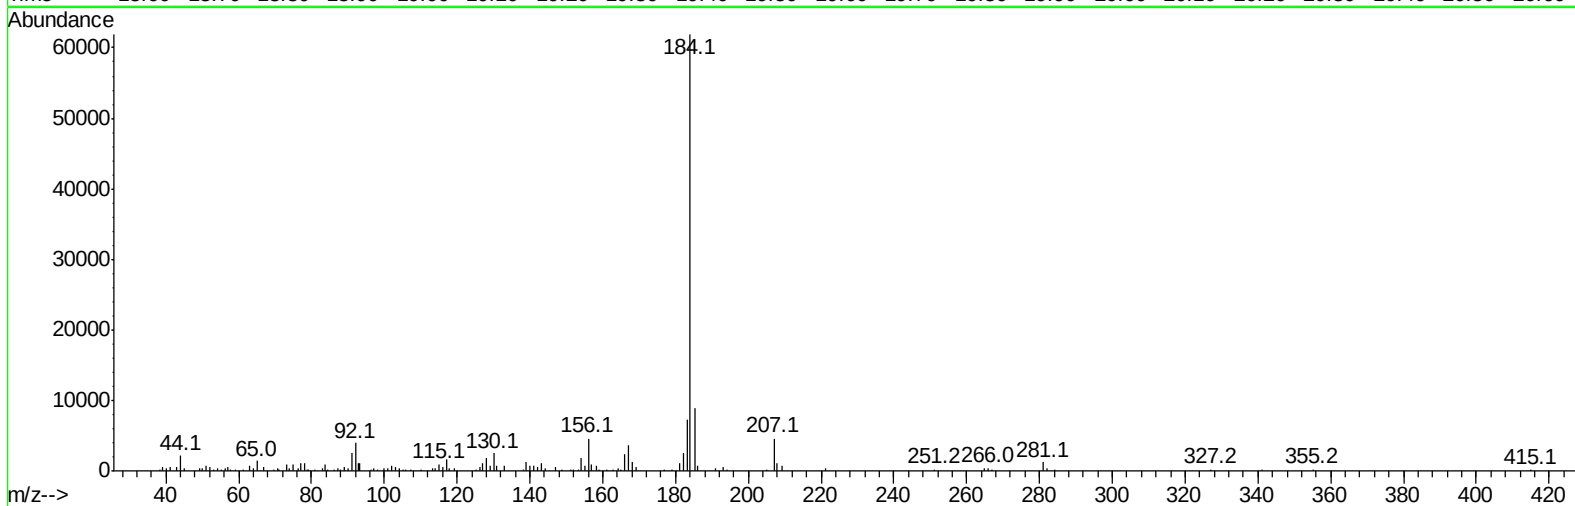


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041917\
Data File : BG026670.D
Acq On : 20 Apr 2017 00:49
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 08:18:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

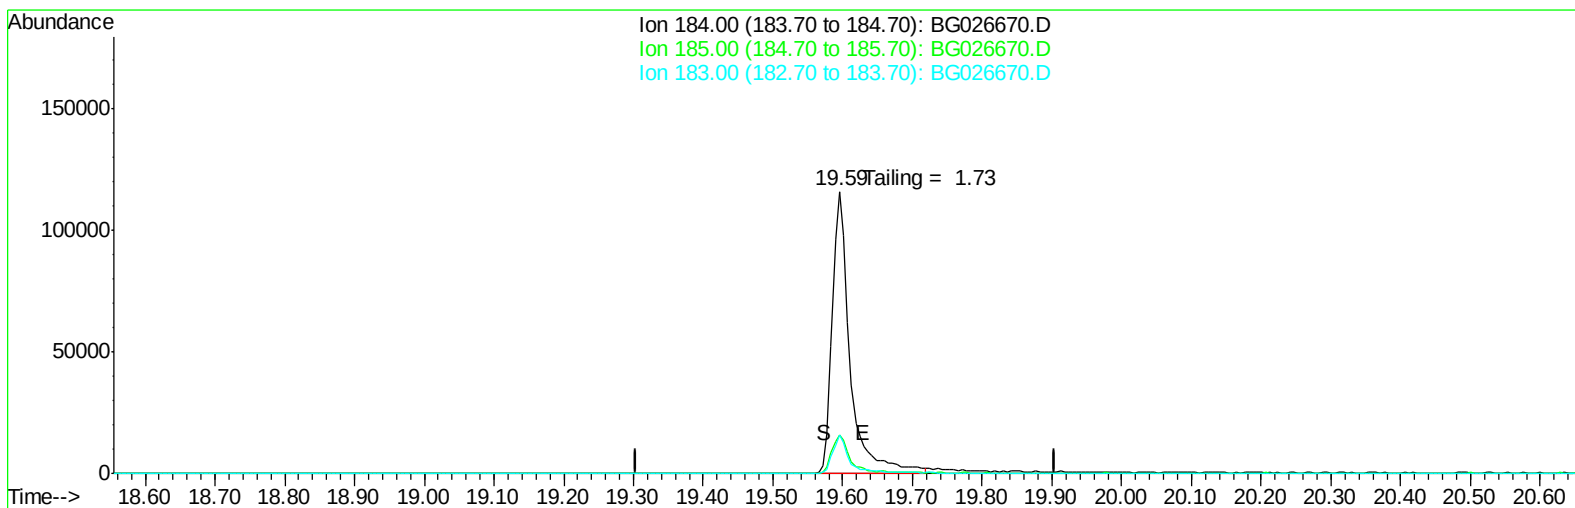

TIC: BG026670.D

(76) Benzidine



19.604min (-19.604) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.30	0.00#
183.00	13.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041917\
Data File : BG026670.D
Acq On : 20 Apr 2017 00:49
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 08:18:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

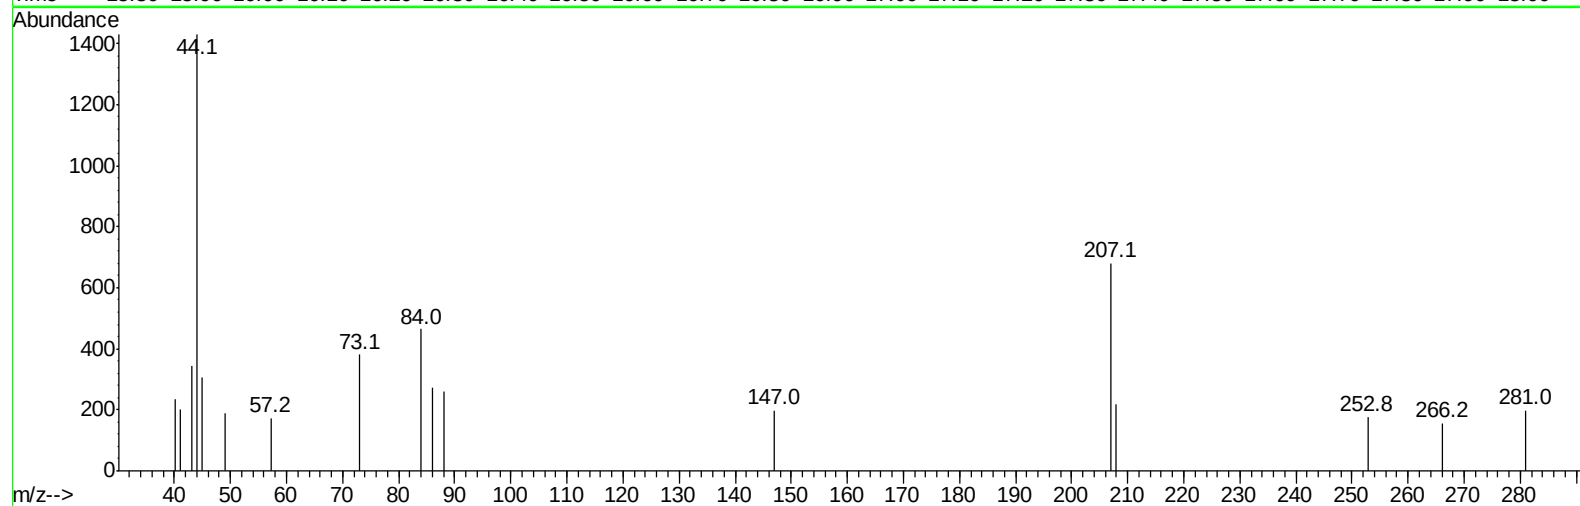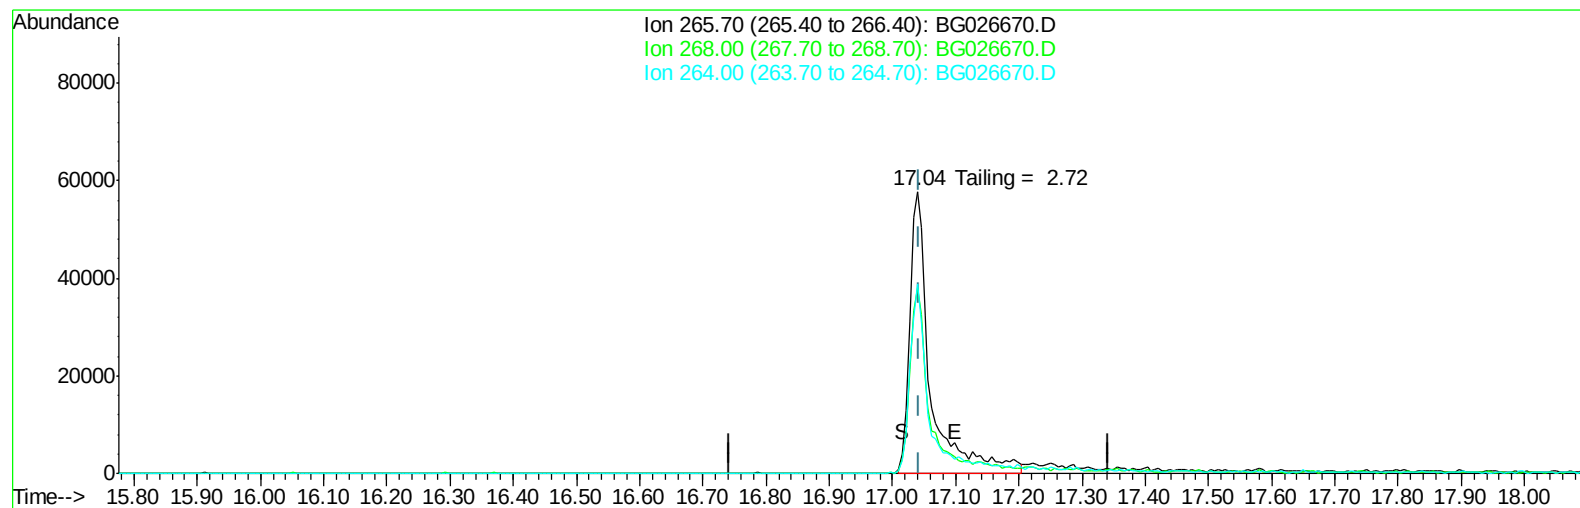

TIC: BG026670.D

(69) Pentachlorophenol (C)

16.786min (-0.256) 135.33ng

response 55

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00