


Data Path : Z:\HPCHEM1\BNA G\Data\BG041917\
 Data File : BG026654.D
 Acq On : 19 Apr 2017 13:04
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 18 18:04:39 2017

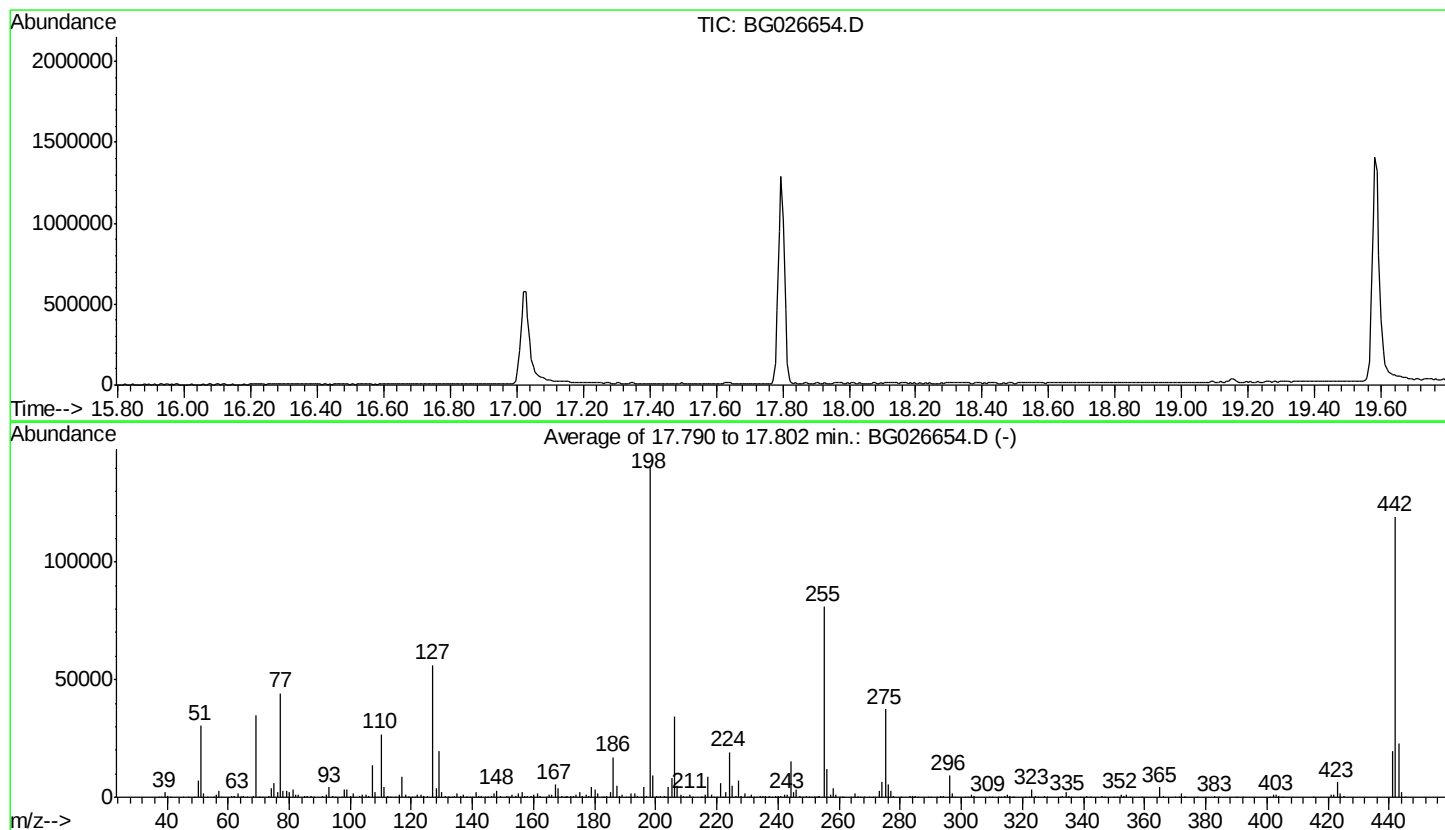

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	30291	PASS
68	69	0.00	2	1.0	353	PASS
69	198	0.00	100	24.6	34668	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	39.8	56077	PASS
197	198	0.00	2	0.4	494	PASS
198	198	100	100	100.0	141002	PASS
199	198	5	9	6.7	9489	PASS
275	198	10	60	26.5	37317	PASS
365	198	1	100	2.9	4105	PASS
441	442	0.01	24	16.2	19384	PASS
442	198	50	100	84.7	119488	PASS
443	442	15	24	19.1	22837	PASS