


Data Path : Z:\HPCHEM1\BNA_G\Data\BG041917\
 Data File : BG026670.D
 Acq On : 20 Apr 2017 00:49
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 18 18:04:39 2017

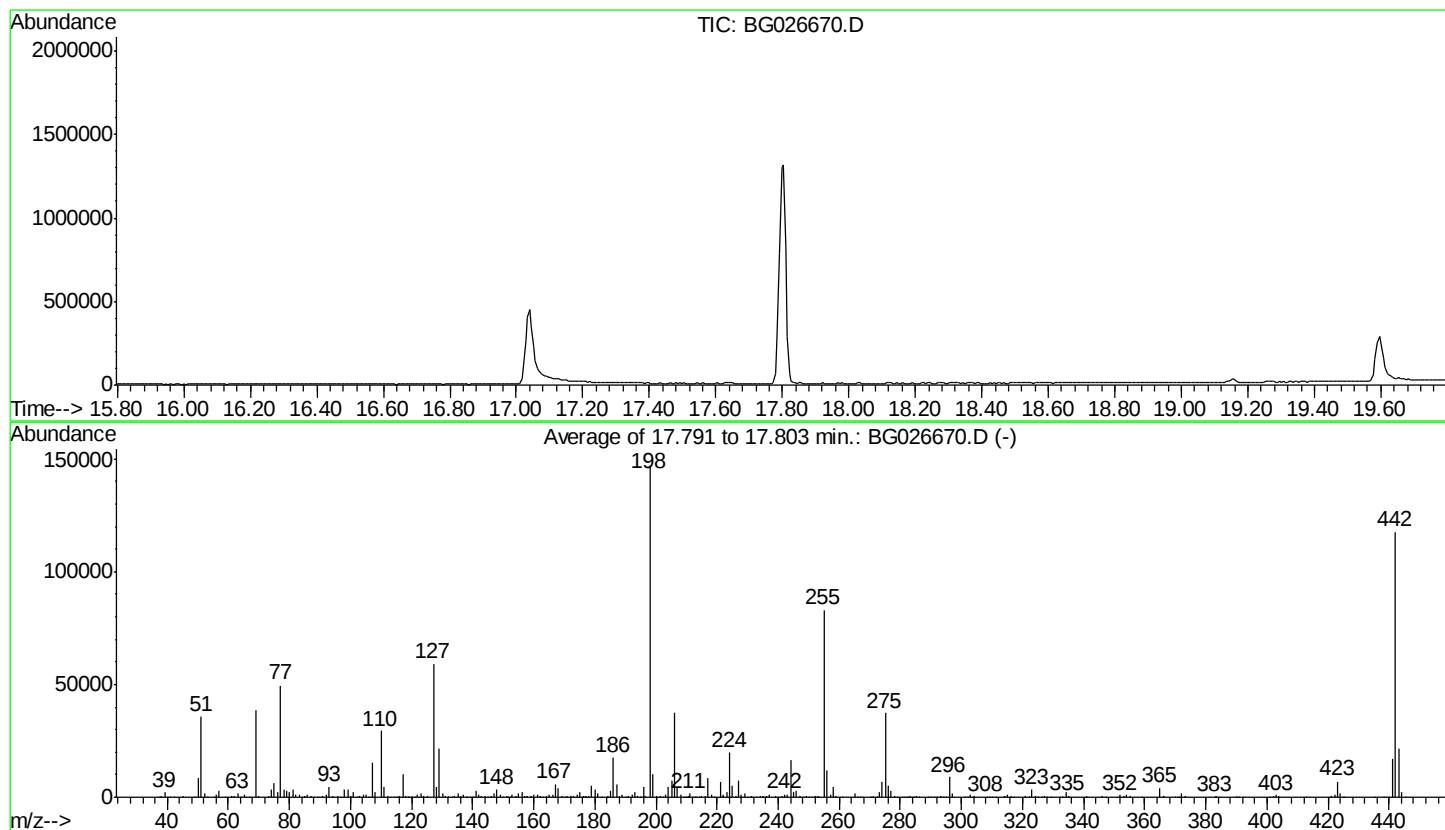

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.1	35488	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.1	38400	PASS
70	69	0.00	2	0.8	308	PASS
127	198	10	80	40.2	59096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146965	PASS
199	198	5	9	6.9	10213	PASS
275	198	10	60	25.5	37437	PASS
365	198	1	100	2.8	4144	PASS
441	442	0.01	24	14.5	17096	PASS
442	198	50	100	80.1	117728	PASS
443	442	15	24	18.3	21527	PASS