
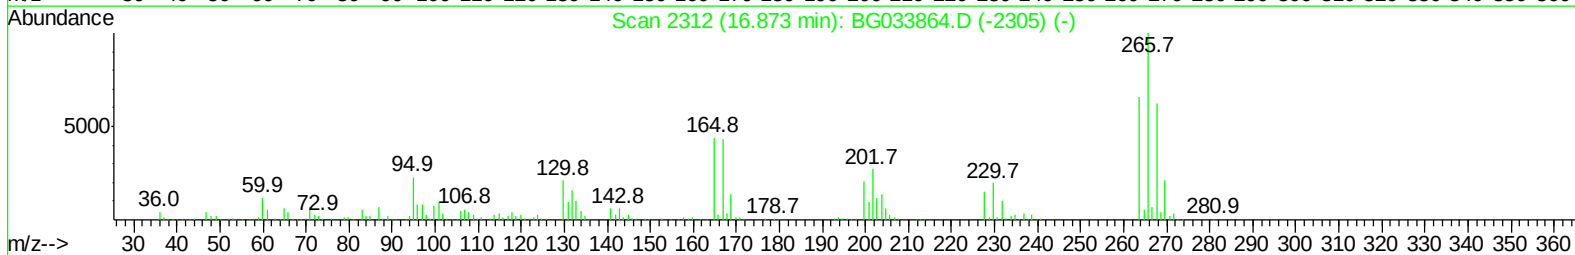
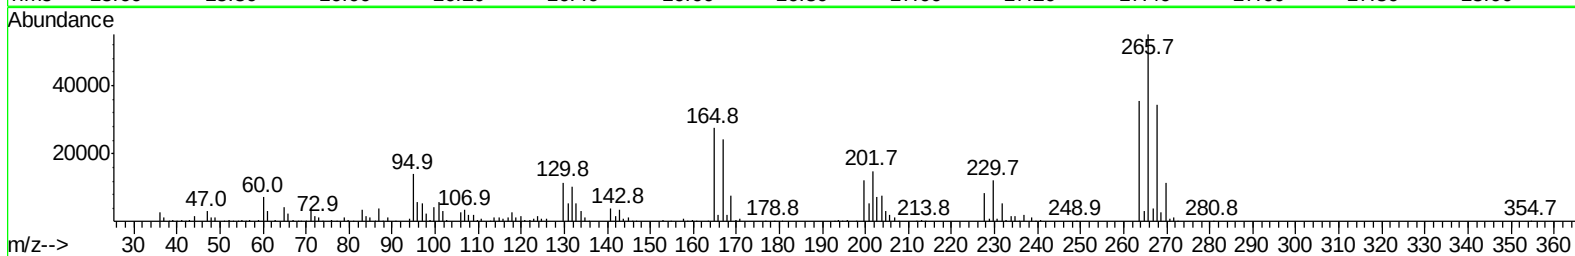


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041918\  
Data File : BG033860.D  
Acq On : 19 Apr 2018 8:42  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:11:22 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 19 13:56:22 2018  
Response via : Initial Calibration

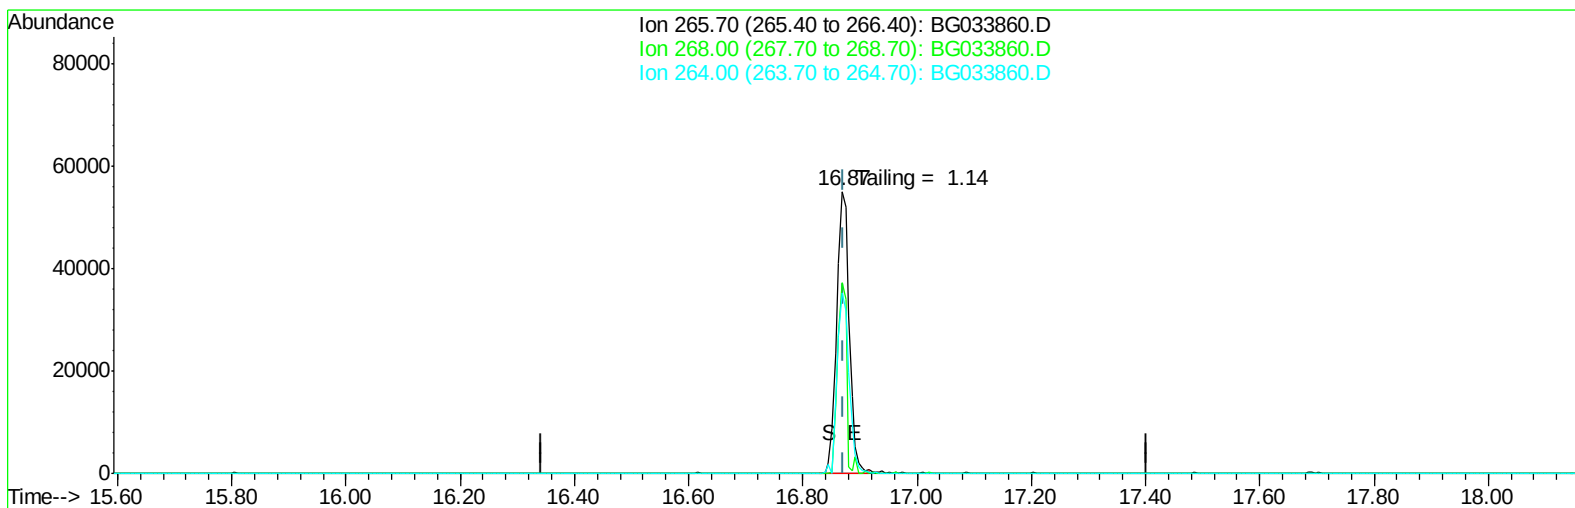

TIC: BG033860.D

(69) Pentachlorophenol (C)




16.869min (-0.004) 27543.51ng

response 84423

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 67.80 |
| 264.00 | 62.00 | 70.01 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041918\  
Data File : BG033860.D  
Acq On : 19 Apr 2018 8:42  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:11:22 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 19 13:56:22 2018  
Response via : Initial Calibration

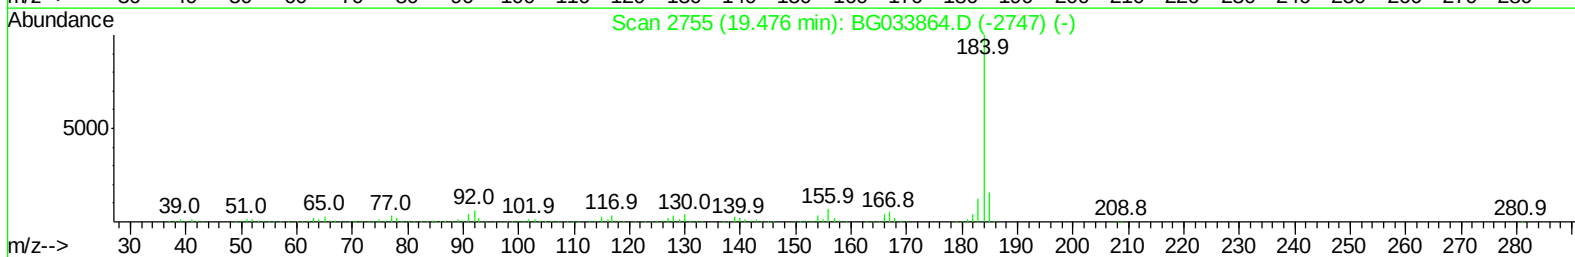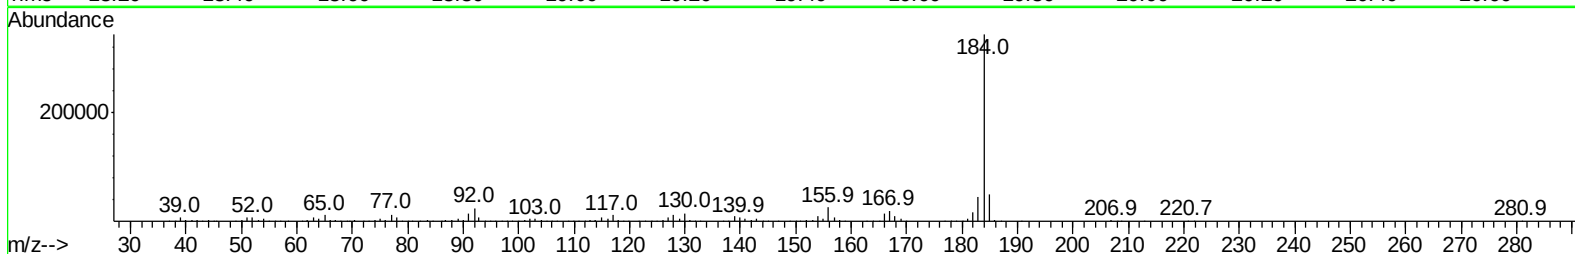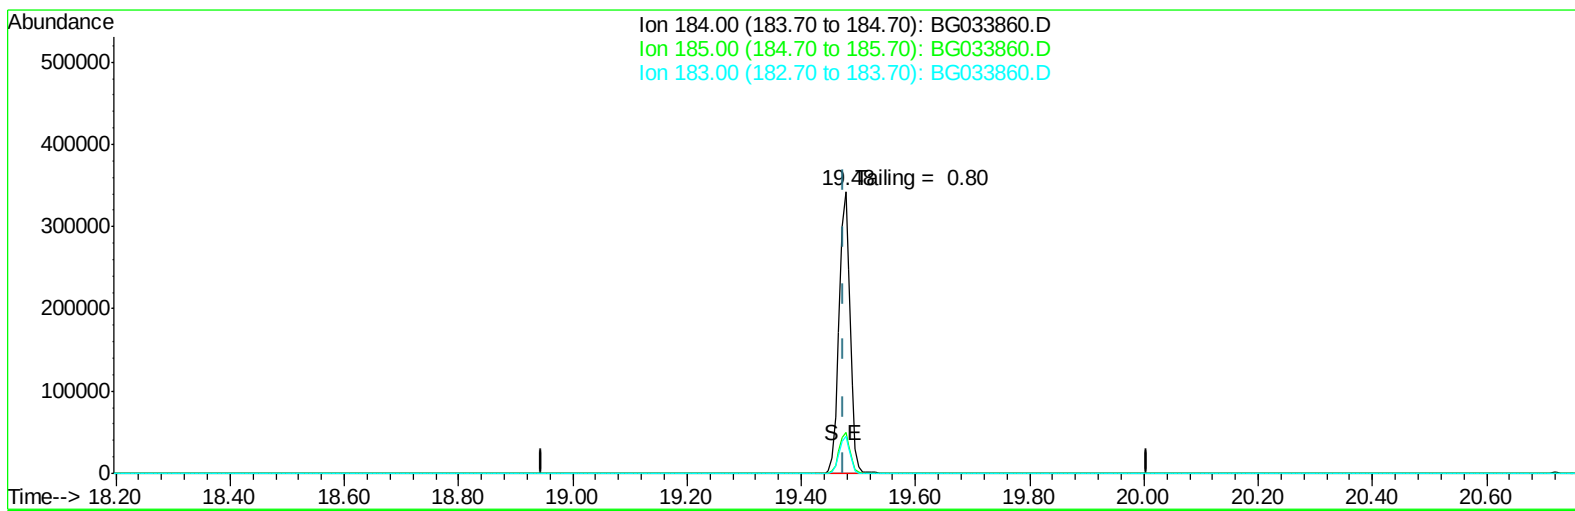

TIC: BG033860.D

(76) Benzidine

19.477min (+0.001) 0.00ng

response 459147

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.63 |
| 183.00 | 13.30 | 13.26 |
| 0.00   | 0.00  | 0.00  |