
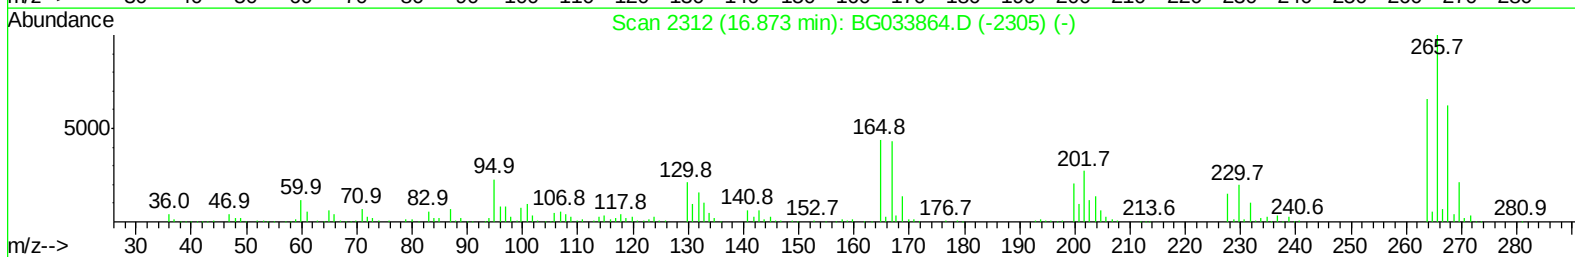
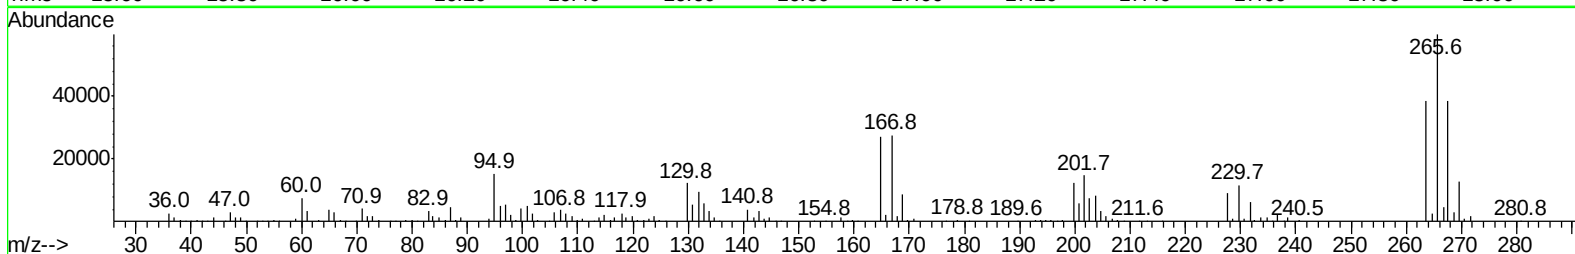


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041918\
Data File : BG033869.D
Acq On : 19 Apr 2018 14:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:12:49 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

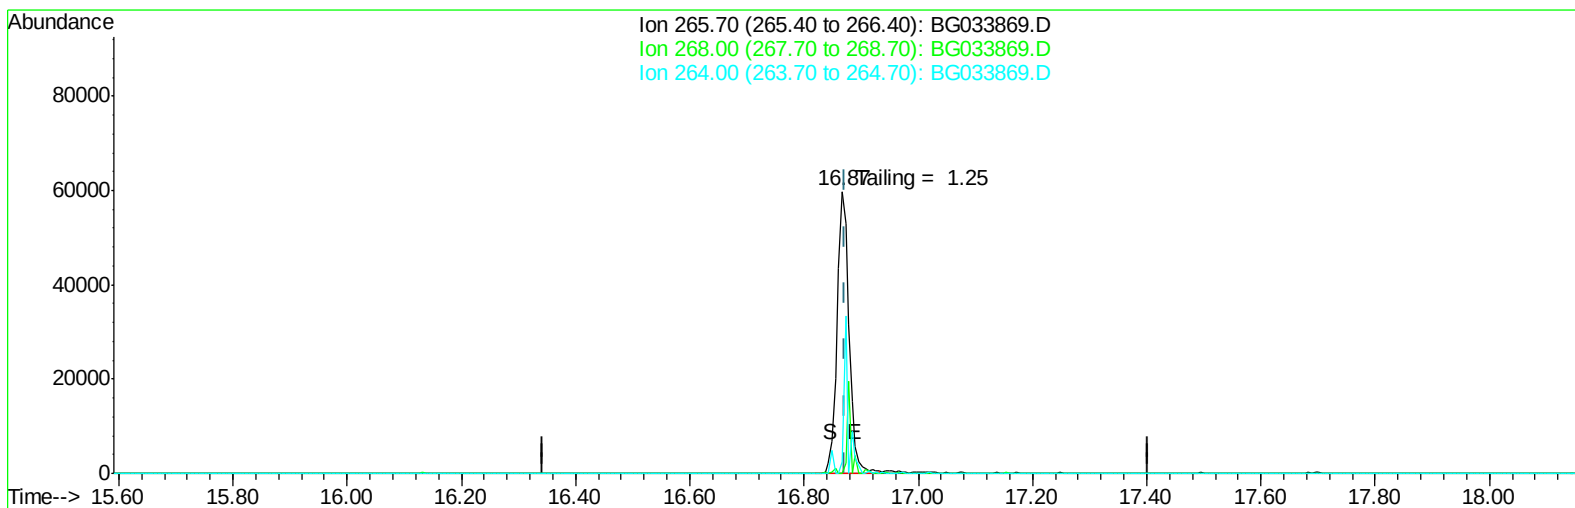

TIC: BG033869.D

(69) Pentachlorophenol (C)




16.866min (-0.007) 29565.80ng

response 86578

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	4.75#
264.00	62.00	4.30#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041918\
Data File : BG033869.D
Acq On : 19 Apr 2018 14:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:12:49 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

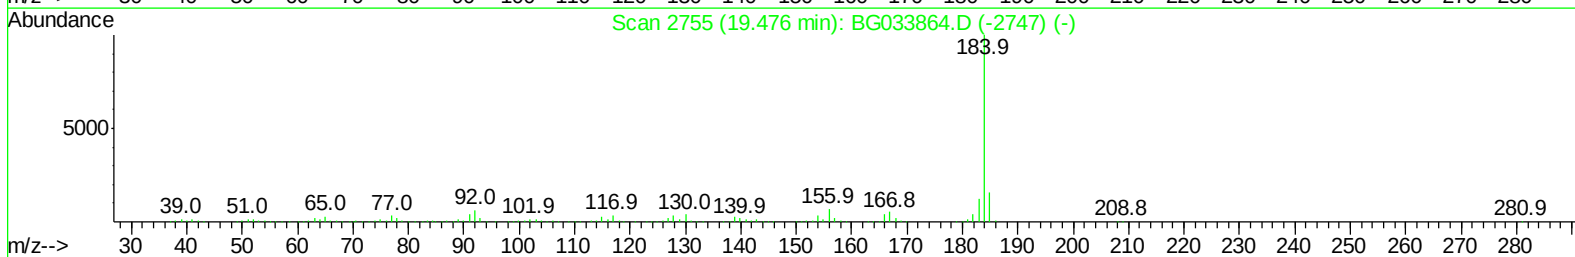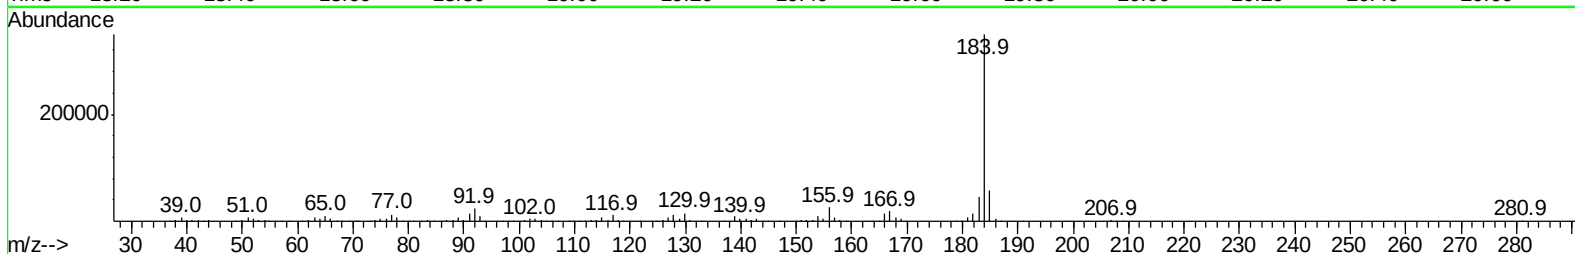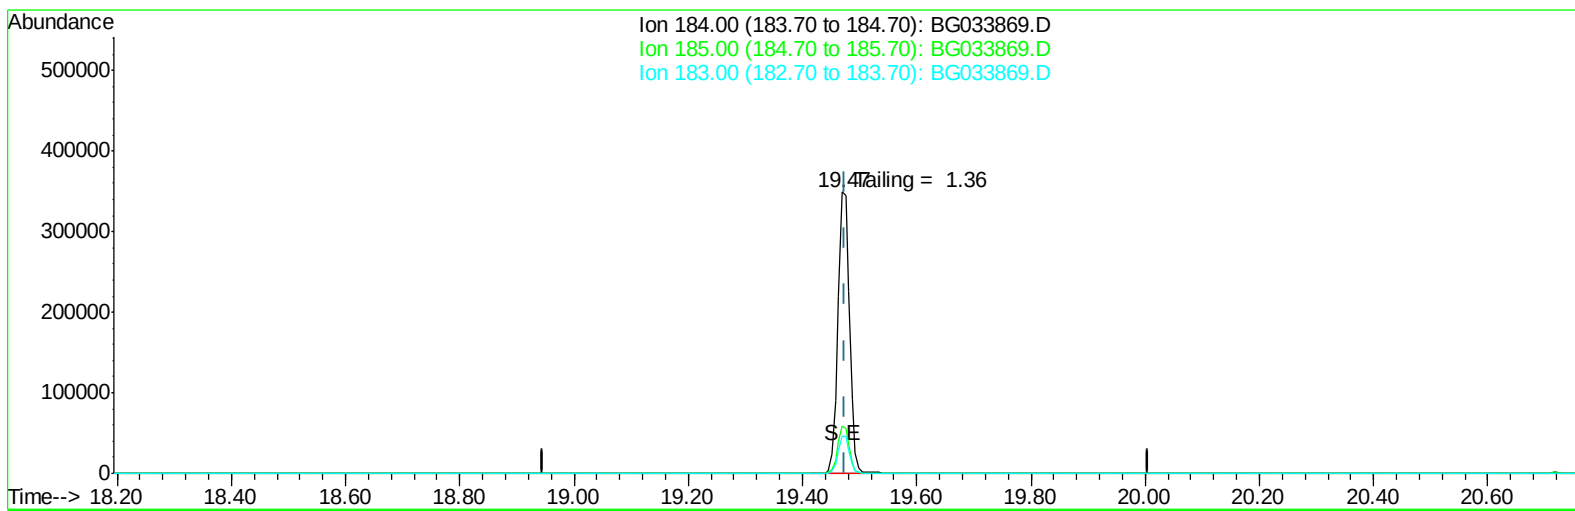

TIC: BG033869.D

(76) Benzidine

19.469min (-0.007) 0.00ng

response 491356

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.79#
183.00	13.30	13.30
0.00	0.00	0.00