


Data Path : Z:\HPCHEM1\BNA G\Data\BG041918\
 Data File : BG033860.D
 Acq On : 19 Apr 2018 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

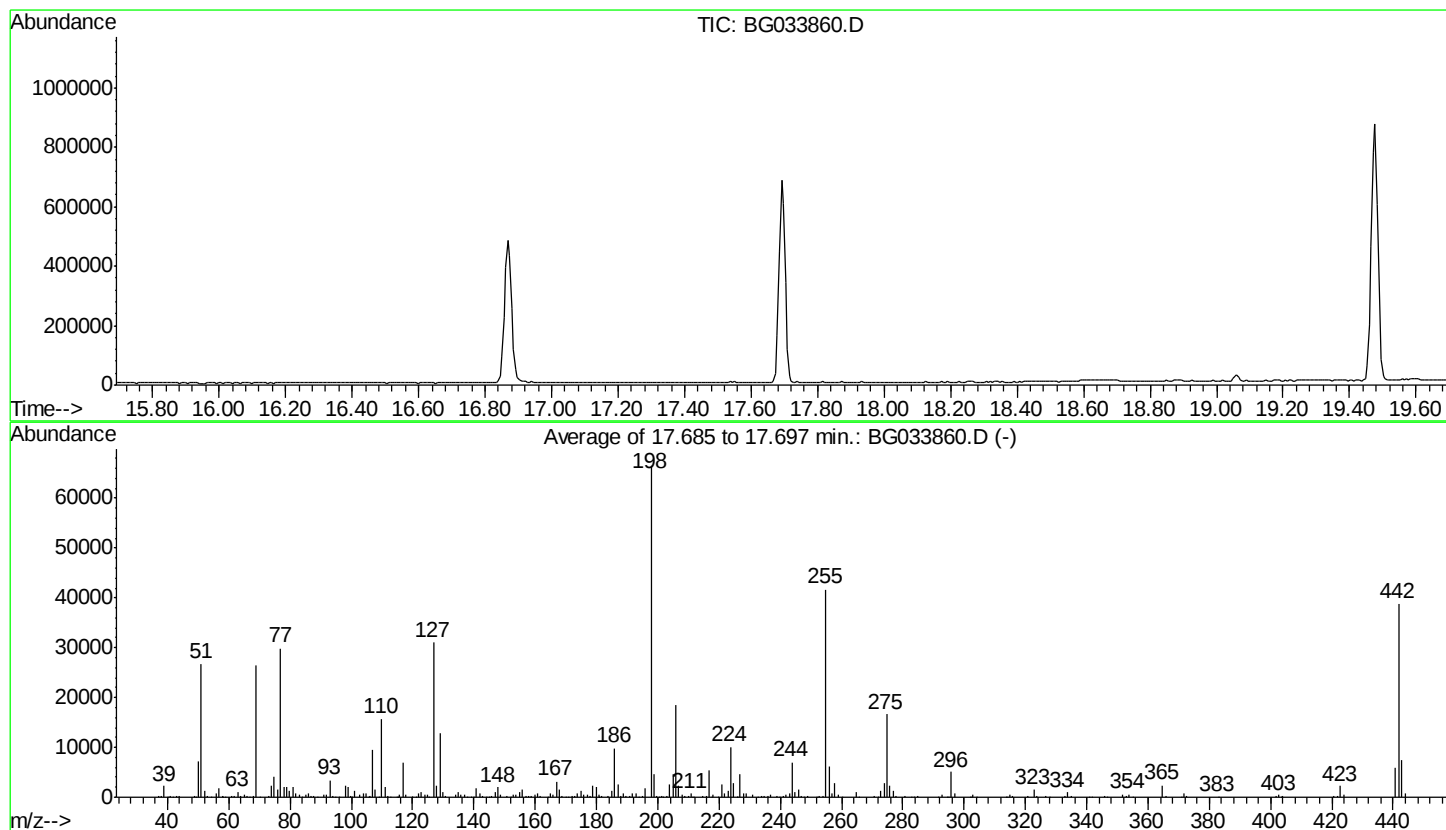

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	26777	PASS
68	69	0.00	2	0.8	210	PASS
69	198	0.00	100	39.7	26410	PASS
70	69	0.00	2	0.5	133	PASS
127	198	10	80	46.6	30997	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66552	PASS
199	198	5	9	6.9	4615	PASS
275	198	10	60	25.0	16613	PASS
365	198	1	100	3.5	2334	PASS
441	443	0.01	100	79.9	6001	PASS
442	198	50	100	58.4	38874	PASS
443	442	15	24	19.3	7508	PASS