


Data Path : Z:\HPCHEM1\BNA G\Data\BG041918\
 Data File : BG033869.D
 Acq On : 19 Apr 2018 14:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

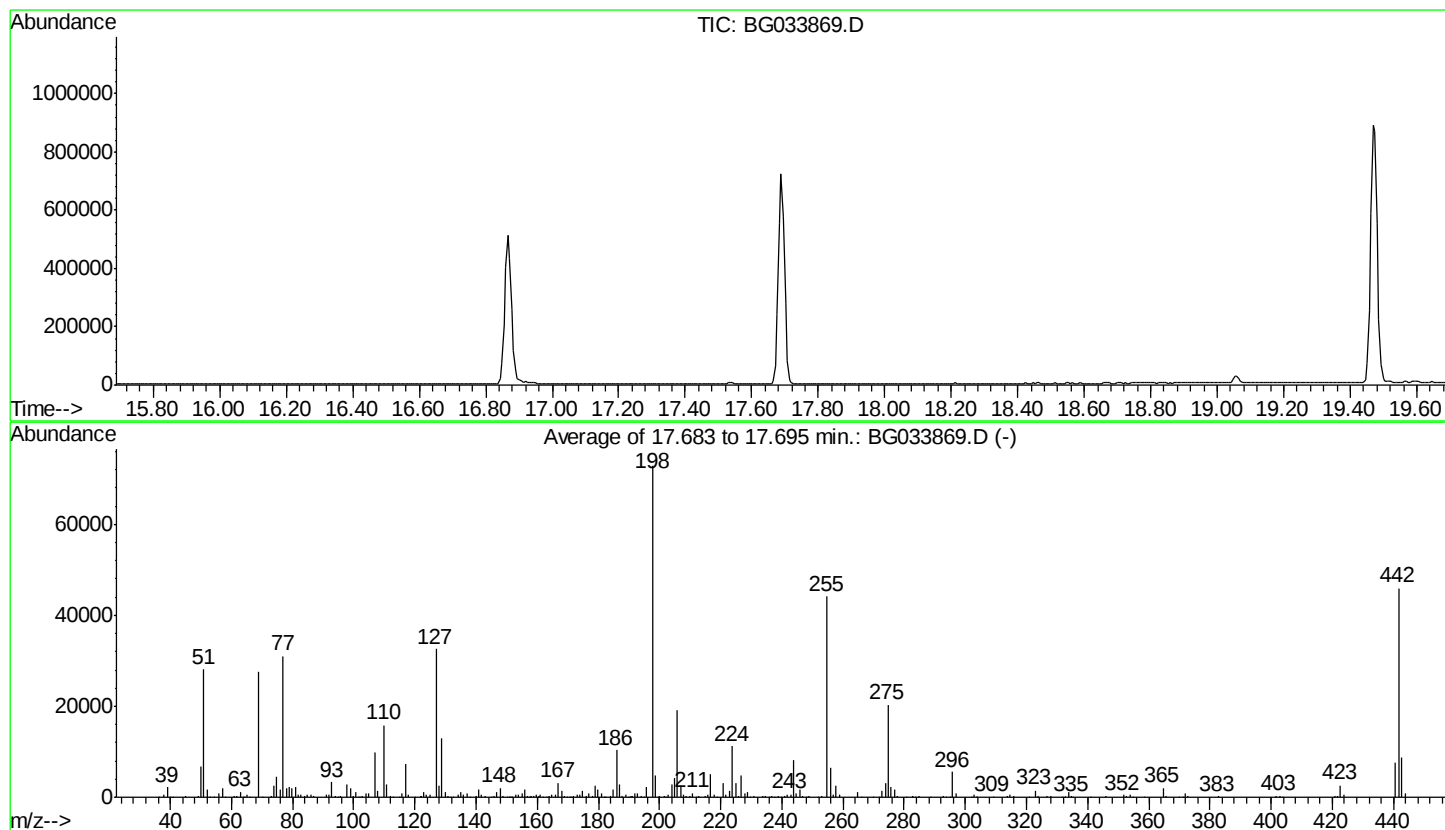

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	28013	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.7	27501	PASS
70	69	0.00	2	0.4	121	PASS
127	198	10	80	44.7	32570	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72896	PASS
199	198	5	9	6.7	4860	PASS
275	198	10	60	27.8	20280	PASS
365	198	1	100	2.8	2038	PASS
441	443	0.01	100	86.6	7528	PASS
442	198	50	100	63.0	45936	PASS
443	442	15	24	18.9	8688	PASS