
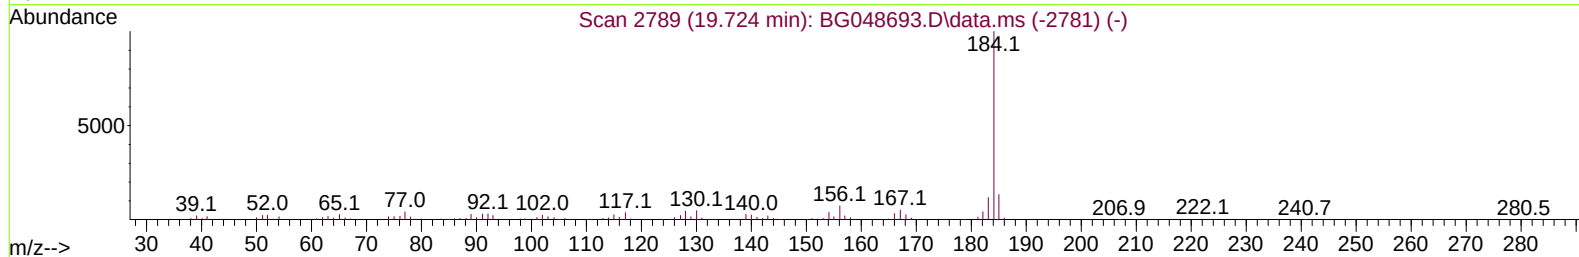
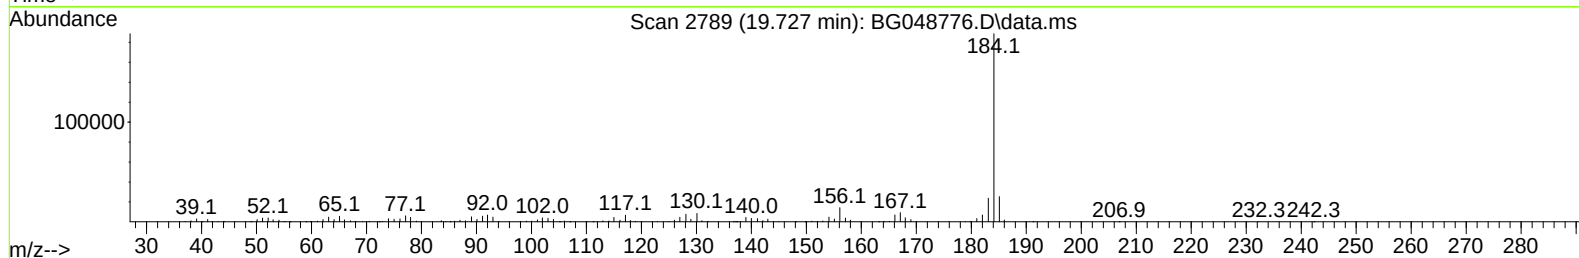


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048776.D
 Acq On : 19 Apr 2021 23:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 05:46:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 15:59:00 2021
 Response via : Initial Calibration

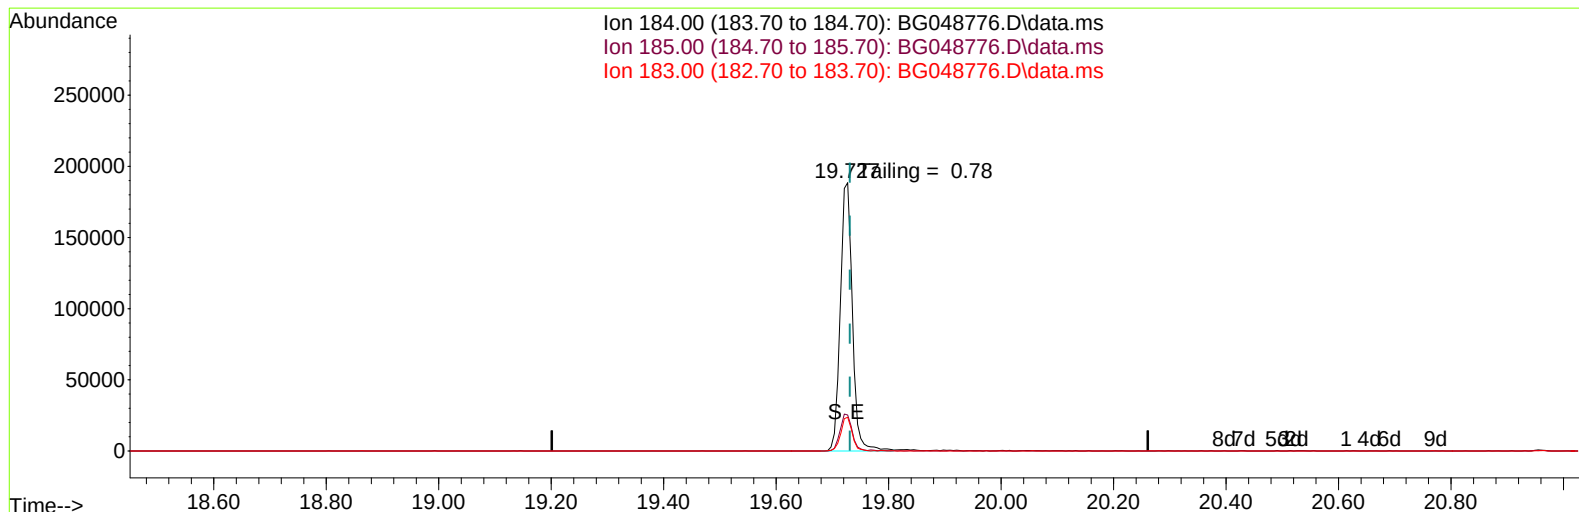

TIC: BG048776.D\data.ms

(77) Benzidine




19.727min (-0.004) 197808.81 ng m

response 284703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.45
183.00	11.70	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
Data File : BG048776.D
Acq On : 19 Apr 2021 23:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 05:46:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

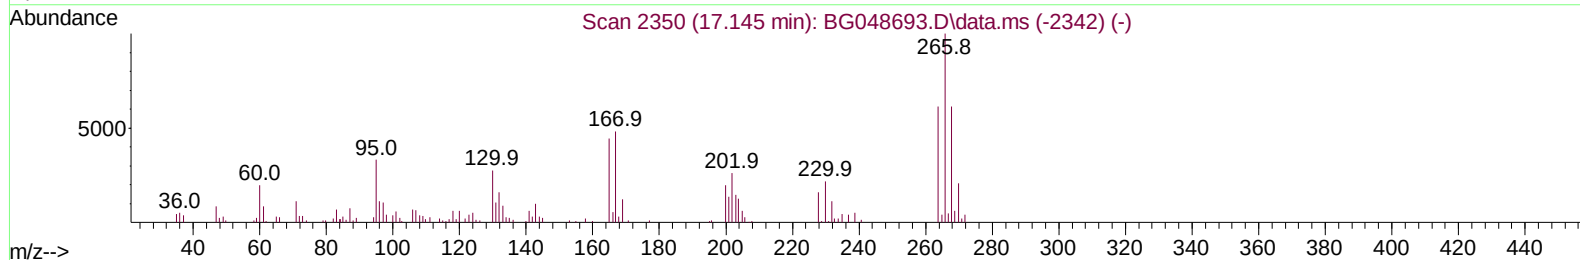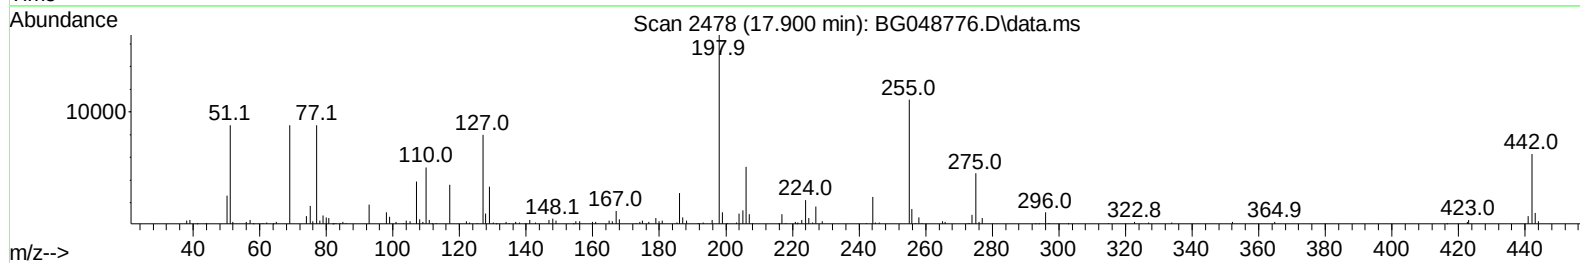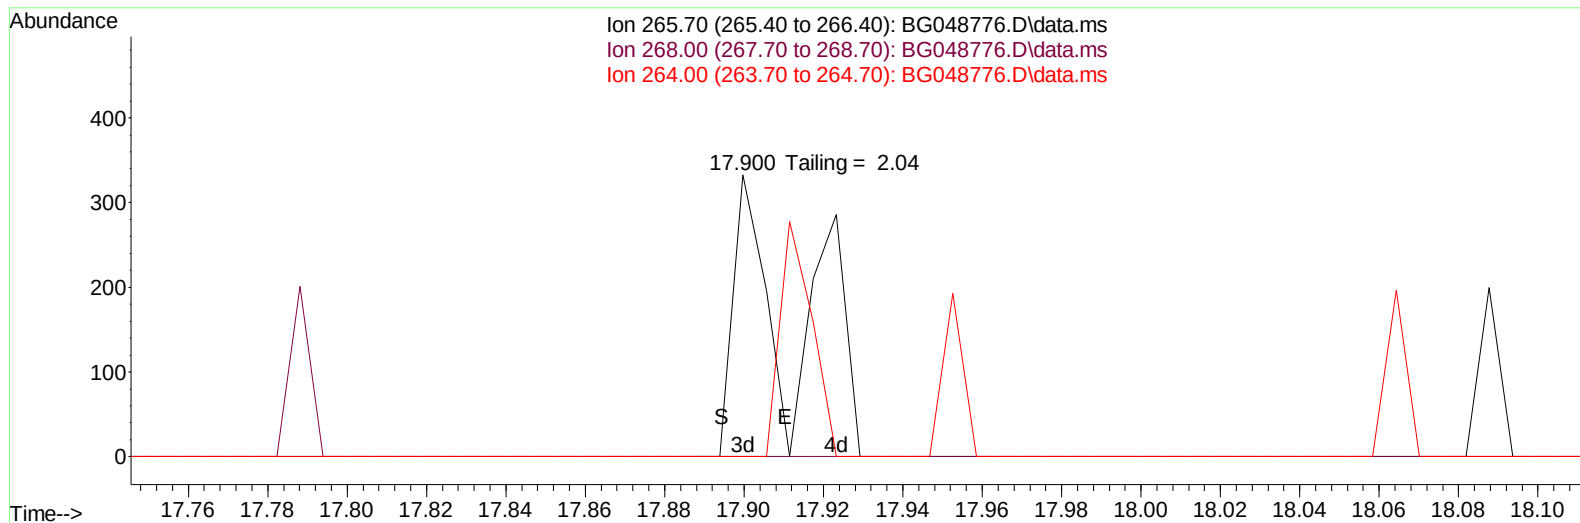

TIC: BG048776.D\data.ms

(70) Pentachlorophenol (C)

17.900min (+ 0.754) 61.23 ng m

response 186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	0.00#
264.00	61.30	0.00#
0.00	0.00	0.00