

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048781.D
 Acq On : 20 Apr 2021 3:02
 Operator : CG/JU
 Sample : M2079-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.554	370	377	382	rVB3	17336	30418	1.61%	0.233%
2	5.624	382	389	396	rBV	251222	399689	21.10%	3.060%
3	6.547	541	546	552	rBV4	16714	28072	1.48%	0.215%
4	7.040	625	630	638	rVB2	17458	28854	1.52%	0.221%
5	7.240	653	664	672	rBV	212910	394377	20.82%	3.020%
6	7.328	675	679	685	rVB4	11766	22017	1.16%	0.169%
7	7.458	694	701	707	rVB	14240	22965	1.21%	0.176%
8	8.074	801	806	812	rBV	76026	134723	7.11%	1.032%
9	8.456	863	871	876	rBV6	16188	40540	2.14%	0.310%
10	8.568	884	890	895	rVB2	71357	119103	6.29%	0.912%
11	8.721	910	916	920	rBV3	53721	85719	4.52%	0.656%
12	8.774	920	925	935	rVB5	24254	44414	2.34%	0.340%
13	9.038	965	970	973	rVB3	16233	26210	1.38%	0.201%
14	9.103	973	981	991	rBV9	47442	190618	10.06%	1.459%
15	9.191	991	996	1000	rVV3	87926	172661	9.11%	1.322%
16	9.255	1000	1007	1016	rVB2	374389	858094	45.29%	6.570%
17	9.438	1030	1038	1044	rVB10	17969	46448	2.45%	0.356%
18	9.537	1049	1055	1061	rVV4	11881	22628	1.19%	0.173%
19	9.714	1080	1085	1091	rVB	77969	121365	6.41%	0.929%
20	9.772	1091	1095	1101	rVB	69096	111334	5.88%	0.852%
21	9.896	1105	1116	1121	rBV6	20062	44240	2.33%	0.339%
22	9.972	1121	1129	1135	rBV5	17999	35216	1.86%	0.270%
23	10.084	1143	1148	1157	rBV10	21198	50452	2.66%	0.386%
24	10.172	1158	1163	1170	rVB6	45318	82466	4.35%	0.631%
25	10.301	1180	1185	1190	rVB9	13772	26606	1.40%	0.204%
26	10.360	1190	1195	1199	rBV3	19999	32706	1.73%	0.250%
27	10.442	1205	1209	1211	rBV2	16884	23648	1.25%	0.181%
28	10.671	1238	1248	1254	rBV2	71312	123847	6.54%	0.948%
29	10.760	1254	1263	1265	rBV9	13168	33461	1.77%	0.256%
30	10.901	1276	1287	1292	rBV2	104718	259034	13.67%	1.983%
31	10.953	1292	1296	1302	rVV4	79086	167766	8.85%	1.285%
32	11.000	1302	1304	1311	rVB4	15896	26739	1.41%	0.205%
33	11.112	1318	1323	1330	rBV2	23649	39088	2.06%	0.299%
34	11.529	1390	1394	1399	rVB7	20941	34029	1.80%	0.261%
35	11.688	1416	1421	1429	rBV10	18323	39013	2.06%	0.299%
36	11.811	1438	1442	1445	rBV5	18015	24139	1.27%	0.185%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048781.D
 Acq On : 20 Apr 2021 3:02
 Operator : CG/JU
 Sample : M2079-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.852	1445	1449	1455	rVB9	13099	27536	1.45%	0.211%
38	12.011	1467	1476	1485	rVB9	25233	75894	4.01%	0.581%
39	12.164	1498	1502	1507	rVB7	14304	28579	1.51%	0.219%
40	12.223	1508	1512	1516	rVB2	20376	31224	1.65%	0.239%
41	12.275	1517	1521	1529	rVB7	33310	72479	3.83%	0.555%
42	12.358	1531	1535	1539	rBV7	13973	27176	1.43%	0.208%
43	12.458	1545	1552	1556	rBV5	29102	64190	3.39%	0.491%
44	12.534	1561	1565	1569	rVV7	35464	67533	3.56%	0.517%
45	12.587	1570	1574	1583	rVB6	32781	67416	3.56%	0.516%
46	12.781	1598	1607	1611	rBV8	27331	76891	4.06%	0.589%
47	12.863	1617	1621	1624	rBV5	16017	30090	1.59%	0.230%
48	12.933	1627	1633	1645	rVB2	118026	228752	12.07%	1.751%
49	13.063	1650	1655	1661	rVB8	21421	50507	2.67%	0.387%
50	13.139	1664	1668	1672	rBV6	19095	32109	1.69%	0.246%
51	13.257	1685	1688	1696	rVB10	13174	26739	1.41%	0.205%
52	13.357	1696	1705	1710	rBV	915909	1394541	73.60%	10.677%
53	13.409	1710	1714	1718	rVB6	20852	31074	1.64%	0.238%
54	13.550	1734	1738	1740	rBV5	18299	23892	1.26%	0.183%
55	13.691	1758	1762	1768	rBV7	25675	46468	2.45%	0.356%
56	13.780	1770	1777	1785	rBV2	240048	515178	27.19%	3.944%
57	13.985	1810	1812	1818	rVB7	17752	27227	1.44%	0.208%
58	14.073	1821	1827	1835	rVV9	43561	115104	6.08%	0.881%
59	14.144	1835	1839	1842	rVB6	14168	20454	1.08%	0.157%
60	14.185	1842	1846	1848	rBV2	14321	21500	1.13%	0.165%
61	14.391	1877	1881	1888	rBV7	47893	107134	5.65%	0.820%
62	14.455	1890	1892	1897	rVV6	21797	35246	1.86%	0.270%
63	14.508	1897	1901	1903	rVV5	24179	33259	1.76%	0.255%
64	14.549	1904	1908	1912	rVB7	23877	38436	2.03%	0.294%
65	14.673	1926	1929	1932	rBV5	14300	22200	1.17%	0.170%
66	14.737	1932	1940	1945	rVV	182827	317050	16.73%	2.428%
67	14.861	1953	1961	1969	rBV4	73552	166440	8.78%	1.274%
68	15.049	1991	1993	1998	rVB6	14085	19733	1.04%	0.151%
69	15.143	2006	2009	2014	rBV7	25294	44041	2.32%	0.337%
70	15.260	2024	2029	2033	rBV7	32735	67343	3.55%	0.516%
71	15.348	2040	2044	2049	rVB7	36512	59246	3.13%	0.454%
72	15.554	2075	2079	2085	rVB5	41940	70291	3.71%	0.538%
73	15.624	2088	2091	2097	rVB5	28562	39656	2.09%	0.304%
74	15.912	2136	2140	2143	rBV5	34920	47592	2.51%	0.364%
75	15.995	2149	2154	2158	rBV8	24545	39208	2.07%	0.300%
76	16.130	2172	2177	2180	rBV6	24048	45734	2.41%	0.350%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048781.D
 Acq On : 20 Apr 2021 3:02
 Operator : CG/JU
 Sample : M2079-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	16.230	2188	2194	2202	rBV2	803199	1194917	63.07%	9.149%
78	16.365	2213	2217	2225	rVB10	15348	37135	1.96%	0.284%
79	16.494	2235	2239	2246	rVB3	34751	58390	3.08%	0.447%
80	16.553	2246	2249	2253	rBV6	30571	43801	2.31%	0.335%
81	16.782	2284	2288	2290	rBV5	13093	20190	1.07%	0.155%
82	17.193	2354	2358	2361	rBV6	16766	28991	1.53%	0.222%
83	17.228	2361	2364	2369	rVB7	15858	25903	1.37%	0.198%
84	17.493	2403	2409	2414	rVB	221009	334328	17.65%	2.560%
85	18.380	2555	2560	2574	rBV2	130856	273046	14.41%	2.091%
86	19.649	2772	2776	2785	rBV4	62396	134594	7.10%	1.031%
87	20.102	2847	2853	2860	rVB	1485593	1894667	100.00%	14.507%
88	21.406	3070	3075	3079	rBV4	60262	89060	4.70%	0.682%
89	21.788	3134	3140	3146	rVB	215938	344497	18.18%	2.638%
90	25.125	3696	3708	3720	rVB2	119196	383326	20.23%	2.935%




Sum of corrected areas: 13060706

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
Data File : BG048781.D
Acq On : 20 Apr 2021 3:02
Operator : CG/JU
Sample : M2079-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

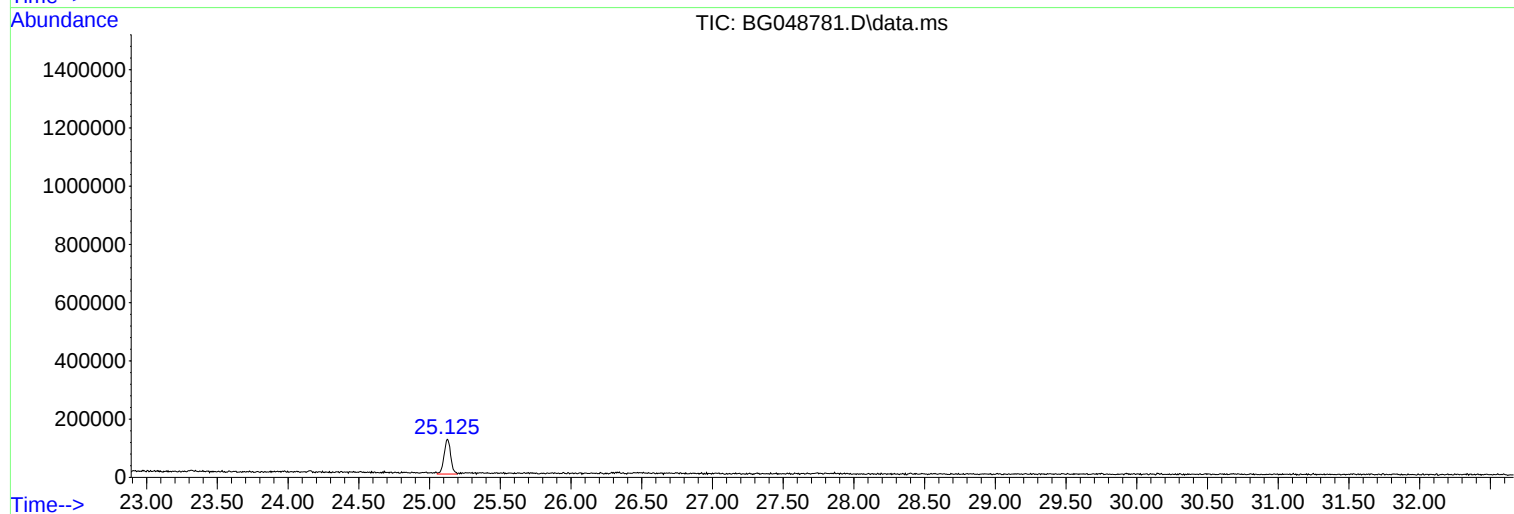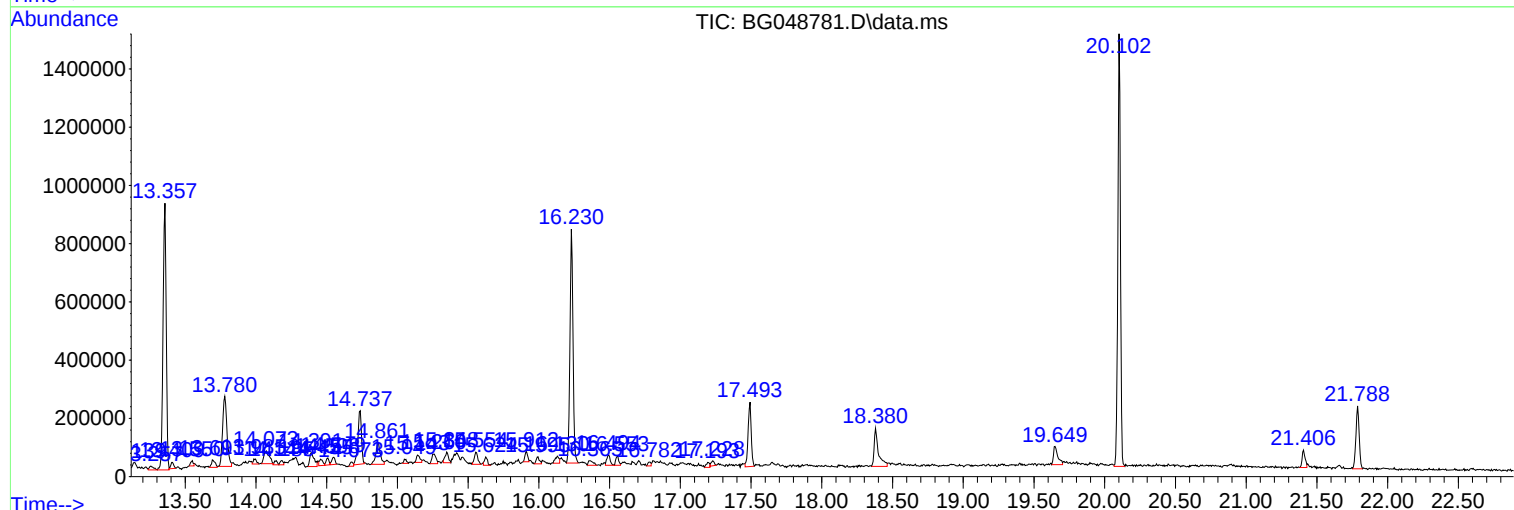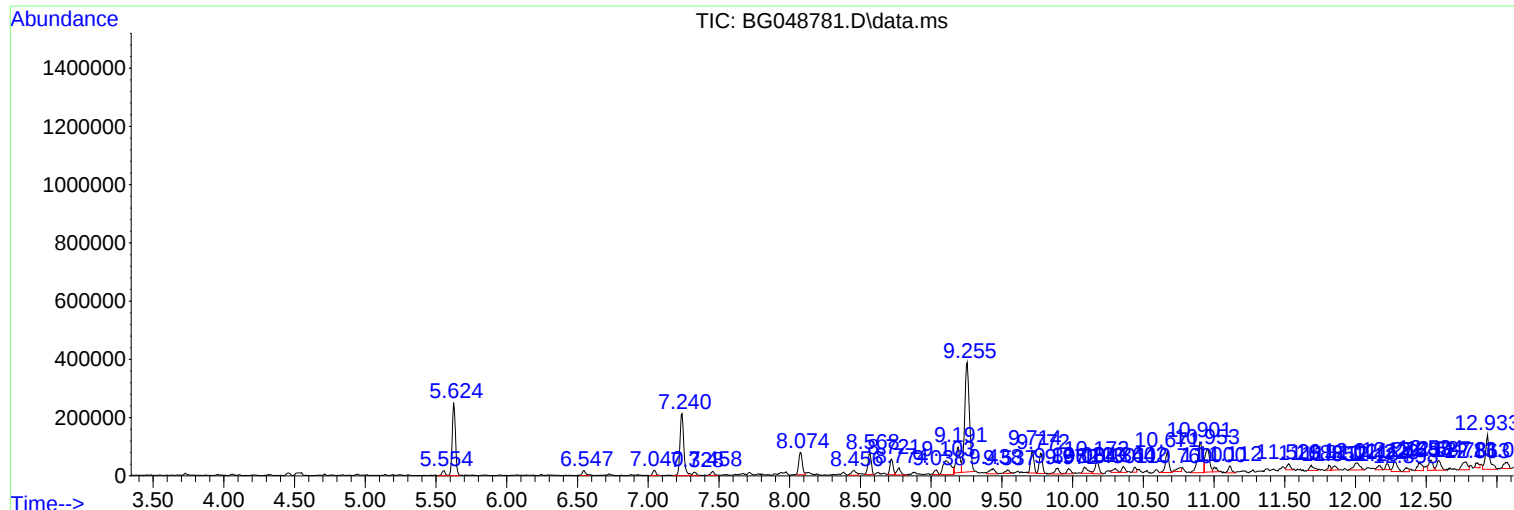

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
Data File : BG048781.D
Acq On : 20 Apr 2021 3:02
Operator : CG/JU
Sample : M2079-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
Data File : BG048781.D
Acq On : 20 Apr 2021 3:02
Operator : CG/JU
Sample : M2079-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
