
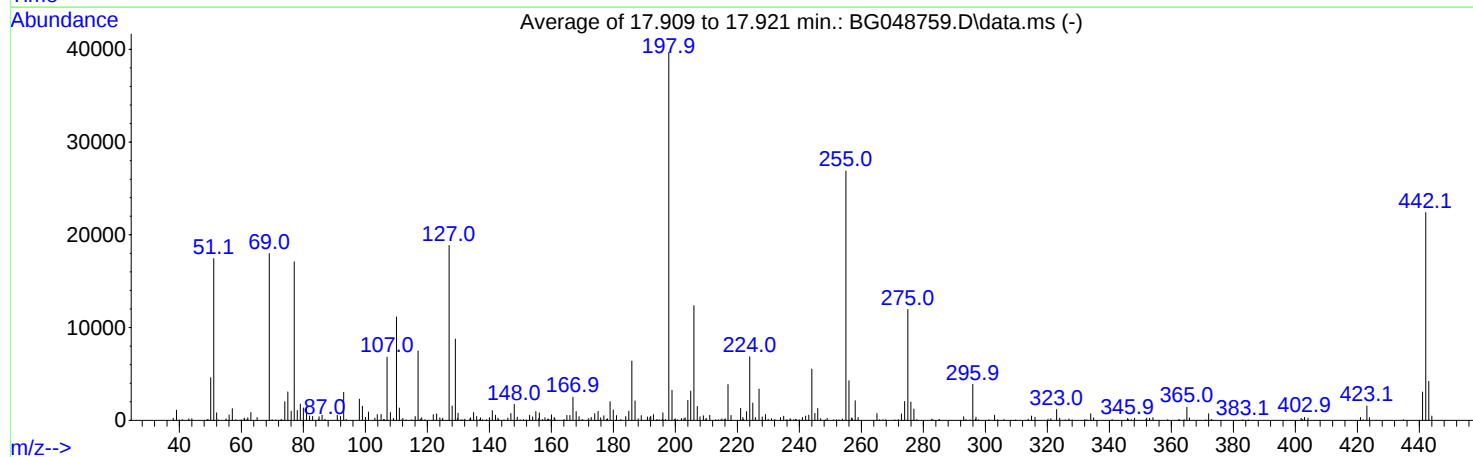


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048759.D
 Acq On : 19 Apr 2021 8:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 15:59:00 2021

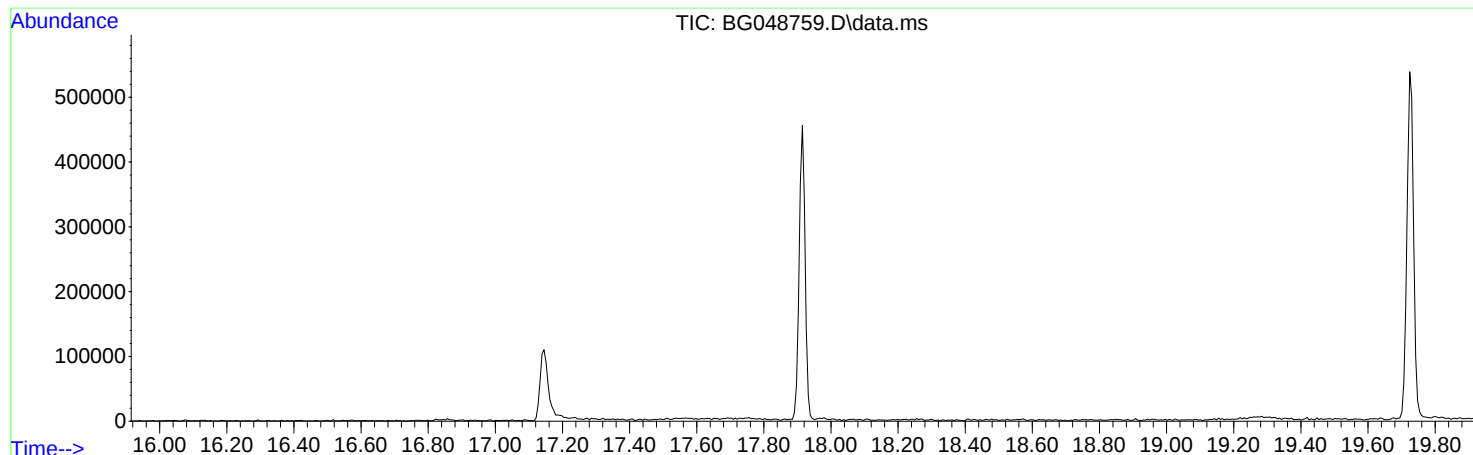




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	17440	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.4	17997	PASS
70	69	0.00	2	0.4	64	PASS
127	198	10	80	47.6	18860	PASS
197	198	0.00	2	0.3	112	PASS
198	198	100	100	100.0	39651	PASS
199	198	5	9	8.2	3249	PASS
275	198	10	60	30.1	11946	PASS
365	198	1	100	3.6	1419	PASS
441	198	0.01	100	7.7	3061	PASS
442	198	50	100	56.5	22411	PASS
443	442	15	24	18.8	4216	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048759.D
 Acq On : 19 Apr 2021 8:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 11:05:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 15:59:00 2021
 Response via : Initial Calibration

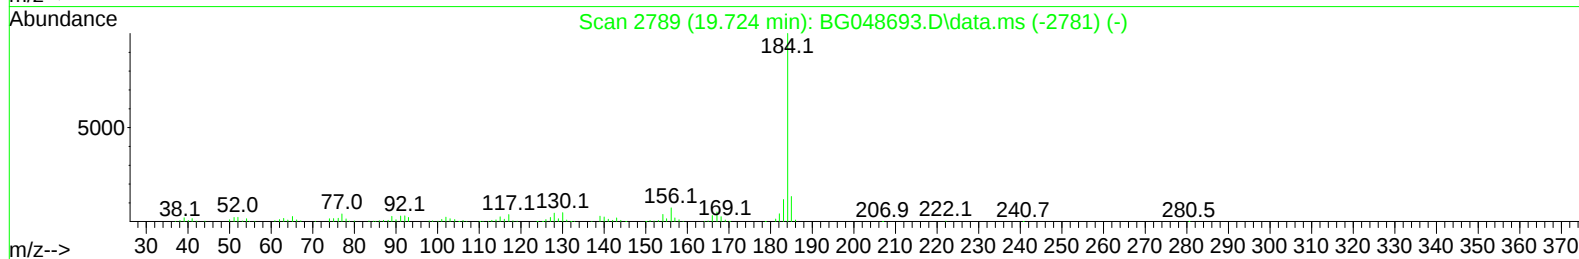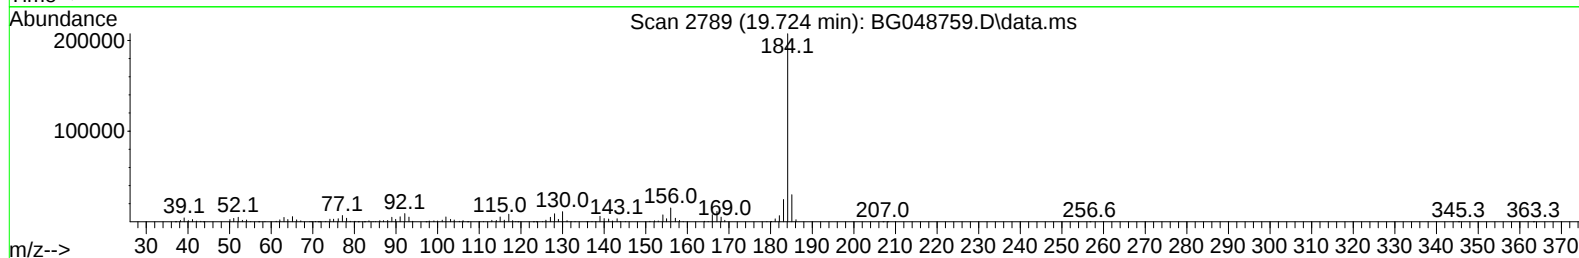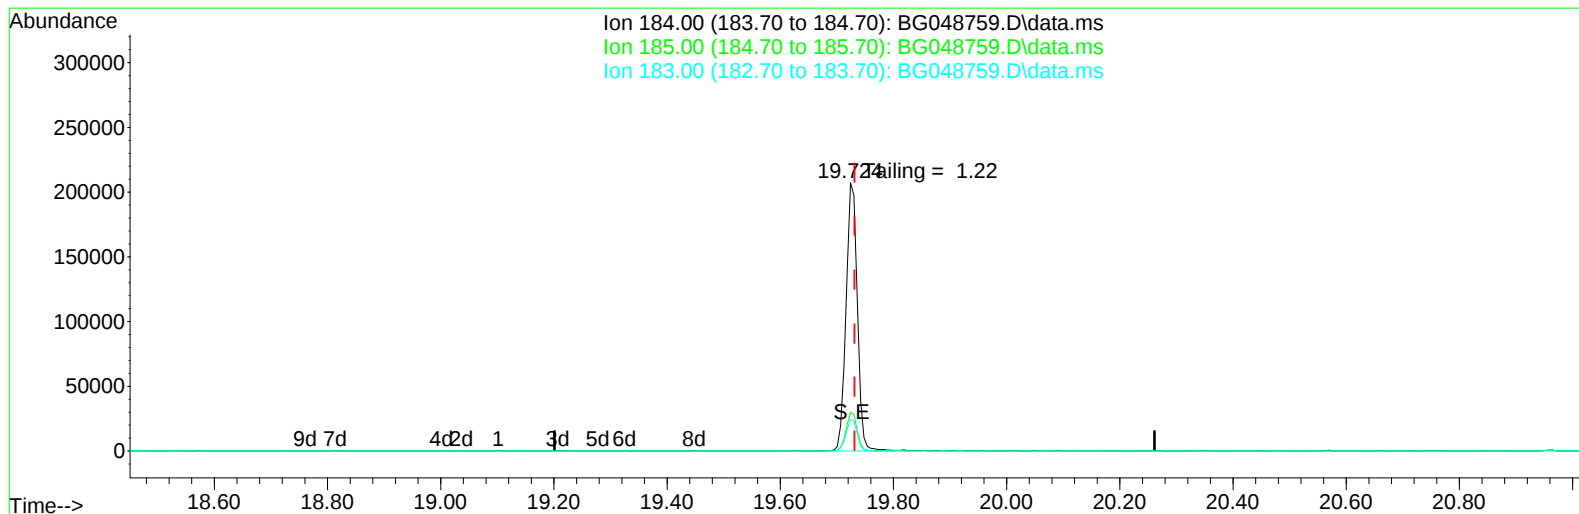

TIC: BG048759.D\data.ms

(77) Benzidine

19.724min (-0.007) 137855.67 ng m




response 288261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.46
183.00	11.70	11.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
Data File : BG048759.D
Acq On : 19 Apr 2021 8:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 11:05:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 15:59:00 2021
Response via : Initial Calibration

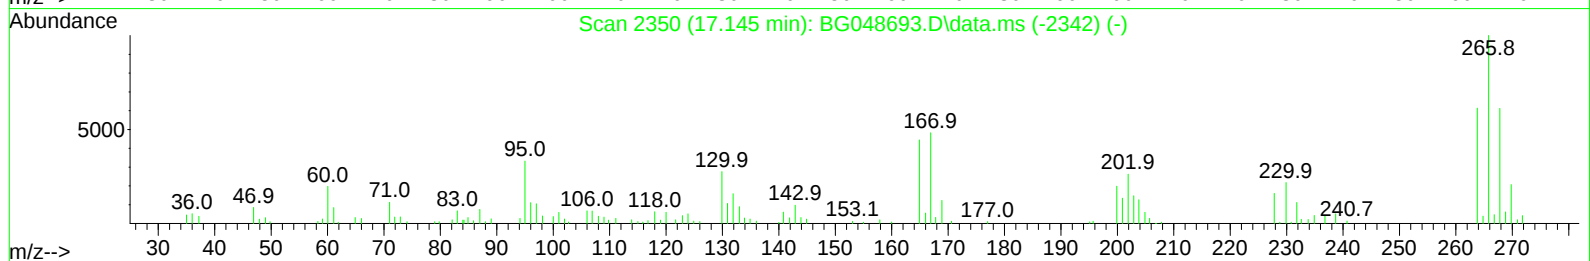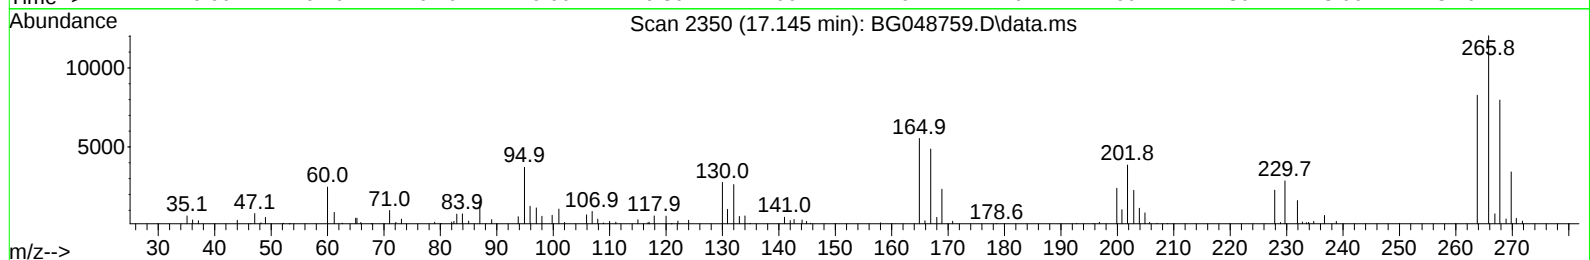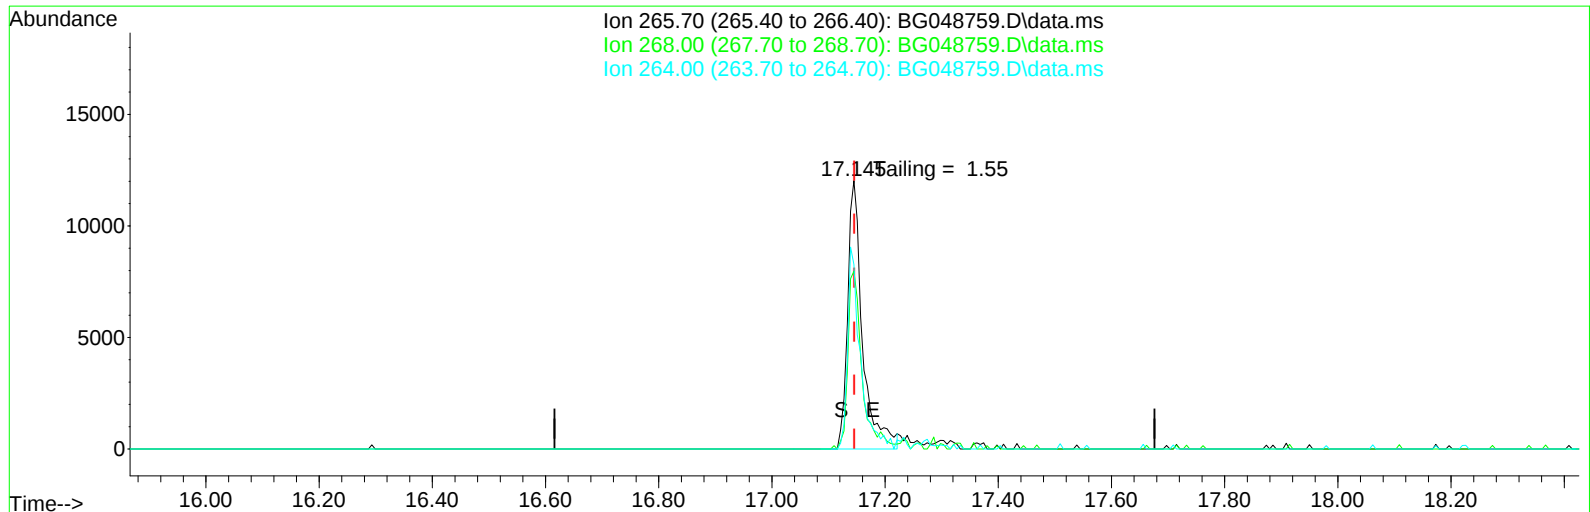

TIC: BG048759.D\data.ms

(70) Pentachlorophenol (C)

17.145min (-0.001) 66326.35 ng

response 23074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	66.25
264.00	61.30	68.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_G	BG048759.D
Compound Name	Response	Retention Time
DDT	138373	20.95
DDD	5568	20.51
DDE	805	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6373	144746	4.40