


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048776.D
 Acq On : 19 Apr 2021 23:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 15:59:00 2021

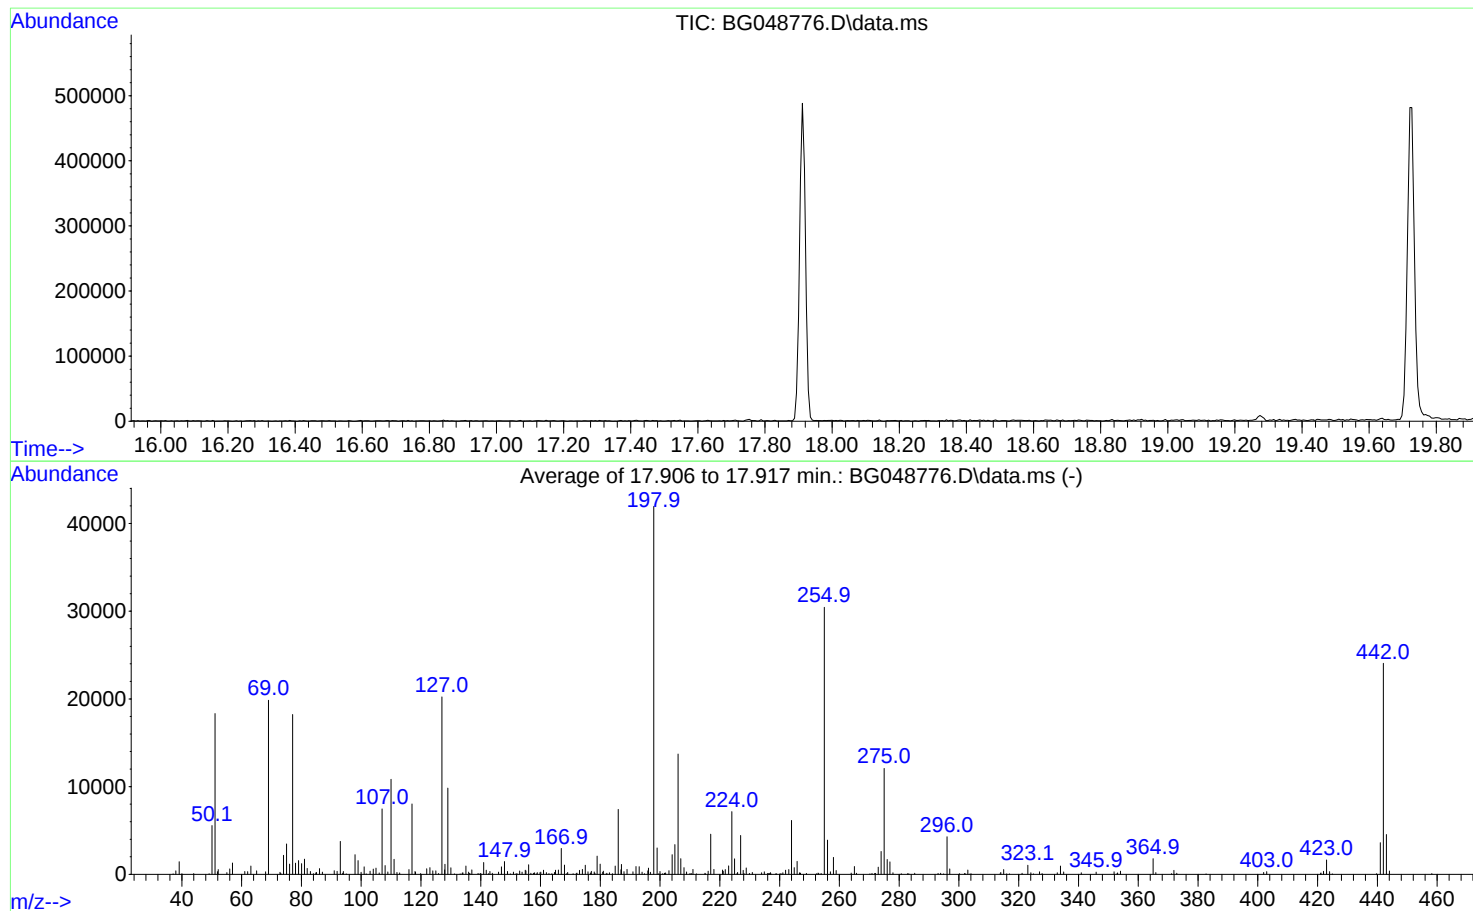




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	18335	PASS
68	69	0.00	2	1.5	288	PASS
69	198	0.00	100	47.3	19840	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	20227	PASS
197	198	0.00	2	0.6	247	PASS
198	198	100	100	100.0	41933	PASS
199	198	5	9	7.2	3018	PASS
275	198	10	60	28.8	12080	PASS
365	198	1	100	4.3	1793	PASS
441	198	0.01	100	8.6	3605	PASS
442	198	50	100	57.4	24056	PASS
443	442	15	24	18.9	4548	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048776.D
 Acq On : 19 Apr 2021 23:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 20 05:46:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 15:59:00 2021
 Response via : Initial Calibration

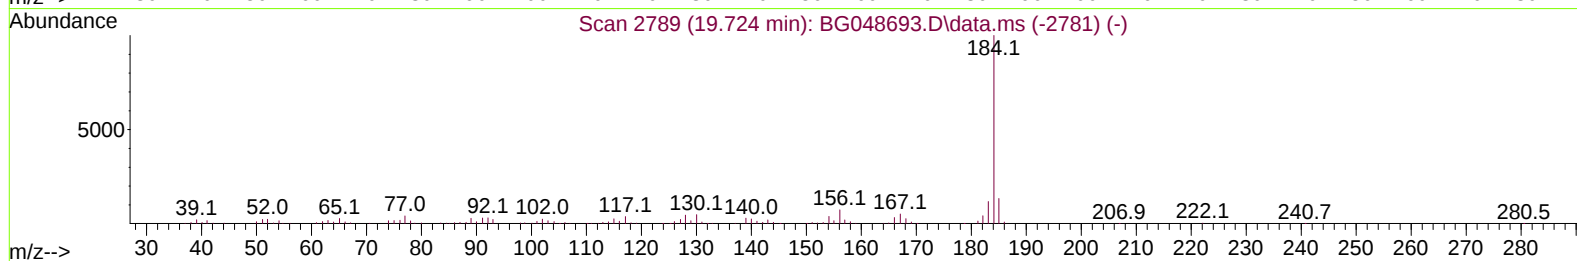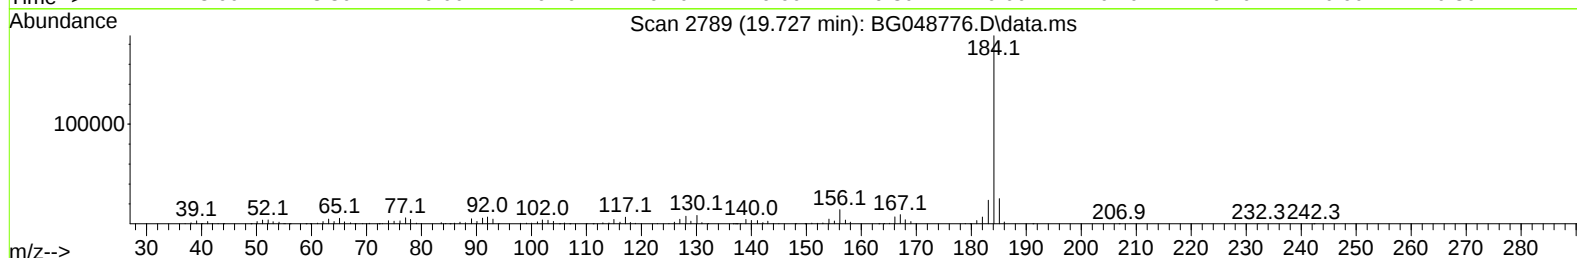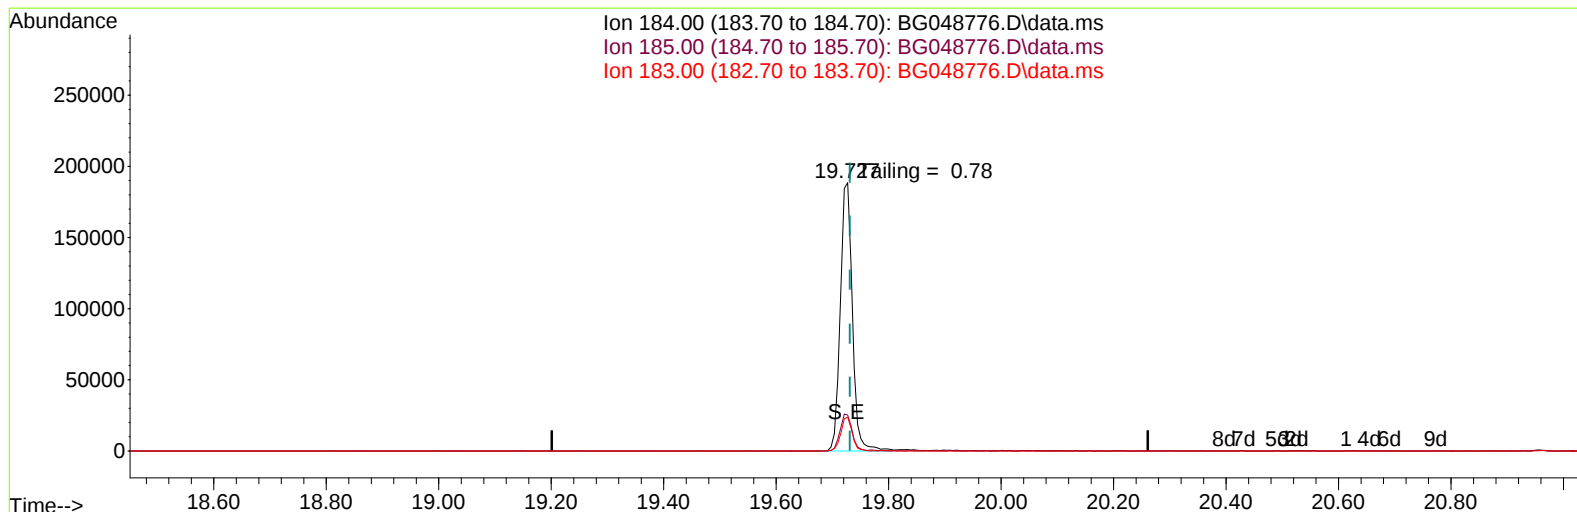

TIC: BG048776.D\data.ms

(77) Benzidine

19.727min (-0.004) 197808.81 ng m




response 284703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.45
183.00	11.70	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041921\
 Data File : BG048776.D
 Acq On : 19 Apr 2021 23:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 20 05:46:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 15:59:00 2021
 Response via : Initial Calibration

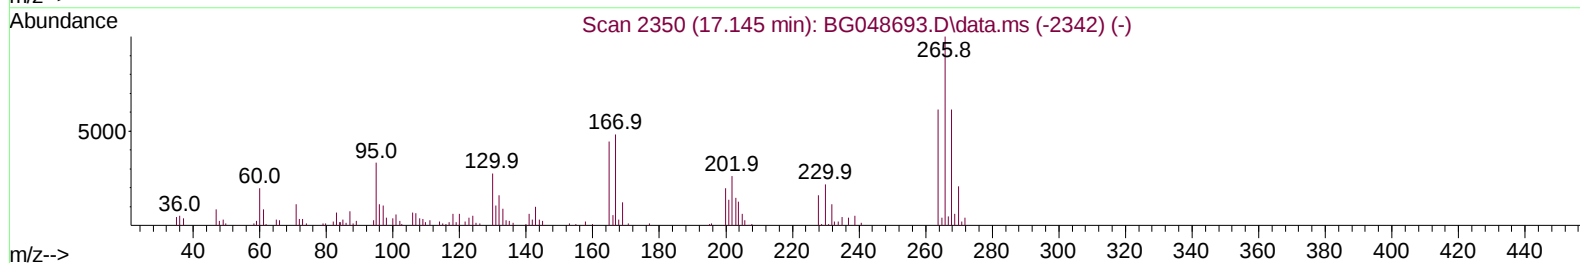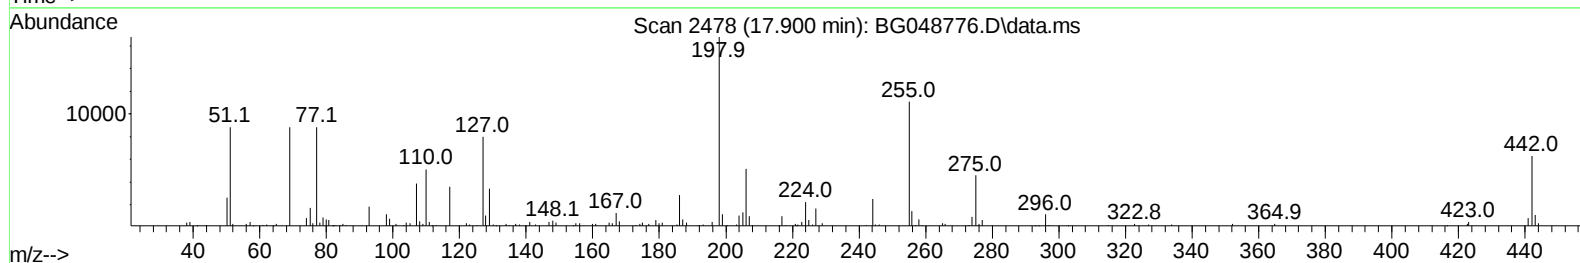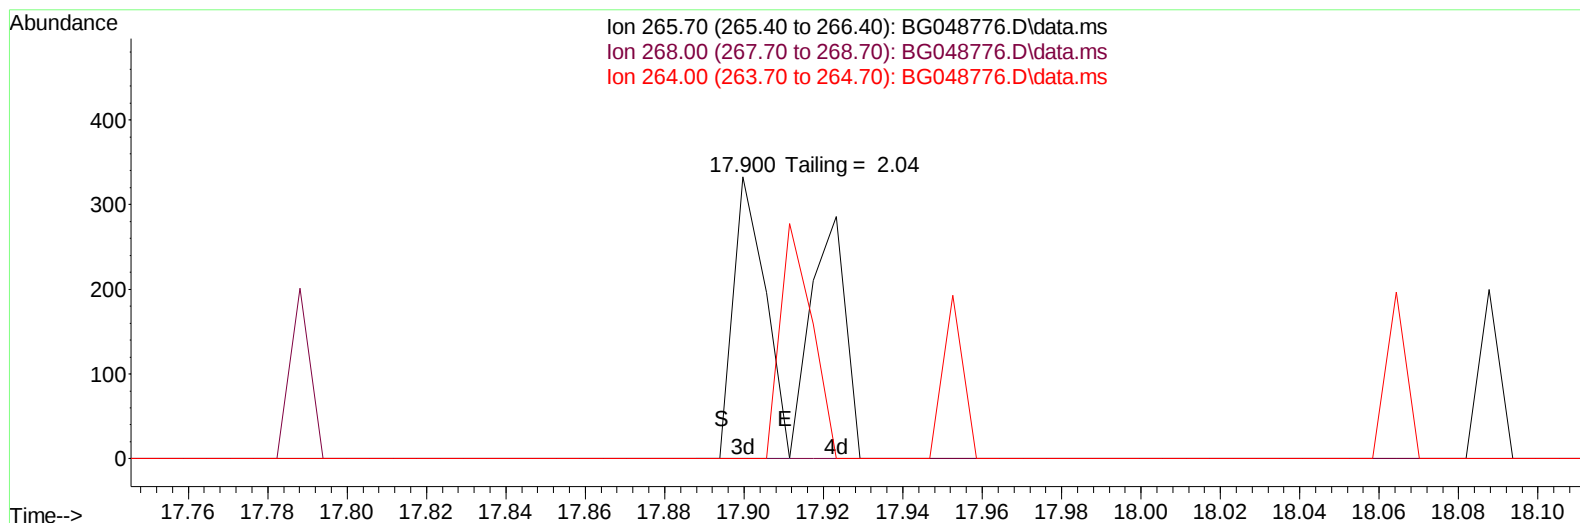

TIC: BG048776.D\data.ms

(70) Pentachlorophenol (C)

17.900min (+ 0.754) 61.23 ng m

response 186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	0.00#
264.00	61.30	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_G	BG048776.D
Compound Name	Response	Retention Time
DDT	140092	20.961
DDD	8752	20.514
DDE	685	20.009
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9437	149529	6.31