

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042015\
 Data File : BG016548.D
 Acq On : 20 Apr 2015 13:10
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Quant Time: Apr 21 01:44:47 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 14:00:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	62969	20.00	ng	-0.03
21) Naphthalene-d8	10.43	136	286305	20.00	ng	-0.03
38) Acenaphthene-d10	14.29	164	171430	20.00	ng	-0.02
63) Phenanthrene-d10	17.03	188	351315	20.00	ng	-0.03
75) Chrysene-d12	21.22	240	303377	20.00	ng	-0.02
86) Perylene-d12	23.44	264	288920	20.00	ng	-0.03

System Monitoring Compounds

5) 2-Fluorophenol	5.23	112	323242	81.01	ng	-0.03
7) Phenol-d6	6.83	99	456066	76.14	ng	-0.03
23) Nitrobenzene-d5	8.81	82	386073	78.12	ng	-0.03
41) 2,4,6-Tribromophenol	15.79	330	104522	90.15	ng	-0.02
44) 2-Fluorobiphenyl	12.91	172	847584	84.18	ng	-0.02
78) Terphenyl-d14	19.66	244	1049588	80.97	ng	-0.02

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.12	88	69054	38.07	ng	98
3) Pyridine	3.51	79	206486	38.09	ng	96
4) n-Nitrosodimethylamine	3.44	42	59737	37.07	ng	96
6) Aniline	6.97	93	316335	36.98	ng	98
8) 2-Chlorophenol	7.21	128	193409	40.37	ng	93
9) Benzaldehyde	6.79	77	89001	25.37	ng	92
10) Phenol	6.86	94	238098	37.15	ng	99
11) bis(2-Chloroethyl)ether	7.08	93	178359	34.90	ng	97
12) 1,3-Dichlorobenzene	7.53	146	198511	41.03	ng	97
13) 1,4-Dichlorobenzene	7.68	146	201651	40.17	ng	97
14) 1,2-Dichlorobenzene	8.00	146	191145	39.82	ng	98
15) Benzyl Alcohol	7.89	79	154492	37.00	ng	96
16) 2,2'-oxybis(1-Chloropropan	8.18	45	178733	31.06	ng	96
17) 2-Methylphenol	8.10	107	162253	37.76	ng	97
18) Hexachloroethane	8.71	117	71043	37.00	ng	97
19) n-Nitroso-di-n-propylamine	8.45	70	149026	34.73	ng	96
20) 3+4-Methylphenols	8.43	107	230115	38.66	ng	97
22) Acetophenone	8.47	105	265038	39.92	ng	# 96
24) Nitrobenzene	8.85	77	199689	37.78	ng	90
25) Isophorone	9.36	82	423798	38.61	ng	95
26) 2-Nitrophenol	9.55	139	118791	48.20	ng	96
27) 2,4-Dimethylphenol	9.62	122	196820	42.87	ng	99
28) bis(2-Chloroethoxy)methane	9.85	93	239128	38.17	ng	99
29) 2,4-Dichlorophenol	10.09	162	172904	47.60	ng	95
30) 1,2,4-Trichlorobenzene	10.30	180	168453	44.42	ng	99
31) Naphthalene	10.48	128	604210	40.50	ng	99
32) Benzoic acid	9.77	122	102302	36.68	ng	98
33) 4-Chloroaniline	10.60	127	302752	43.25	ng	96
34) Hexachlorobutadiene	10.76	225	74950	44.99	ng	99
35) Caprolactam	11.38	113	105774	46.25	ng	92
36) 4-Chloro-3-methylphenol	11.74	107	202433	42.19	ng	92
37) 2-Methylnaphthalene	12.10	142	445051	41.47	ng	99
39) 1,2,4,5-Tetrachlorobenzene	12.48	216	164276	43.52	ng	98
40) Hexachlorocyclopentadiene	12.46	237	56944	32.96	ng	96

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042015\
 Data File : BG016548.D
 Acq On : 20 Apr 2015 13:10
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Quant Time: Apr 21 01:44:47 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 14:00:56 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) 2,4,6-Trichlorophenol	12.73	196	132262	47.16	ng	98
43) 2,4,5-Trichlorophenol	12.80	196	139039	46.40	ng	97
45) 1,1'-Biphenyl	13.13	154	538582	40.95	ng	97
46) 2-Chloronaphthalene	13.17	162	416490	41.58	ng	99
47) 2-Nitroaniline	13.38	65	126277	39.11	ng	87
48) Acenaphthylene	14.01	152	731508	41.07	ng	99
49) Dimethylphthalate	13.76	163	528193	42.04	ng	99
50) 2,6-Dinitrotoluene	13.88	165	129627	42.66	ng	90
51) Acenaphthene	14.36	154	436098	40.97	ng	97
52) 3-Nitroaniline	14.21	138	163476	42.13	ng	90
53) 2,4-Dinitrophenol	14.42	184	46967	32.21	ng	# 91
54) Dibenzofuran	14.69	168	606376	41.05	ng	98
55) 4-Nitrophenol	14.54	139	122244	38.12	ng	92
56) 2,4-Dinitrotoluene	14.67	165	183349	44.30	ng	89
57) Fluorene	15.34	166	539847	41.43	ng	99
58) 2,3,4,6-Tetrachlorophenol	14.93	232	103956	44.95	ng	93
59) Diethylphthalate	15.12	149	562522	42.06	ng	99
60) 4-Chlorophenyl-phenylether	15.34	204	221843	41.62	ng	94
61) 4-Nitroaniline	15.38	138	183823	41.73	ng	95
62) Azobenzene	15.63	77	498401	35.01	ng	98
64) 4,6-Dinitro-2-methylphenol	15.43	198	91305	37.82	ng	90
65) n-Nitrosodiphenylamine	15.56	169	500233	42.12	ng	99
66) 4-Bromophenyl-phenylether	16.23	248	119438	42.58	ng	91
67) Hexachlorobenzene	16.35	284	120882	41.46	ng	99
68) Atrazine	16.51	200	142343	43.00	ng	99
69) Pentachlorophenol	16.70	266	60892	34.21	ng	98
70) Phenanthrene	17.08	178	801986	40.59	ng	99
71) Anthracene	17.17	178	814532	41.60	ng	100
72) Carbazole	17.44	167	811467	41.29	ng	99
73) Di-n-butylphthalate	18.00	149	1005512	41.81	ng	100
74) Fluoranthene	19.09	202	846351	41.55	ng	96
76) Benzidine	19.28	184	413821	32.17	ng	98
77) Pyrene	19.46	202	869399	41.15	ng	100
79) Butylbenzylphthalate	20.36	149	463480	44.66	ng	92
80) Benzo(a)anthracene	21.20	228	747578	41.69	ng	99
81) 3,3'-Dichlorobenzidine	21.14	252	256125	43.44	ng	98
82) Chrysene	21.25	228	716860	41.41	ng	99
83) Bis(2-ethylhexyl)phthalate	21.13	149	630691	44.89	ng	97
84) Di-n-octyl phthalate	22.00	149	1060773	46.34	ng	97
85) Indeno(1,2,3-cd)pyrene	25.70	276	806586	44.85	ng	96
87) Benzo(b)fluoranthene	22.77	252	709560	41.93	ng	98
88) Benzo(k)fluoranthene	22.81	252	684513	41.34	ng	98
89) Benzo(a)pyrene	23.34	252	673592	42.47	ng	97
90) Dibenzo(a,h)anthracene	25.71	278	663063	42.97	ng	96
91) Benzo(g,h,i)perylene	26.39	276	666925	43.27	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042015\
 Data File : BG016548.D
 Acq On : 20 Apr 2015 13:10
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 Client Sample ID :
 SSTDCCC040

Quant Time: Apr 21 01:44:47 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 14:00:56 2015
 Response via : Initial Calibration

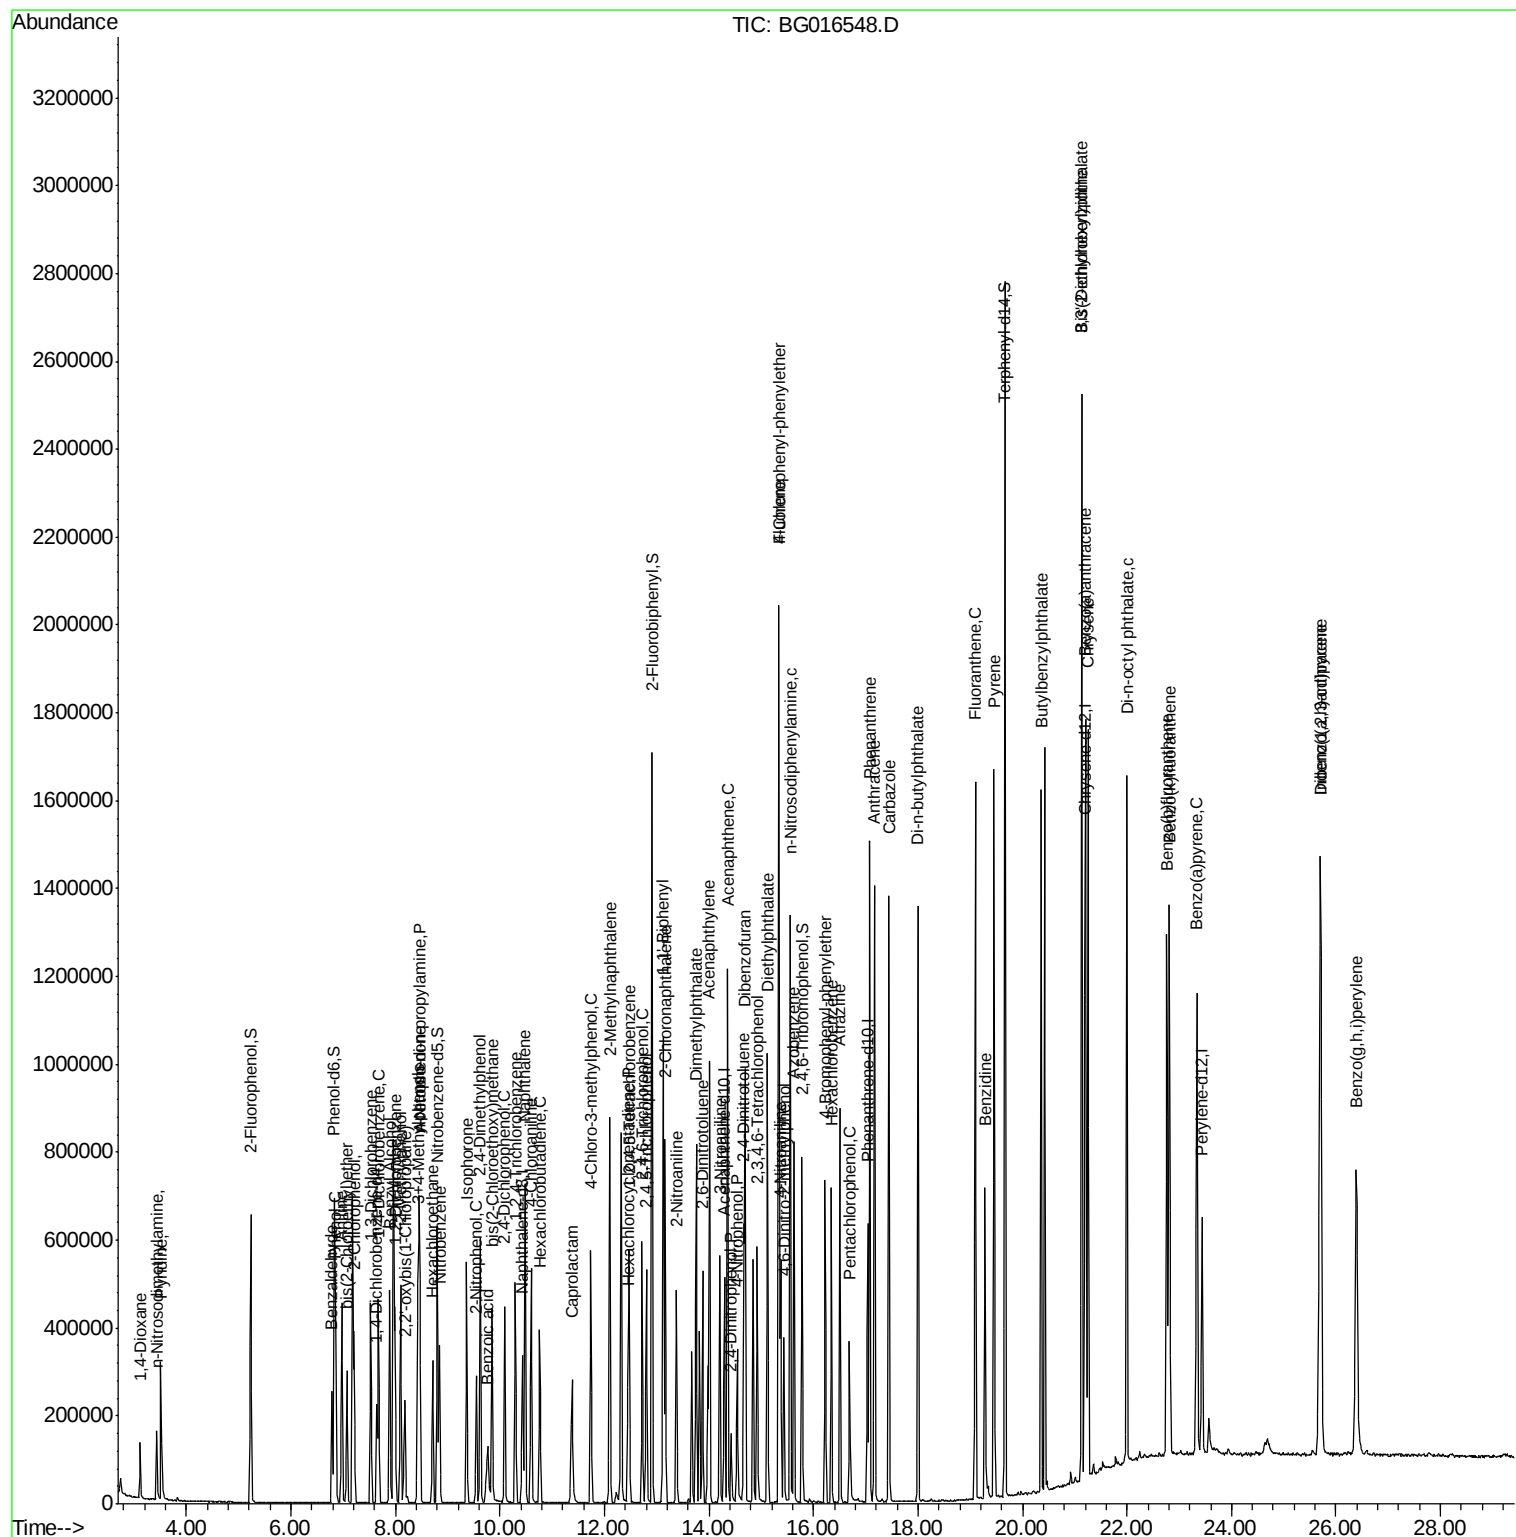

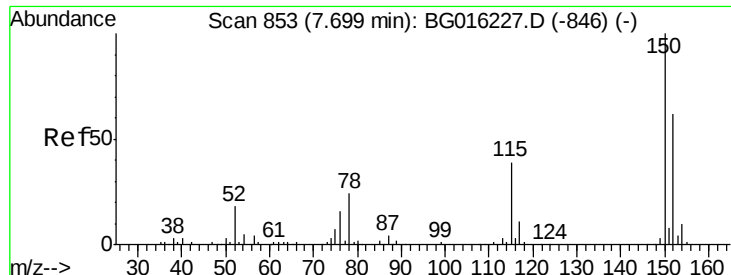


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.64 min Scan# 843
Delta R.T. -0.03 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion:152 Resp: 62969
Ion Ratio Lower Upper
152 100
150 156.7 130.1 195.1
115 55.1 50.5 75.7

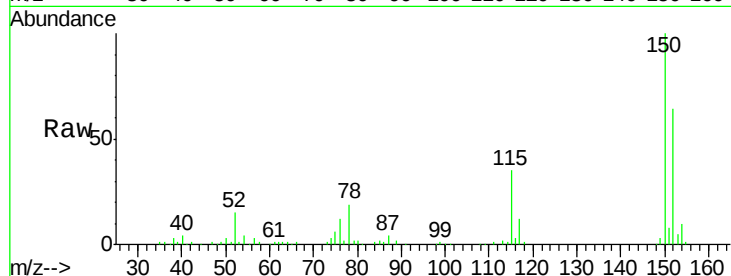


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

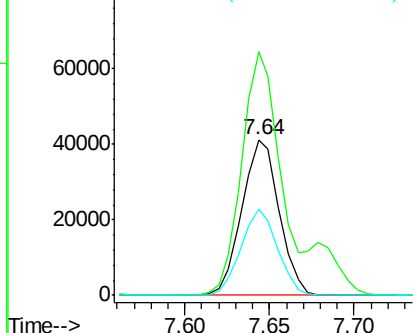



#2


1,4-Dioxane
Concen: 38.07 ng
RT: 3.12 min Scan# 73
Delta R.T. -0.04 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Tgt Ion: 88 Resp: 69054
Ion Ratio Lower Upper
88 100
58 61.3 50.6 76.0
43 21.4 17.0 25.4

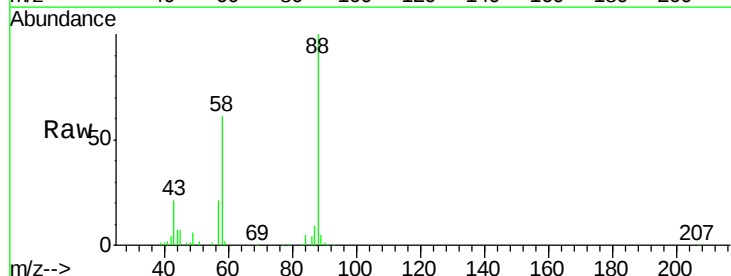

Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 58.00 (57.70 to 58.70): BGC
Ion 43.00 (42.70 to 43.70): BGC

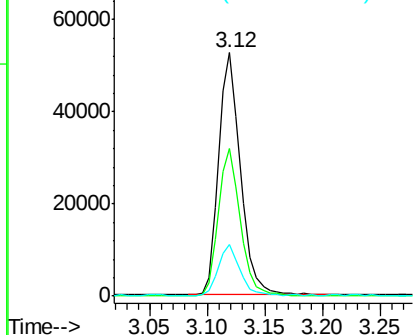

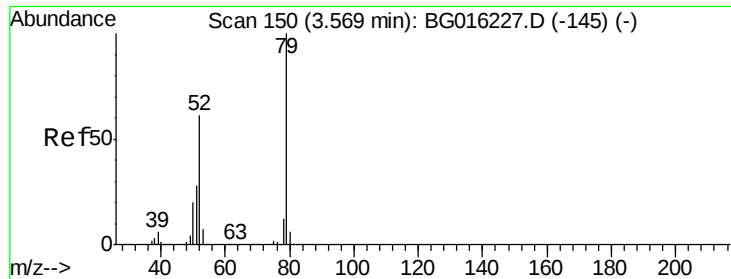

#3

Pyridine

Concen: 38.09 ng

RT: 3.51 min Scan# 140

Delta R.T. -0.04 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 79 Resp: 206486

Ion Ratio Lower Upper




79 100

52 57.7 49.0 73.4

51 27.1 22.5 33.7

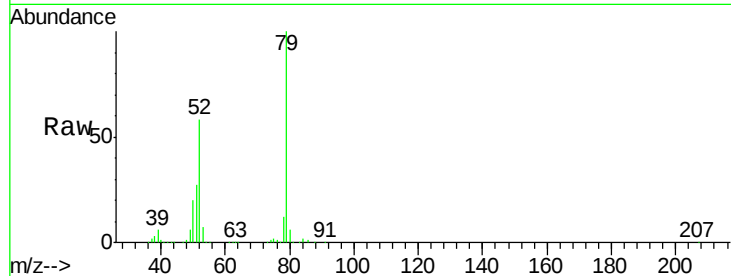

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 52.00 (51.70 to 52.70): BGC
Ion 51.00 (50.70 to 51.70): BGC

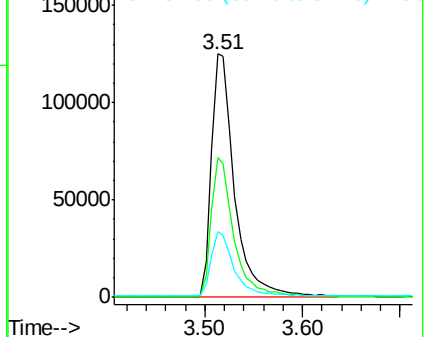

#4

n-Nitrosodimethylamine

Concen: 37.07 ng

RT: 3.44 min Scan# 127

Delta R.T. -0.04 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10


Tgt Ion: 42 Resp: 59737

Ion Ratio Lower Upper



42 100

74 197.9 153.7 230.5

44 6.4 5.3 7.9



Abundance Ion 42.00 (41.70 to 42.70): BGC
Ion 74.00 (73.70 to 74.70): BGC
Ion 44.00 (43.70 to 44.70): BGC

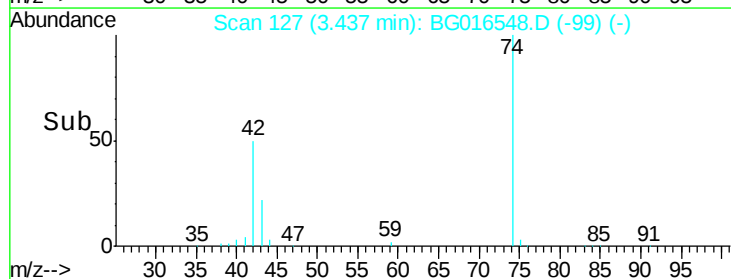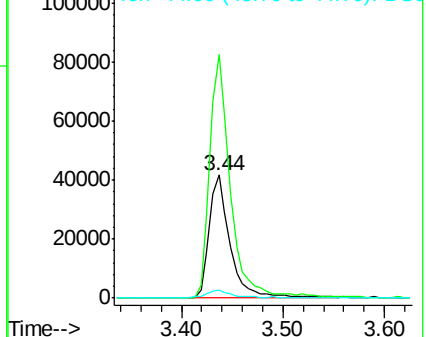



#5

2-Fluorophenol

Concen: 81.01 ng

RT: 5.23 min Scan# 433

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10





Instrument :

BNA_G

ClientSampleId :

SSTDCCC040

Tgt Ion:	112	Resp:	323242
Ion	Ratio	Lower	Upper
112	100		
64	48.6	44.5	66.7
63	23.7	21.4	32.0

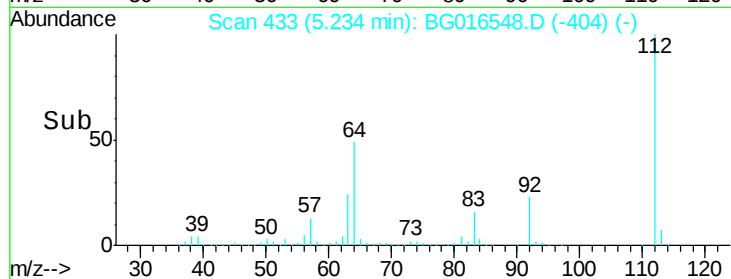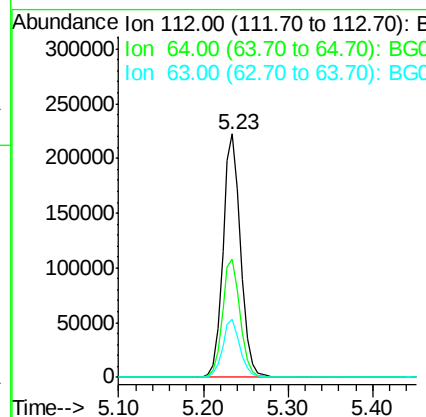

#6

Aniline

Concen: 36.98 ng




RT: 6.97 min Scan# 729


Delta R.T. -0.04 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10

Tgt Ion:	93	Resp:	316335
Ion	Ratio	Lower	Upper
93	100		
66	33.0	27.5	41.3
65	17.9	15.1	22.7

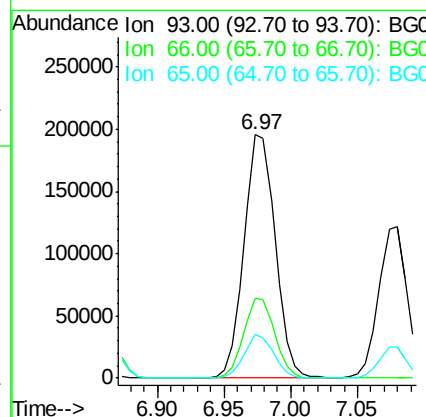

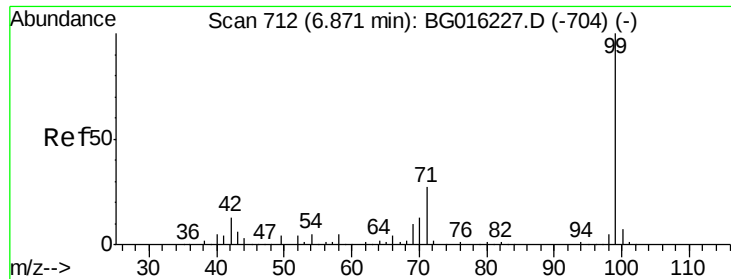

#7

Phenol-d6

Concen: 76.14 ng

RT: 6.83 min Scan# 705

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 99 Resp: 456066

Ion Ratio Lower Upper




99 100

42 11.5 10.0 15.0

71 25.9 21.5 32.3



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

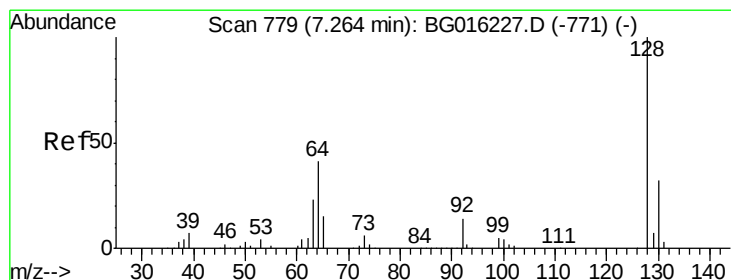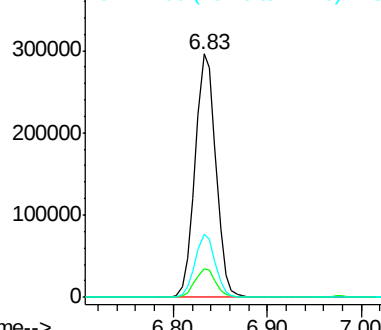

#8

2-Chlorophenol

Concen: 40.37 ng

RT: 7.21 min Scan# 770

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10


Tgt Ion: 128 Resp: 193409

Ion Ratio Lower Upper



128 100


130 32.9 11.6 51.6

64 37.4 24.2 64.2

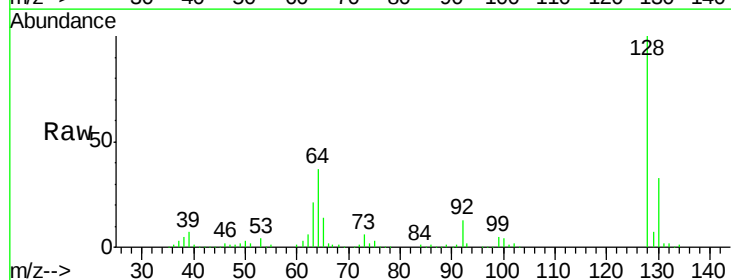

Abundance Ion 128.00 (127.70 to 128.70): BGC
Ion 130.00 (129.70 to 130.70): BGC
Ion 64.00 (63.70 to 64.70): BGC

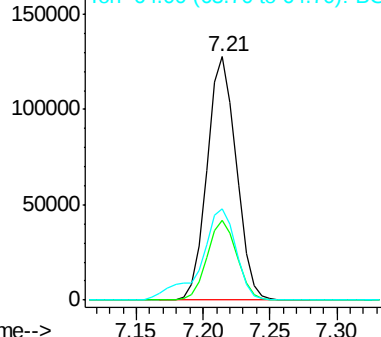

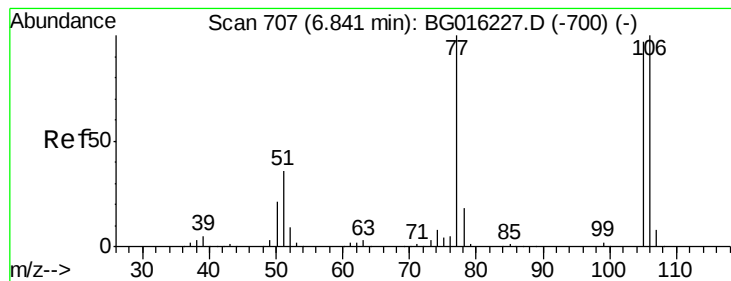

#9

Benzaldehyde

Concen: 25.37 ng

RT: 6.79 min Scan# 698

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040





Tgt Ion: 77 Resp: 89001

Ion Ratio Lower Upper

77 100

105 104.1 76.8 116.8

106 108.9 80.1 120.1

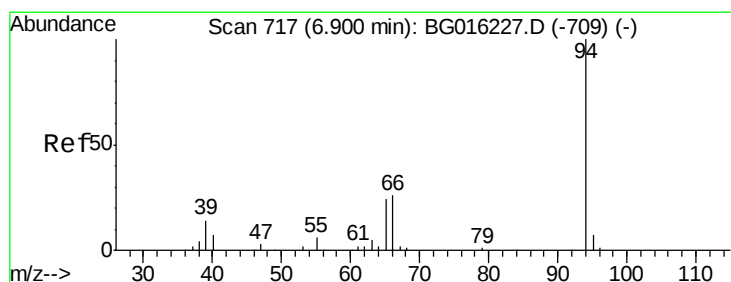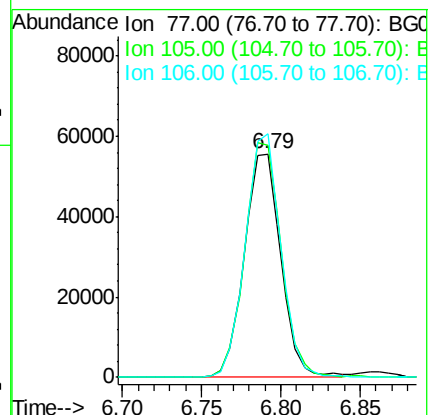

#10

Phenol

Concen: 37.15 ng

RT: 6.86 min Scan# 710

Delta R.T. -0.02 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10




Tgt Ion: 94 Resp: 238098


Ion Ratio Lower Upper

94 100

65 23.3 3.8 43.8

66 27.9 7.4 47.4

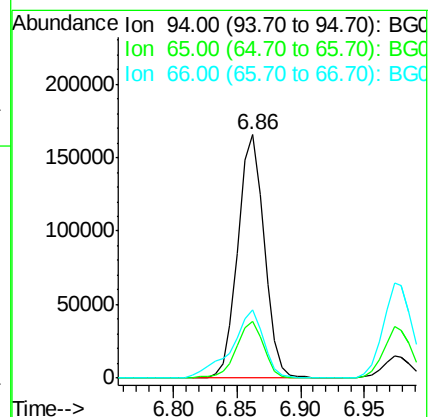


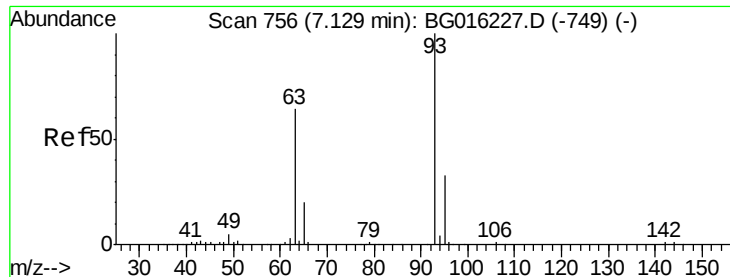




#11
 bis(2-Chloroethyl)ether
 Concen: 34.90 ng
 RT: 7.08 min Scan# 747
 Delta R.T. -0.03 min
 Lab File: BG016548.D
 Acq: 20 Apr 2015 13:10

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Tgt Ion:	93	Resp:	178359
Ion	Ratio	Lower	Upper
93	100		
63	61.5	44.1	84.1
95	33.5	12.5	52.5

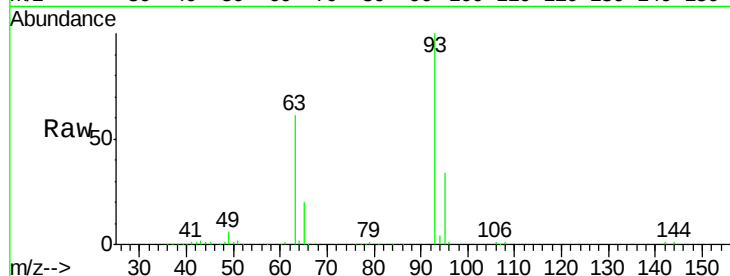


Abundance Ion 93.00 (92.70 to 93.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 95.00 (94.70 to 95.70): BGC

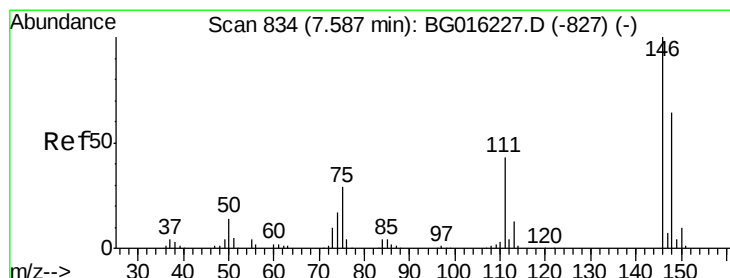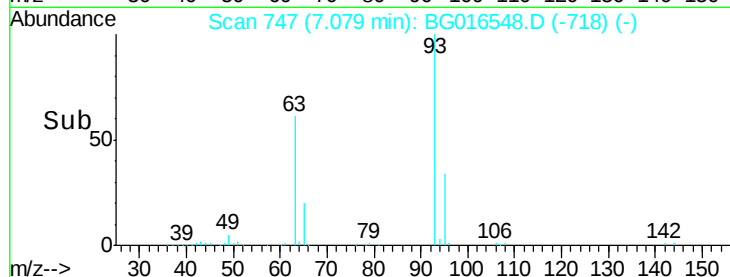
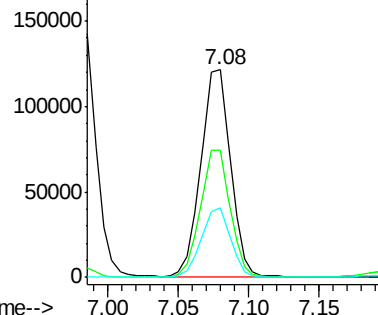



#12
 1,3-Dichlorobenzene
 Concen: 41.03 ng
 RT: 7.53 min Scan# 824
 Delta R.T. -0.03 min
 Lab File: BG016548.D
 Acq: 20 Apr 2015 13:10

Tgt Ion:	146	Resp:	198511
Ion	Ratio	Lower	Upper
146	100		
148	63.1	50.9	76.3
75	23.9	23.3	34.9

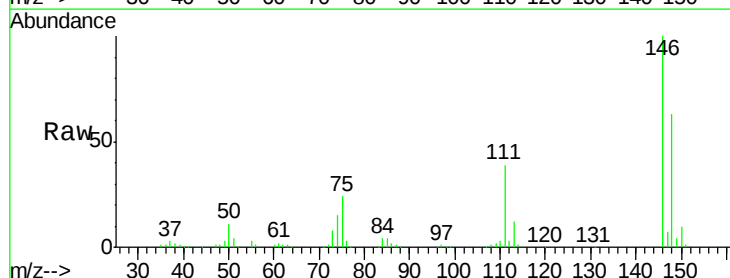

Abundance Ion 146.00 (145.70 to 146.70): BGC
 Ion 148.00 (147.70 to 148.70): BGC
 Ion 75.00 (74.70 to 75.70): BGC

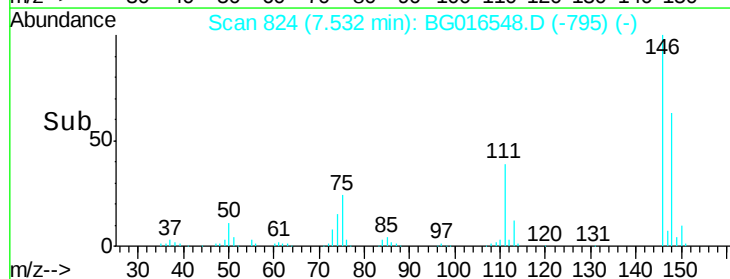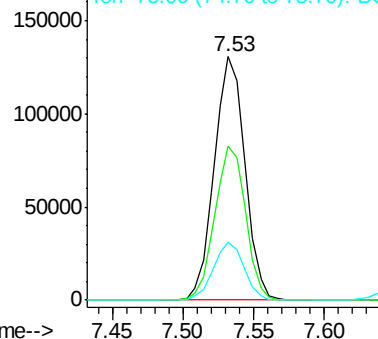


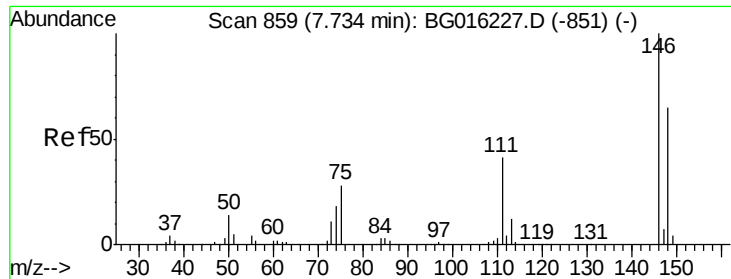




#13
 1,4-Dichlorobenzene
 Concen: 40.17 ng
 RT: 7.68 min Scan# 849
 Delta R.T. -0.04 min
 Lab File: BG016548.D
 Acq: 20 Apr 2015 13:10

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Tgt Ion:146 Resp: 201651
 Ion Ratio Lower Upper
 146 100
 148 64.2 52.0 78.0
 111 37.4 32.6 49.0




Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E


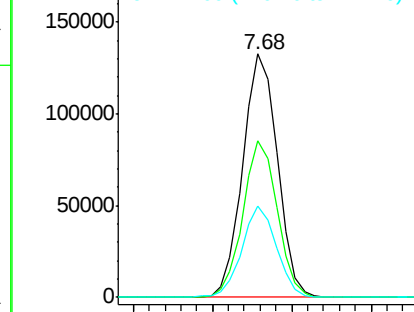



#14
 1,2-Dichlorobenzene
 Concen: 39.82 ng
 RT: 8.00 min Scan# 903
 Delta R.T. -0.03 min
 Lab File: BG016548.D
 Acq: 20 Apr 2015 13:10

Tgt Ion:146 Resp: 191145
 Ion Ratio Lower Upper
 146 100
 148 62.8 50.9 76.3
 111 41.2 34.7 52.1



Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E

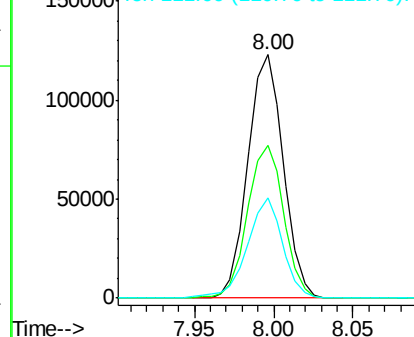

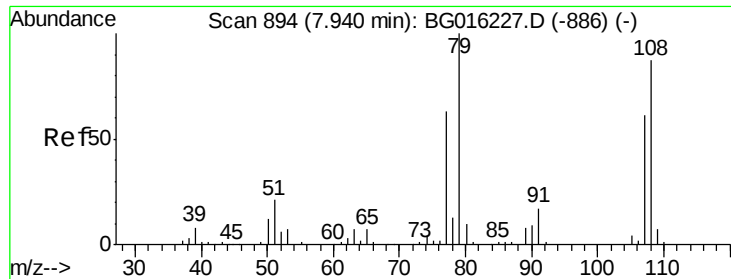

#15

Benzyl Alcohol

Concen: 37.00 ng

RT: 7.89 min Scan# 885

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 79 Resp: 154492

Ion Ratio Lower Upper




79 100

108 90.0 69.3 103.9

77 60.2 50.3 75.5

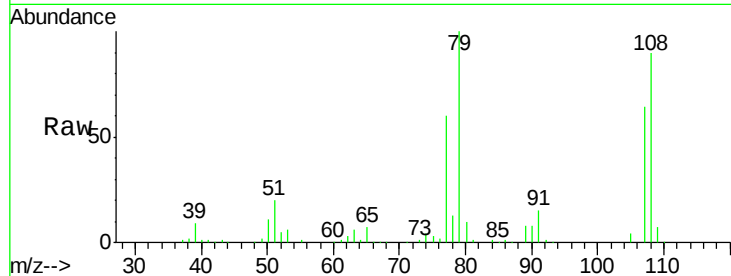

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

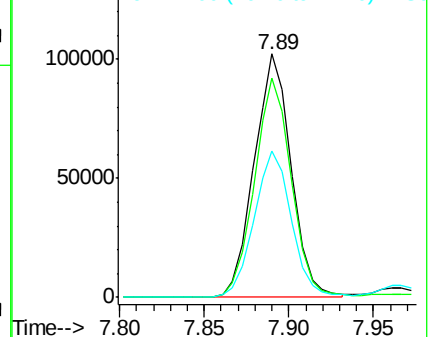

#16

2,2'-oxybis(1-Chloropropane)

Concen: 31.06 ng

RT: 8.18 min Scan# 935

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10


Tgt Ion: 45 Resp: 178733

Ion Ratio Lower Upper



45 100

77 16.8 0.0 35.3

79 13.9 0.0 32.3



Abundance Ion 45.00 (44.70 to 45.70): BGC
Ion 77.00 (76.70 to 77.70): BGC
Ion 79.00 (78.70 to 79.70): BGC

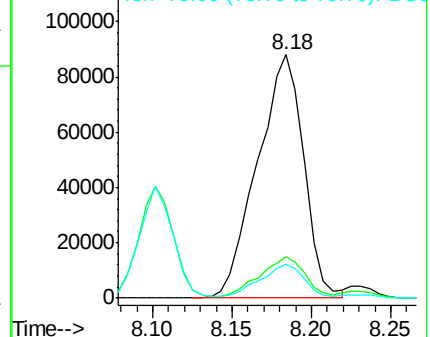






#17
2-Methylphenol
Concen: 37.76 ng
RT: 8.10 min Scan# 921
Delta R.T. -0.02 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion:	107	Resp:	162253
Ion	Ratio	Lower	Upper
107	100		
108	113.7	87.2	130.8
77	37.9	31.1	46.7
79	38.0	29.7	44.5

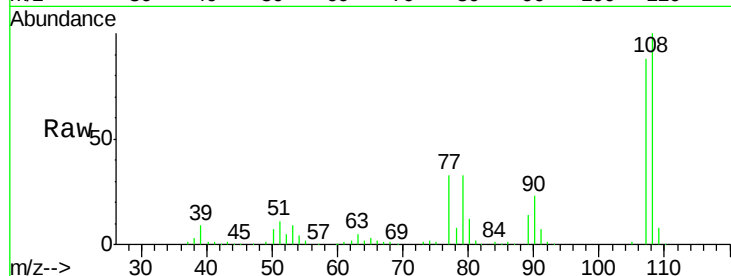


Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BGC
Ion 79.00 (78.70 to 79.70): BGC


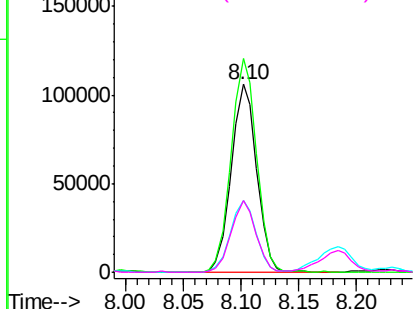



#18
Hexachloroethane
Concen: 37.00 ng
RT: 8.71 min Scan# 1025
Delta R.T. -0.04 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Tgt Ion:	117	Resp:	71043
Ion	Ratio	Lower	Upper
117	100		
119	94.3	78.8	118.2
201	75.3	59.0	88.4

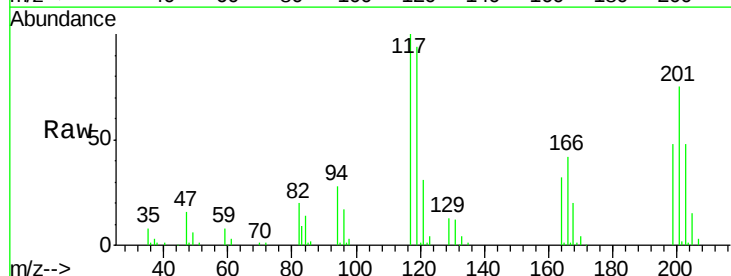

Abundance Ion 117.00 (116.70 to 117.70): E
Ion 119.00 (118.70 to 119.70): E
Ion 201.00 (200.70 to 201.70): E

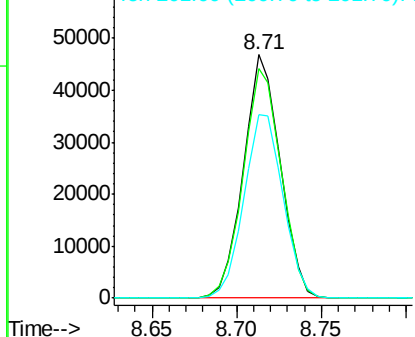


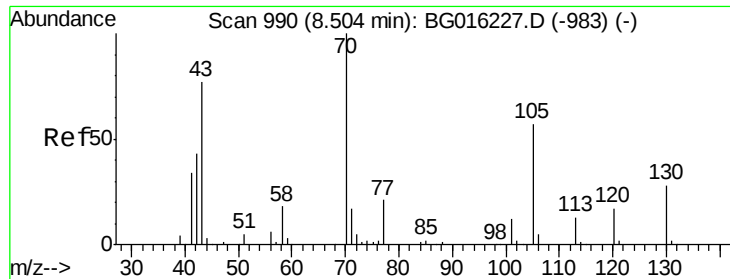




#19
n-Nitroso-di-n-propylamine
Concen: 34.73 ng
RT: 8.45 min Scan# 981
Delta R.T. -0.03 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion: 70 Resp: 149026
Ion Ratio Lower Upper
70 100
42 43.1 34.7 52.1
101 13.1 9.2 13.8
130 33.3 22.6 33.8

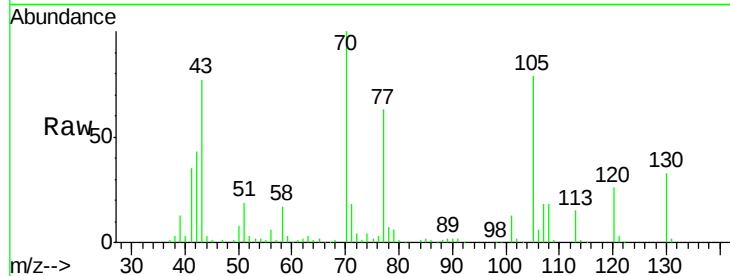


Abundance Ion 70.00 (69.70 to 70.70): BGC
150000
Ion 42.00 (41.70 to 42.70): BGC
100000
Ion 101.00 (100.70 to 101.70): BGC
50000
Ion 130.00 (129.70 to 130.70): BGC
0

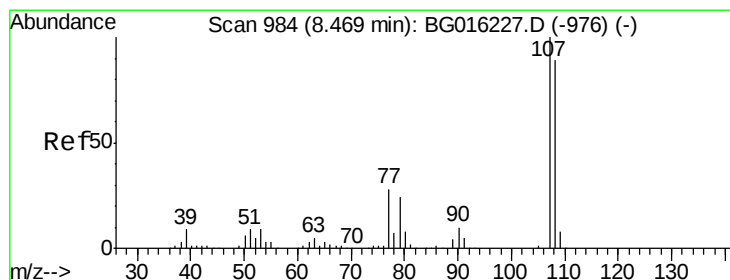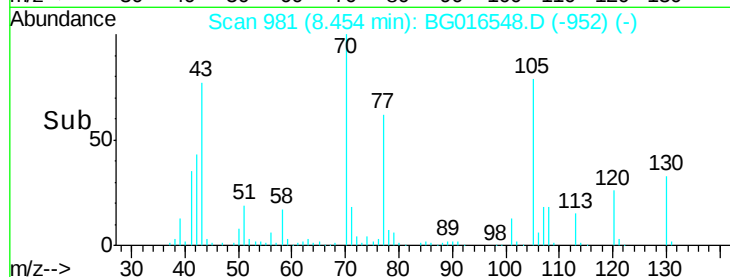
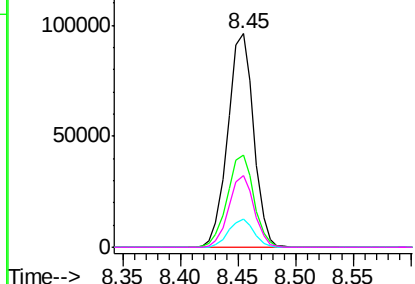



#20
3+4-Methylphenols
Concen: 38.66 ng
RT: 8.43 min Scan# 977
Delta R.T. -0.02 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Tgt Ion: 107 Resp: 230115
Ion Ratio Lower Upper
107 100
108 93.3 69.5 109.5
77 26.9 8.2 48.2
79 24.1 3.8 43.8

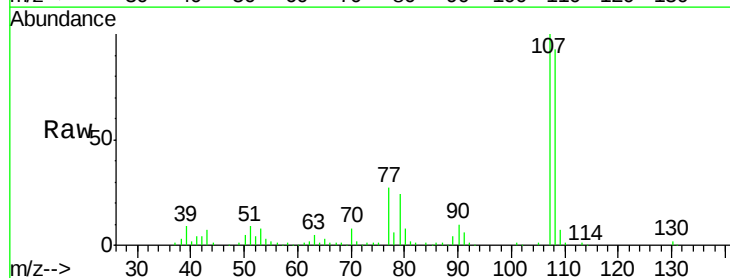

Abundance Ion 107.00 (106.70 to 107.70): BGC
200000
Ion 108.00 (107.70 to 108.70): BGC
150000
Ion 77.00 (76.70 to 77.70): BGC
100000
Ion 79.00 (78.70 to 79.70): BGC
50000
0



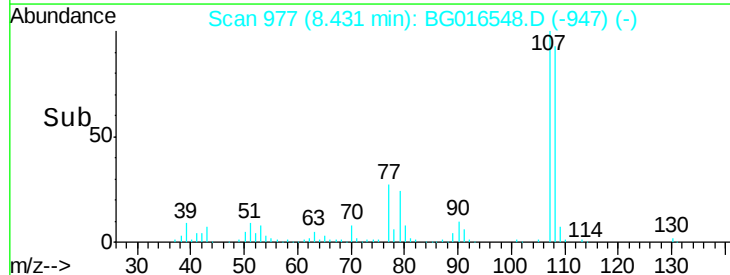
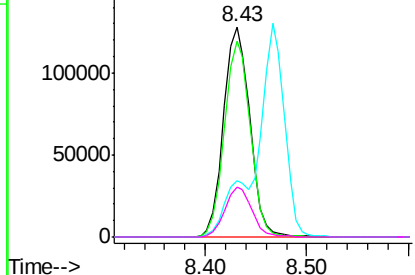


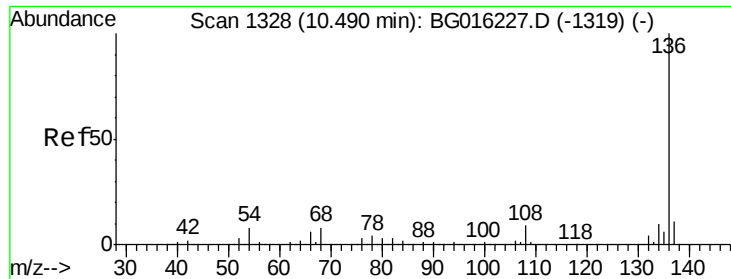

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.43 min Scan# 1318
Delta R.T. -0.03 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10




Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion:	136	Resp:	286305
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	6.6	6.3	9.5
68	6.3	6.5	9.7#

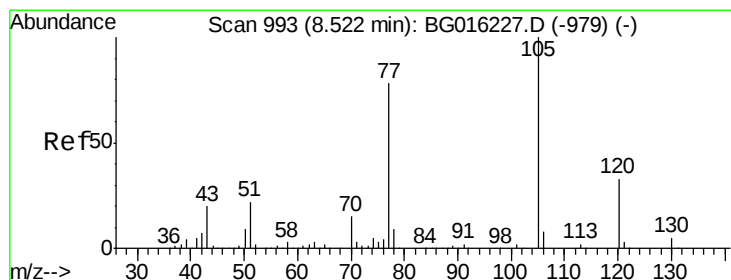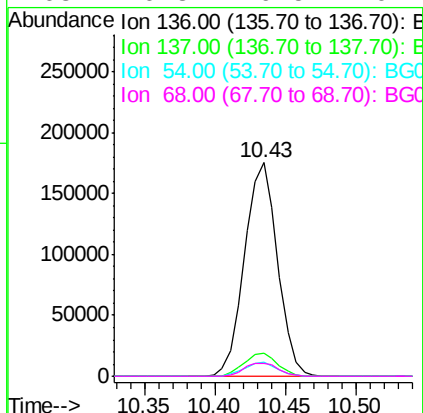

#22
Acetophenone
Concen: 39.92 ng
RT: 8.47 min Scan# 983
Delta R.T. -0.03 min
Lab File: BG016548.D
Acq: 20 Apr 2015 13:10

Tgt Ion:	105	Resp:	265038
Ion	Ratio	Lower	Upper
105	100		
71	3.5	2.0	3.0#
51	20.7	17.9	26.9
120	34.9	26.3	39.5

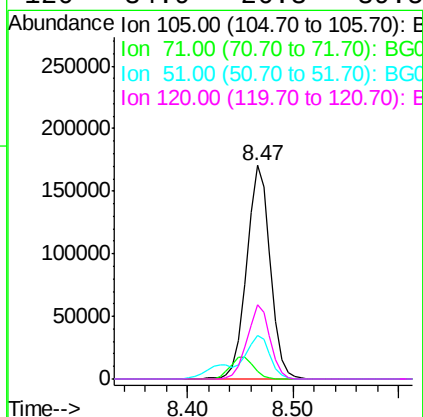







#23
 Nitrobenzene-d5
 Concen: 78.12 ng
 RT: 8.81 min Scan# 1041
 Delta R.T. -0.03 min
 Lab File: BG016548.D
 Acq: 20 Apr 2015 13:10

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Tgt Ion: 82 Resp: 386073
 Ion Ratio Lower Upper
 82 100
 128 54.4 37.8 56.8
 54 38.3 32.6 49.0

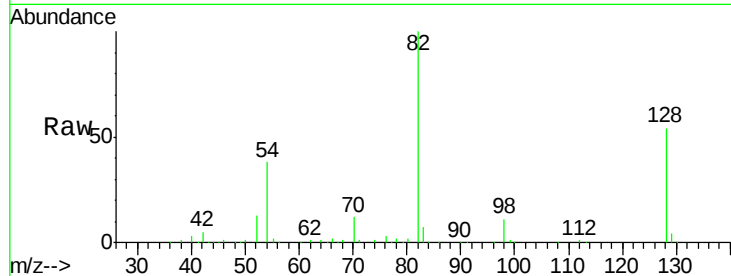


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

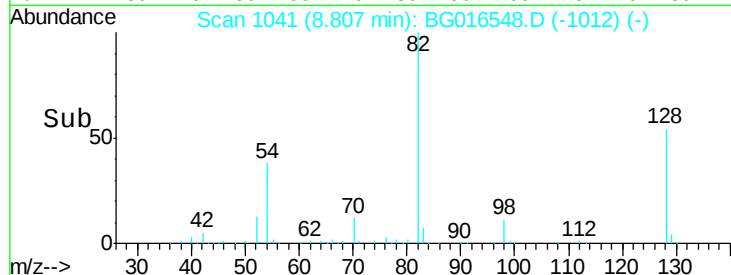
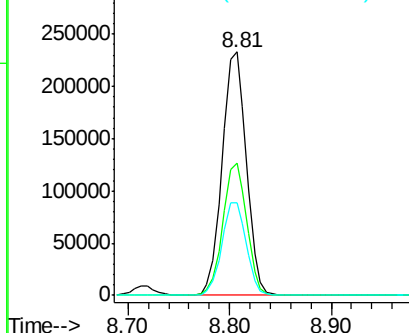


#24
 Nitrobenzene
 Concen: 37.78 ng
 RT: 8.85 min Scan# 1048
 Delta R.T. -0.03 min
 Lab File: BG016548.D
 Acq: 20 Apr 2015 13:10

Tgt Ion: 77 Resp: 199689
 Ion Ratio Lower Upper
 77 100
 123 56.9 38.8 58.2
 65 12.1 9.4 14.2

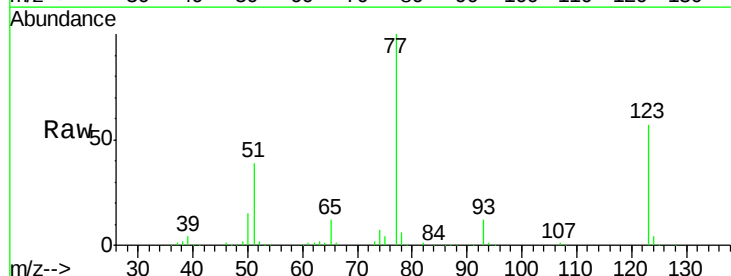

Abundance Ion 77.00 (76.70 to 77.70): BGC
 Ion 123.00 (122.70 to 123.70): BGC
 Ion 65.00 (64.70 to 65.70): BGC

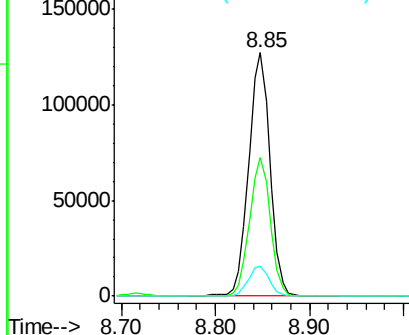



#25

Isophorone

Concen: 38.61 ng

RT: 9.36 min Scan# 1136

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 82 Resp: 423798

Ion Ratio Lower Upper




82 100

95 6.2 5.0 7.6

138 23.4 16.2 24.2

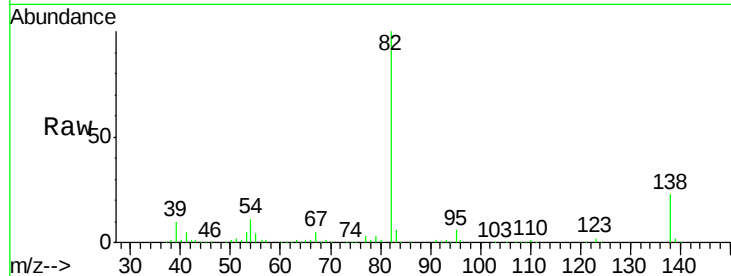

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 95.00 (94.70 to 95.70): BGC
Ion 138.00 (137.70 to 138.70): BGC

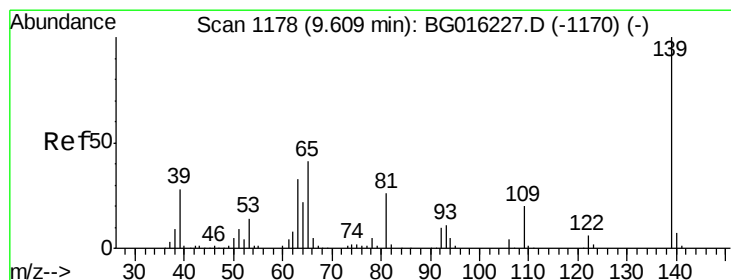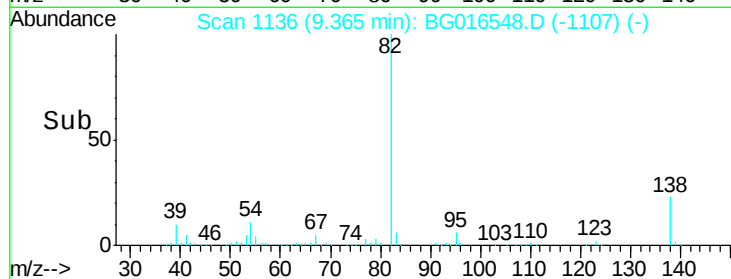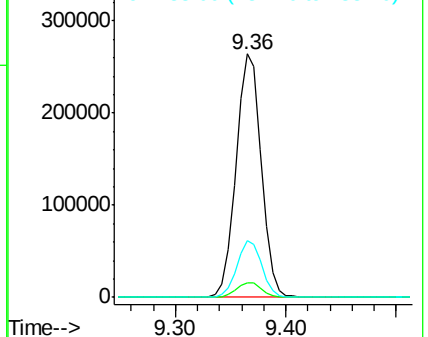

#26

2-Nitrophenol

Concen: 48.20 ng

RT: 9.55 min Scan# 1168

Delta R.T. -0.03 min

Lab File: BG016548.D

Acq: 20 Apr 2015 13:10


Tgt Ion: 139 Resp: 118791

Ion Ratio Lower Upper

139 100

109 20.1 15.9 23.9

65 37.9 32.9 49.3



Abundance Ion 139.00 (138.70 to 139.70): BGC
Ion 109.00 (108.70 to 109.70): BGC
Ion 65.00 (64.70 to 65.70): BGC

