


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042015\
 Data File : BG016547.D
 Acq On : 20 Apr 2015 10:59
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 14 14:00:56 2015

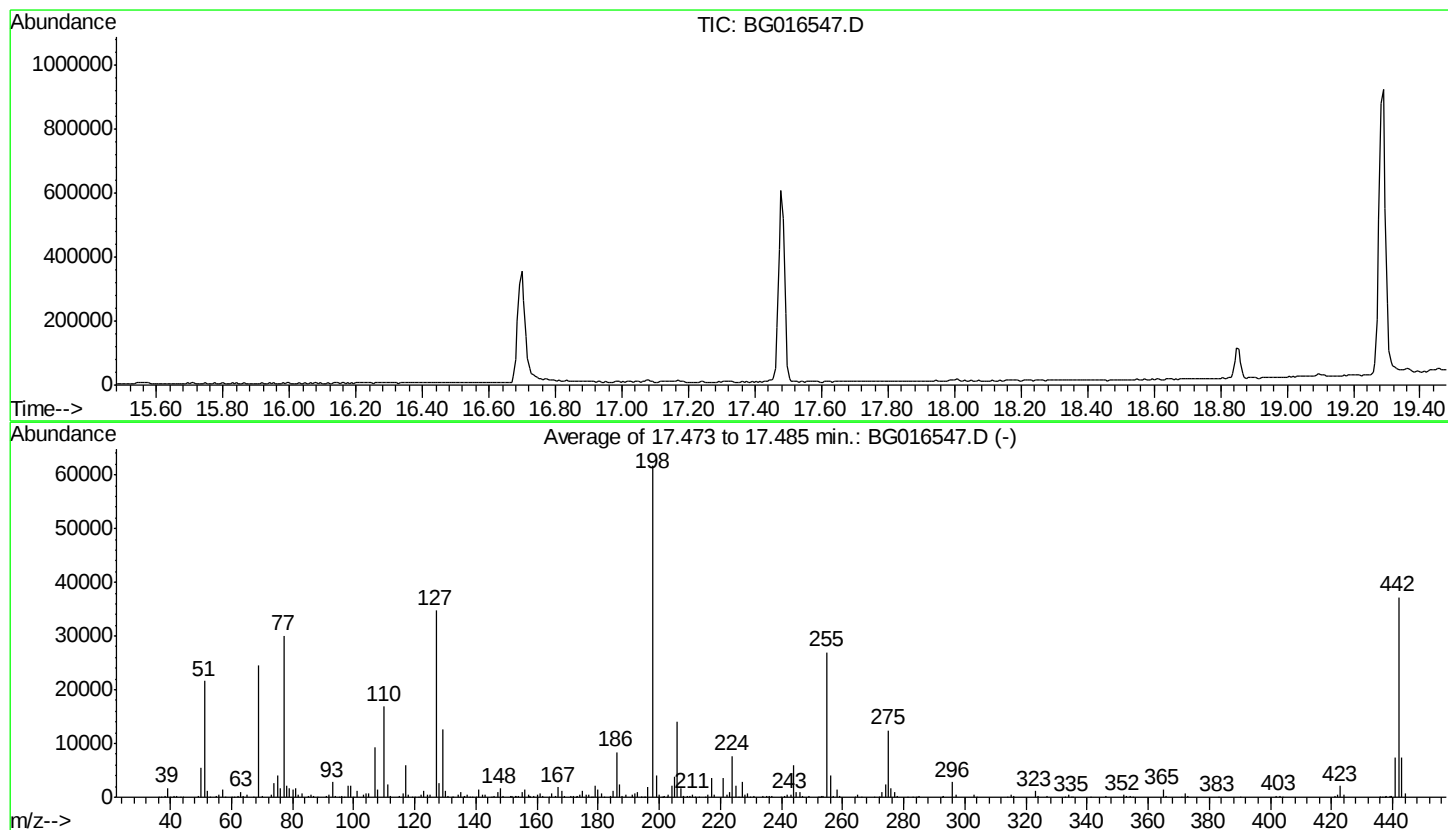

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	21662	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.6	24435	PASS
70	69	0.00	2	1.1	258	PASS
127	198	10	80	56.3	34754	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61706	PASS
199	198	5	9	6.7	4125	PASS
275	198	10	60	20.1	12422	PASS
365	198	1	100	2.3	1425	PASS
441	442	0.01	24	19.8	7350	PASS
442	198	50	100	60.2	37176	PASS
443	442	15	24	20.2	7508	PASS