
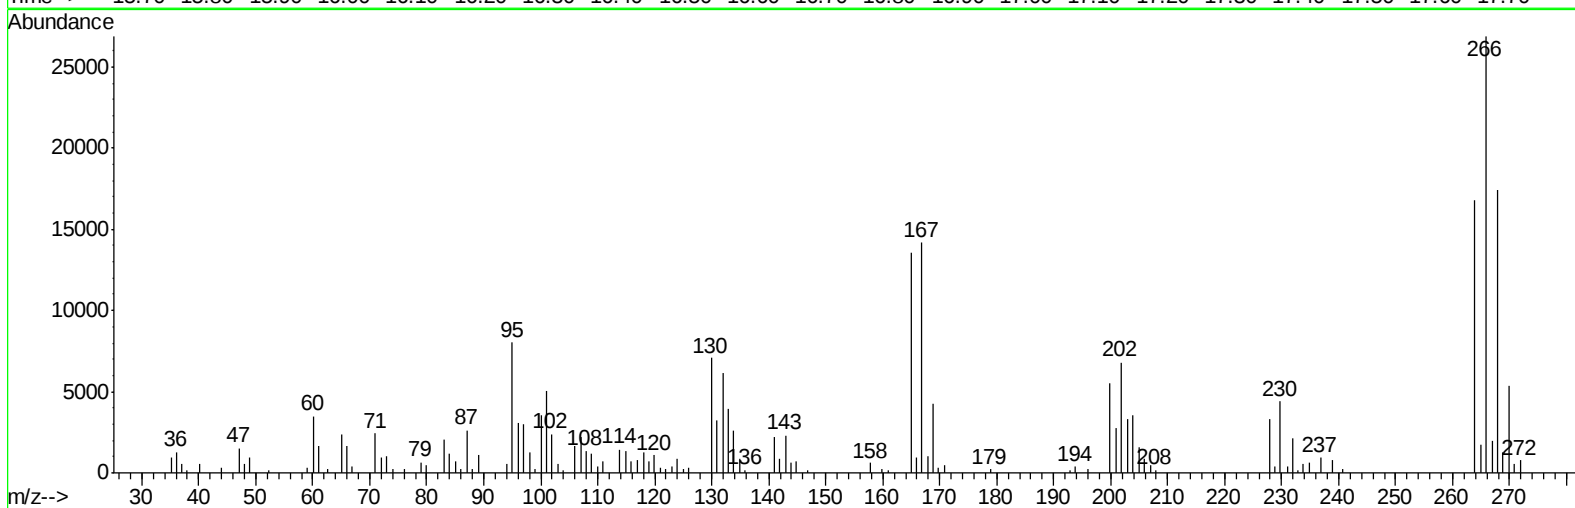


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042015\
Data File : BG016565.D
Acq On : 21 Apr 2015 1:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:20:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 03:54:20 2015
Response via : Initial Calibration

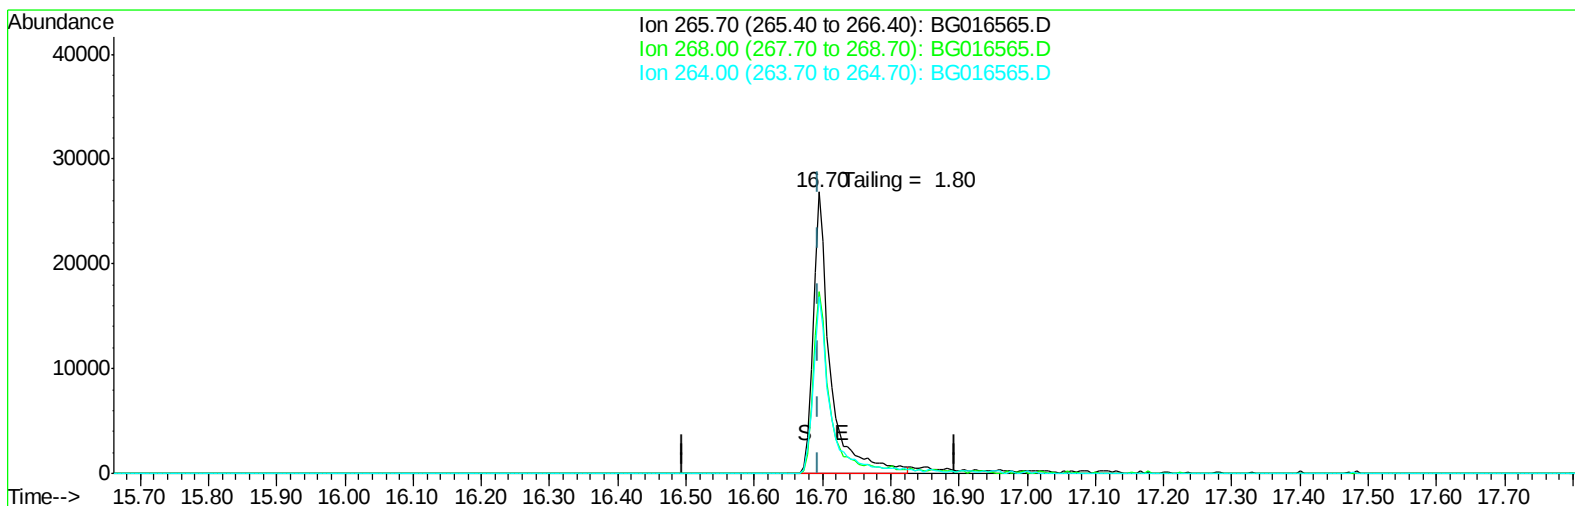

TIC: BG016565.D

(69) Pentachlorophenol (C)



16.695min (+0.001) 34200.82ng

response 46445

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	64.76
264.00	66.00	62.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042015\
Data File : BG016565.D
Acq On : 21 Apr 2015 1:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:20:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 03:54:20 2015
Response via : Initial Calibration

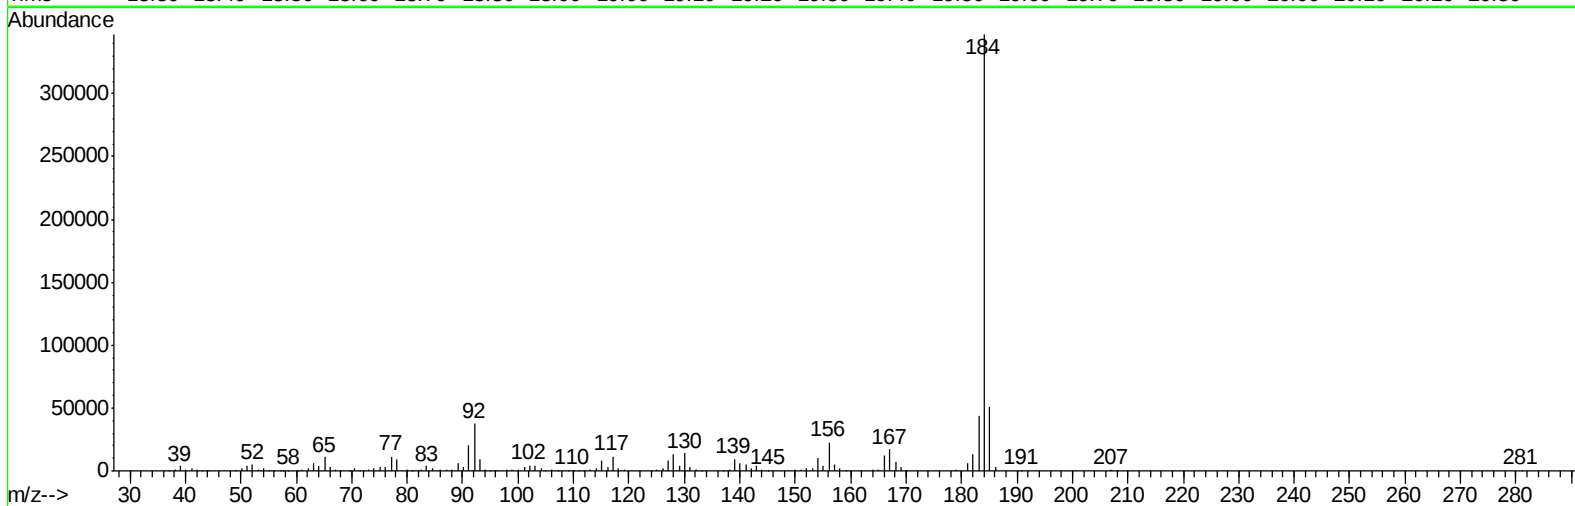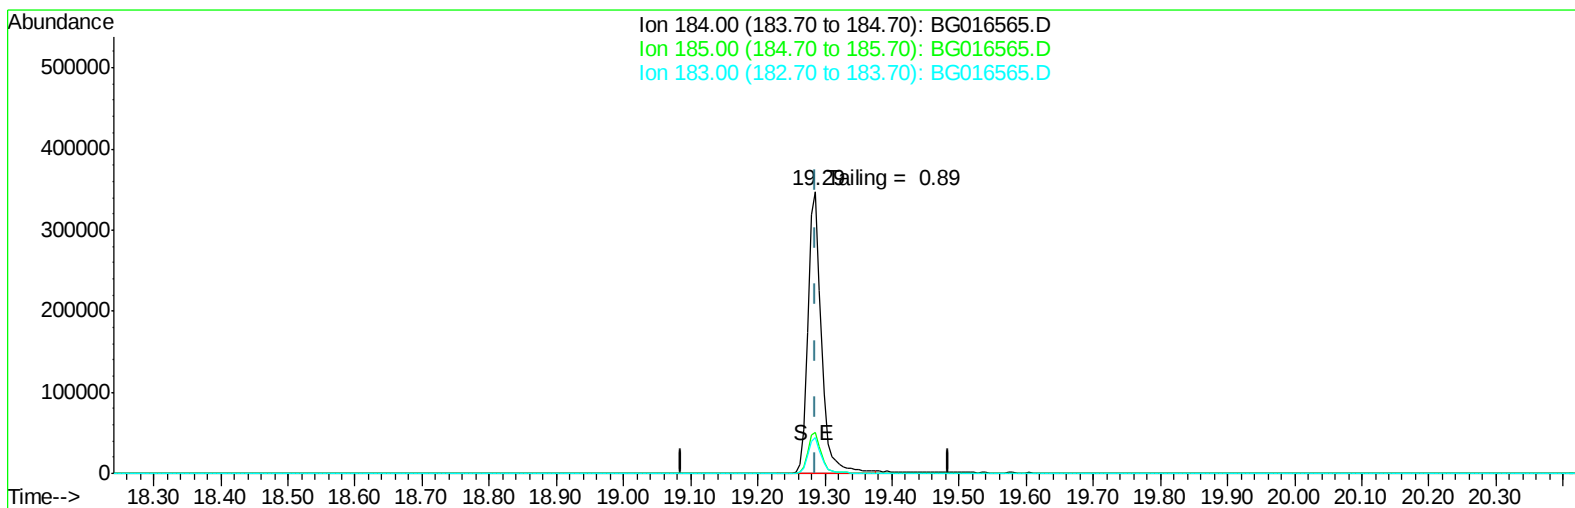

TIC: BG016565.D

(76) Benzidine

19.286min (+0.001) 22303.81ng

response 484273

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.61
183.00	13.00	12.59
0.00	0.00	0.00