
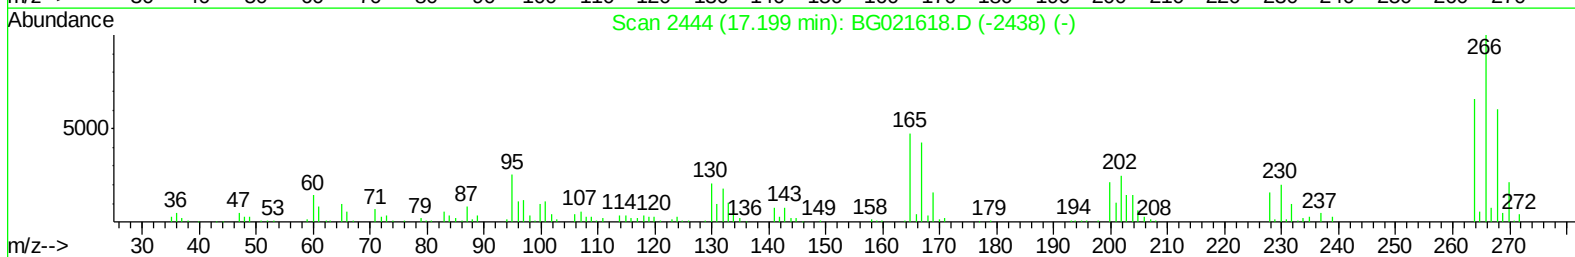
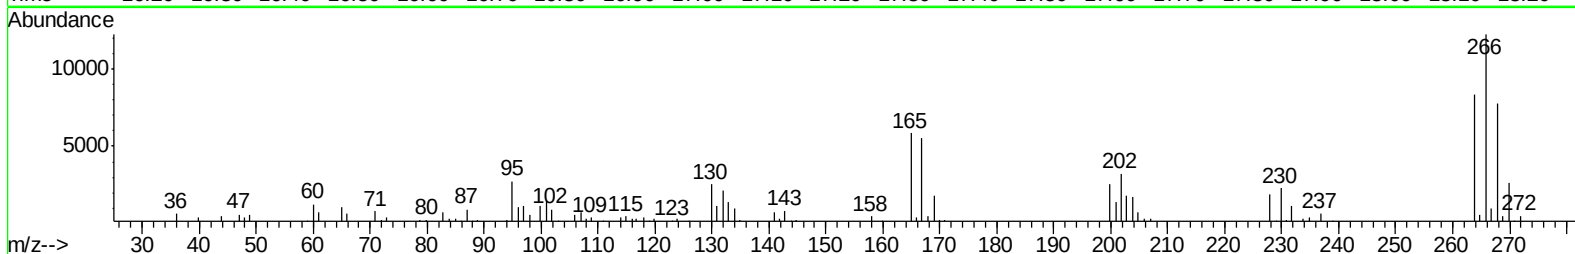


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042016\
Data File : BG021761.D
Acq On : 19 Apr 2016 18:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 04:15:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

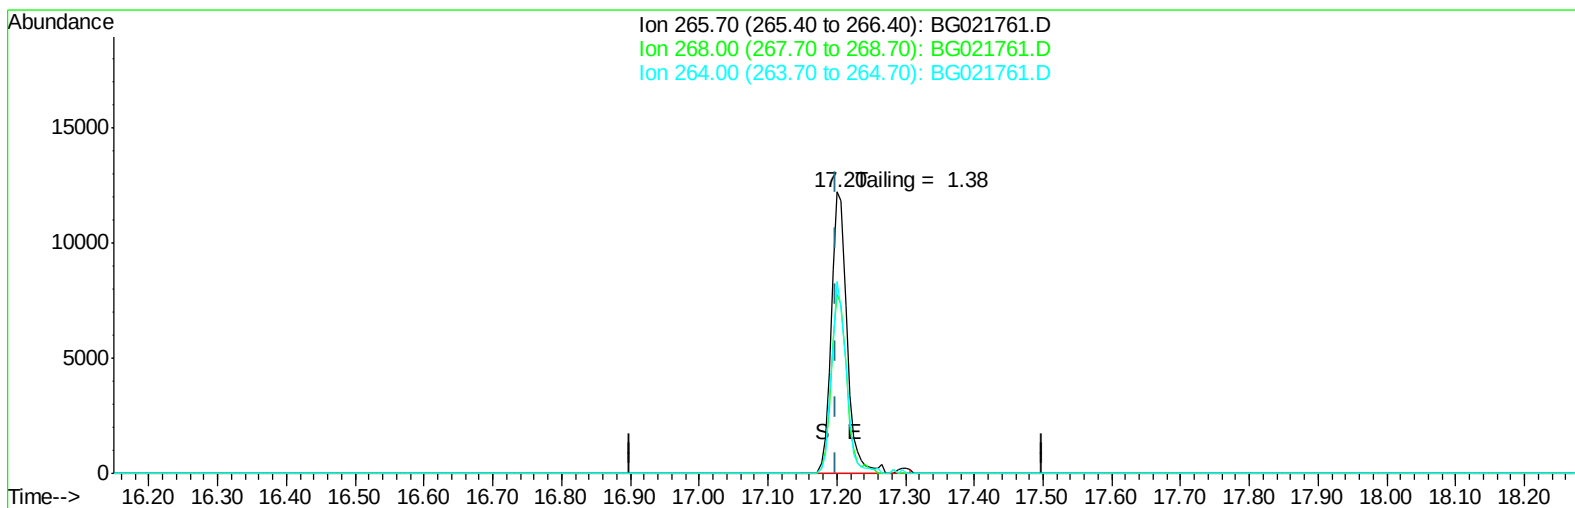

TIC: BG021761.D

(69) Pentachlorophenol (C)




17.201min (+0.002) 0.00ng

response 19202

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	63.44
264.00	67.20	68.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042016\
Data File : BG021761.D
Acq On : 19 Apr 2016 18:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 04:15:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

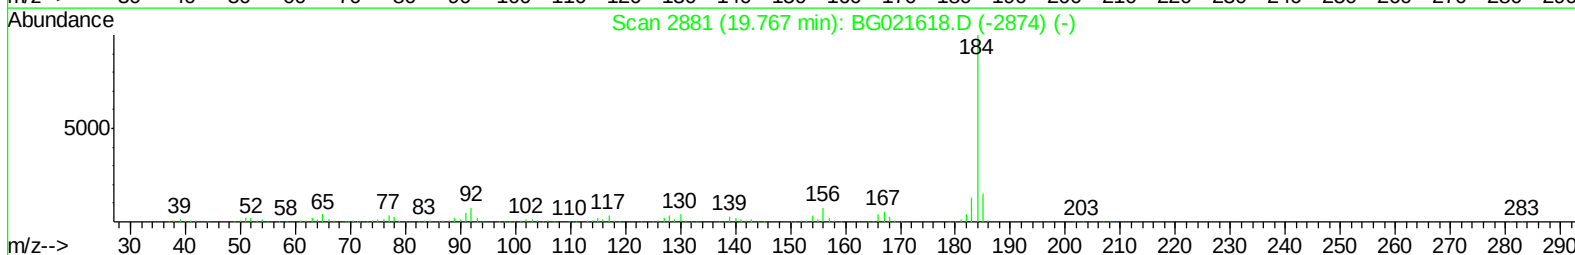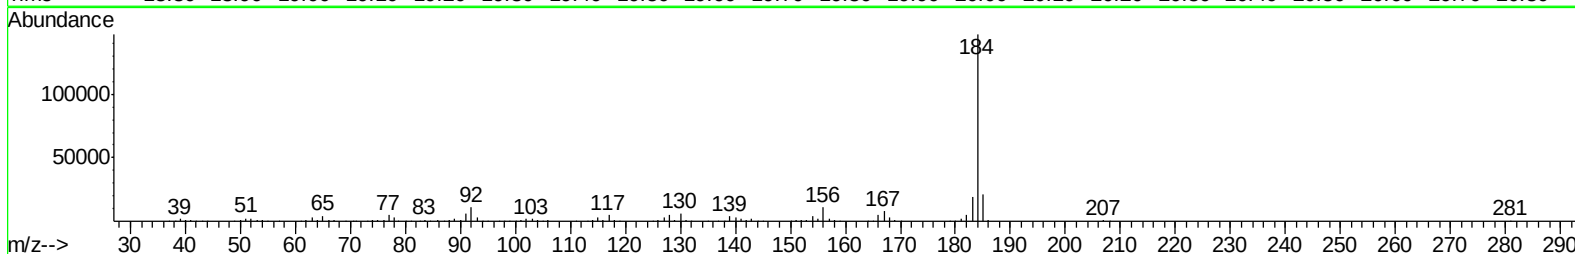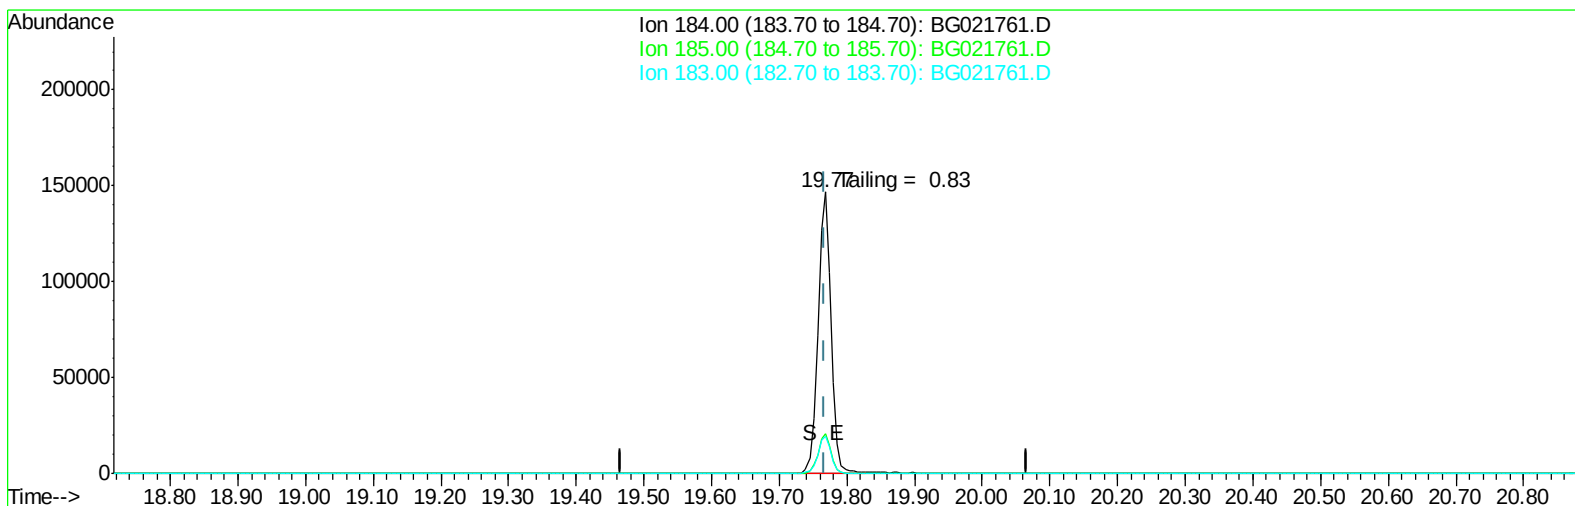

TIC: BG021761.D

(76) Benzidine

19.768min (+0.002) 121546.91ng

response 200574

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.23
183.00	12.80	13.24
0.00	0.00	0.00