

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042016\
 Data File : BG021764.D
 Acq On : 19 Apr 2016 20:57
 Operator : UM/SJ
 Sample : H2620-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EUT01-TU-B2(9-13)-C

Quant Time: Apr 20 03:26:03 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 15:48:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	26565	20.00	ng	0.00
21) Naphthalene-d8	11.03	136	124605	20.00	ng	0.00
38) Acenaphthene-d10	14.82	164	82580	20.00	ng	0.00
63) Phenanthrene-d10	17.56	188	176630	20.00	ng	0.00
75) Chrysene-d12	21.83	240	194326	20.00	ng	0.00
86) Perylene-d12	25.16	264	190058	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.76	112	193526	121.31	ng	0.00
7) Phenol-d6	7.37	99	292394	122.71	ng	0.01
23) Nitrobenzene-d5	9.38	82	180658	74.52	ng	0.00
41) 2,4,6-Tribromophenol	16.30	330	114085	128.18	ng	0.00
44) 2-Fluorobiphenyl	13.45	172	423739	75.18	ng	0.00
78) Terphenyl-d14	20.14	244	533973	68.56	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.26	163	52017	7.29	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042016\
Data File : BG021764.D
Acq On : 19 Apr 2016 20:57
Operator : UM/SJ
Sample : H2620-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EUT01-TU-B2(9-13)-C

Quant Time: Apr 20 03:26:03 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

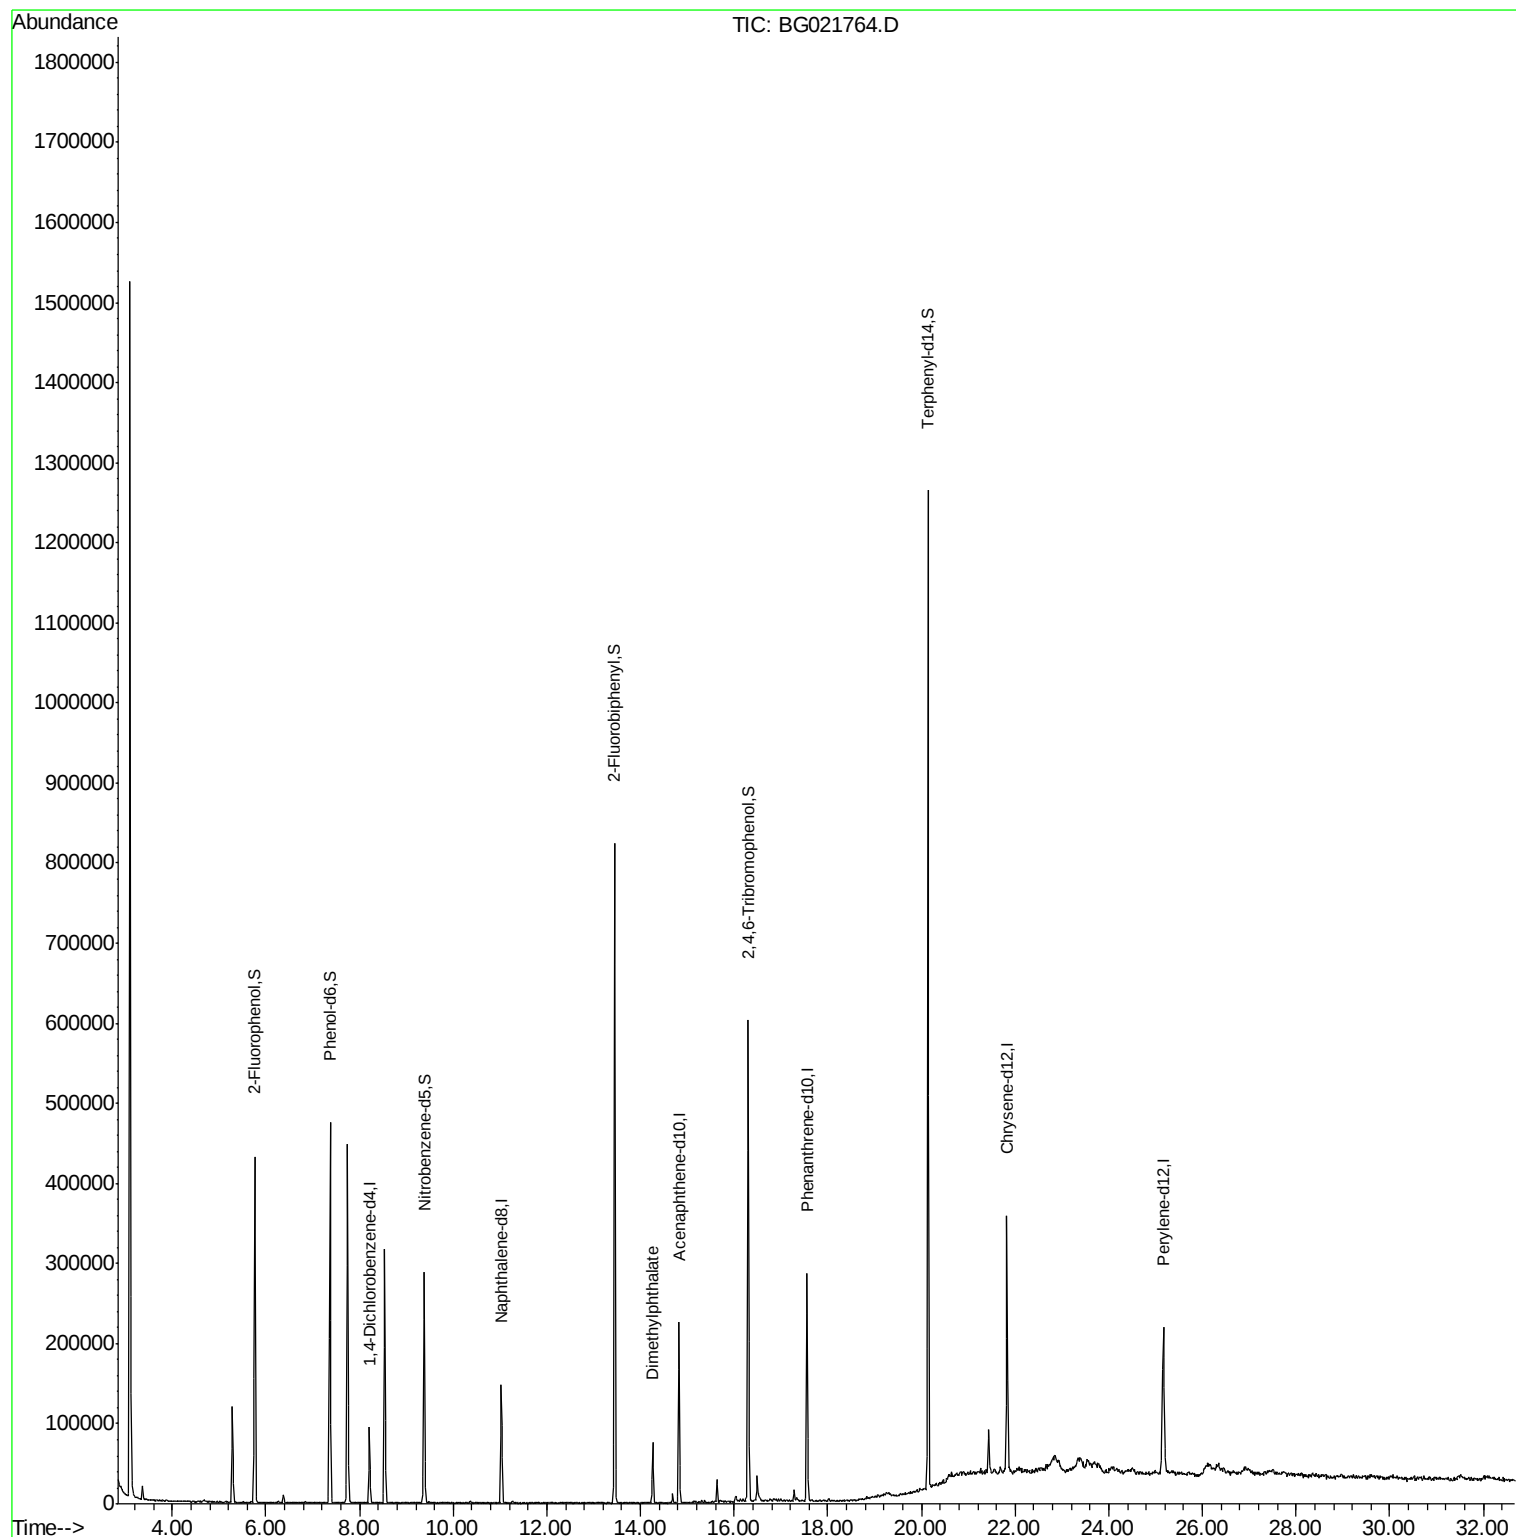

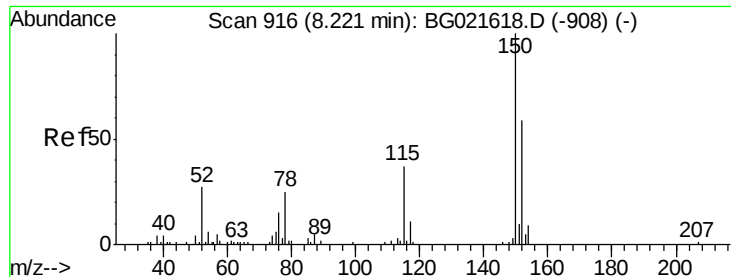


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.21 min Scan# 915
Delta R.T. -0.01 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57

Instrument :
BNA_G
ClientSampleId :
EUT01-TU-B2(9-13)-C

Tot Ion:152 Resp: 26565
Ion Ratio Lower Upper
152 100
150 161.9 130.1 195.1
115 64.3 62.2 93.2

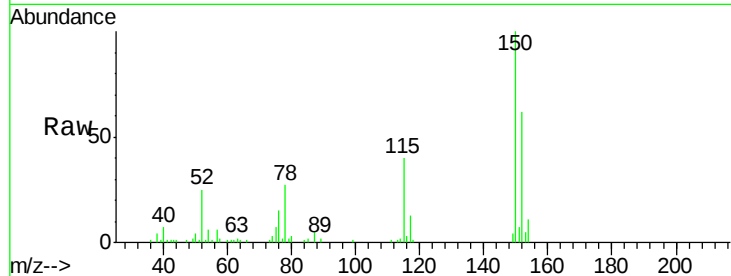


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

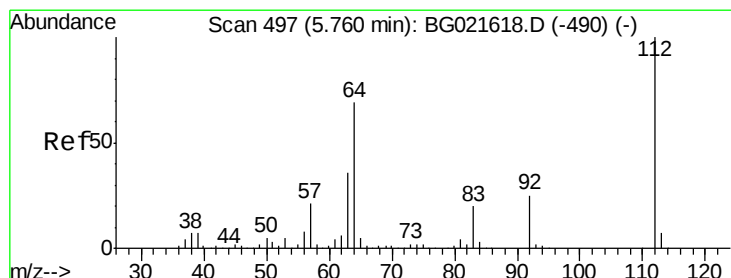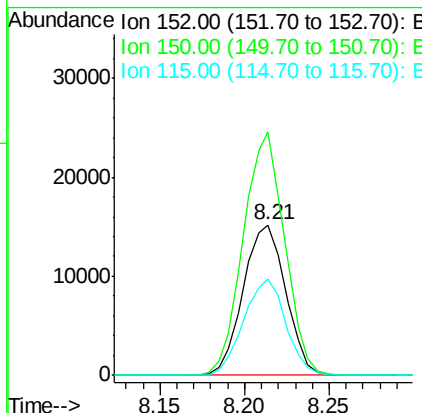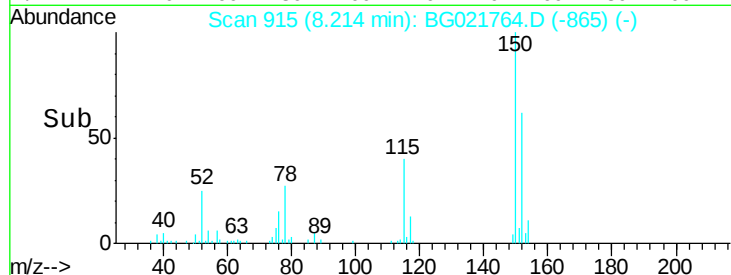



#5


2-Fluorophenol
Concen: 121.31 ng
RT: 5.76 min Scan# 498
Delta R.T. 0.00 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57

Tgt Ion:112 Resp: 193526
Ion Ratio Lower Upper
112 100
64 65.6 51.1 76.7
63 34.9 24.6 37.0

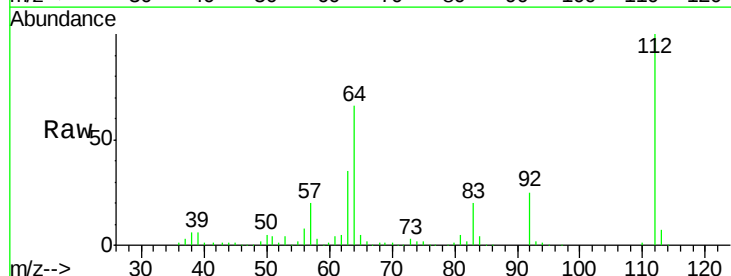

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

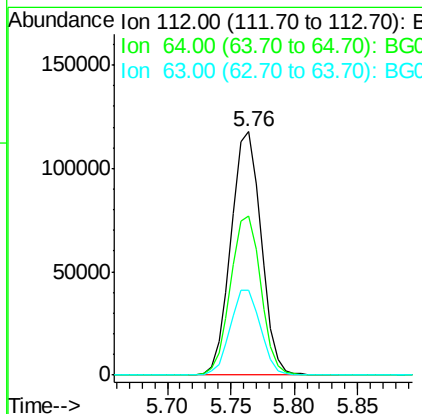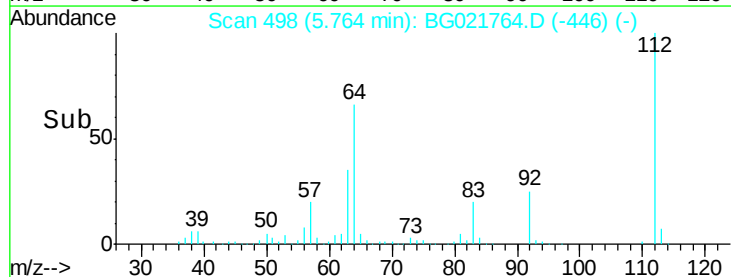

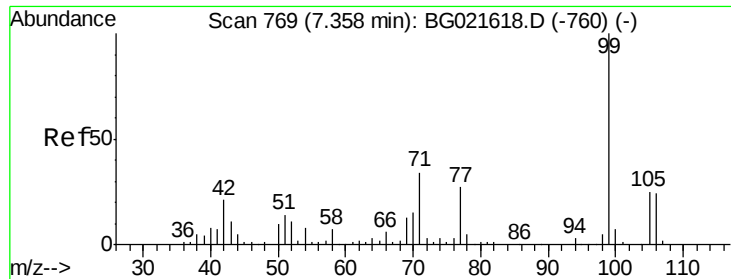

#7

Phenol-d6

Concen: 122.71 ng

RT: 7.37 min Scan# 771

Delta R.T. 0.01 min

Lab File: BG021764.D

Acq: 19 Apr 2016 20:57

Instrument :

BNA_G

ClientSampleId :

EUT01-TU-B2(9-13)-C


Tot Ion: 99 Resp: 292394

Ion Ratio Lower Upper




99 100

42 19.0 16.4 24.6

71 32.9 25.0 37.4

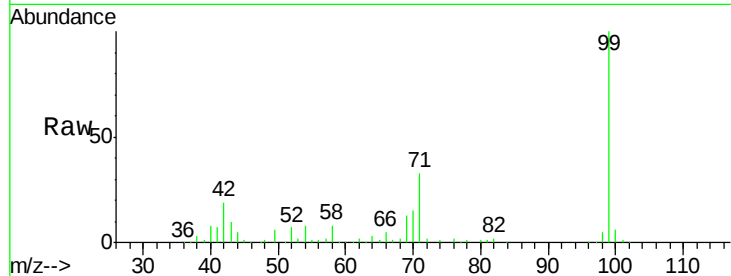

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

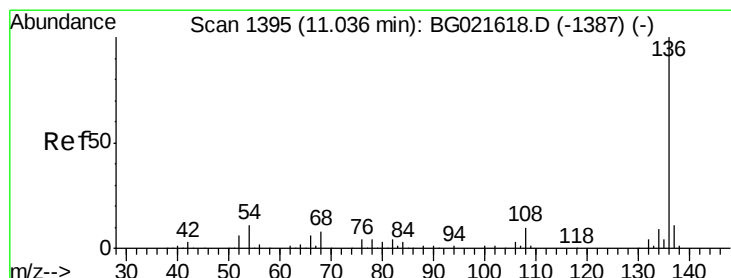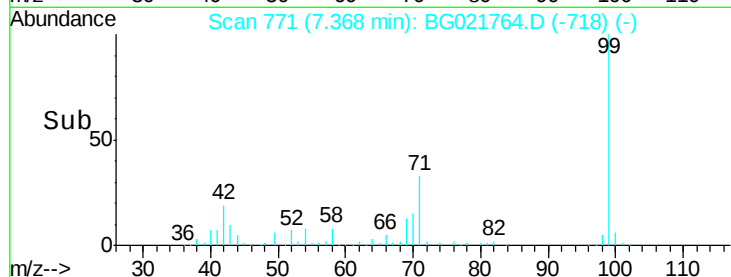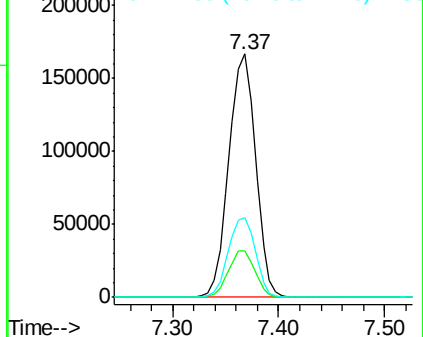

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.03 min Scan# 1394

Delta R.T. -0.01 min

Lab File: BG021764.D

Acq: 19 Apr 2016 20:57

Tgt Ion: 136 Resp: 124605


Ion Ratio Lower Upper

136 100



137 11.7 9.0 13.4


54 10.8 9.6 14.4

68 7.9 6.4 9.6

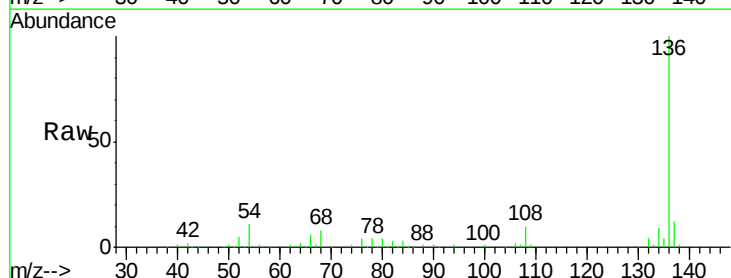

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

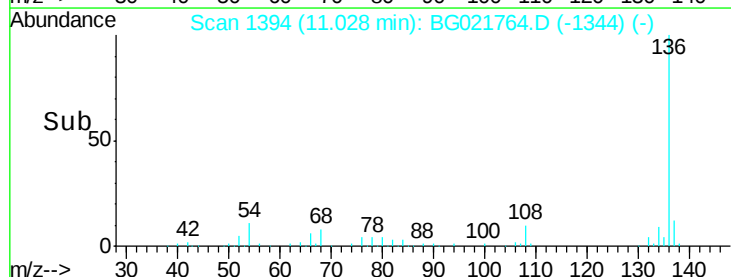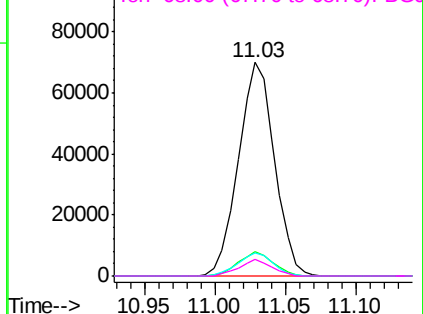


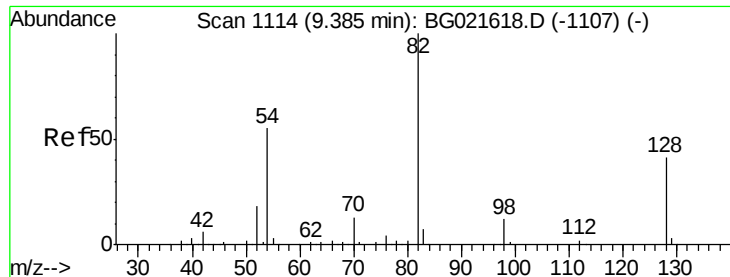




#23
Nitrobenzene-d5
Concen: 74.52 ng
RT: 9.38 min Scan# 1113
Delta R.T. -0.01 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57

Instrument :
BNA_G
ClientSampleId :
EUT01-TU-B2(9-13)-C

Tot Ion	82	Resp	180658
Ion Ratio	100	Lower	Upper
128	41.1	33.4	50.0
54	55.0	46.1	69.1

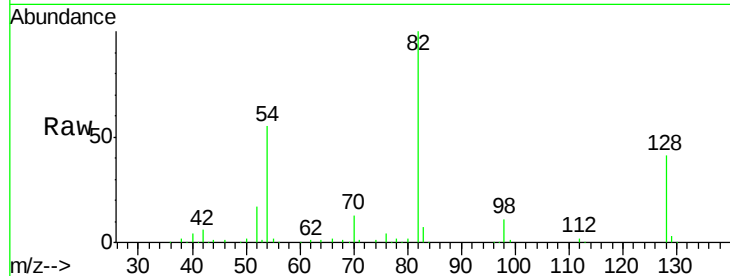


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

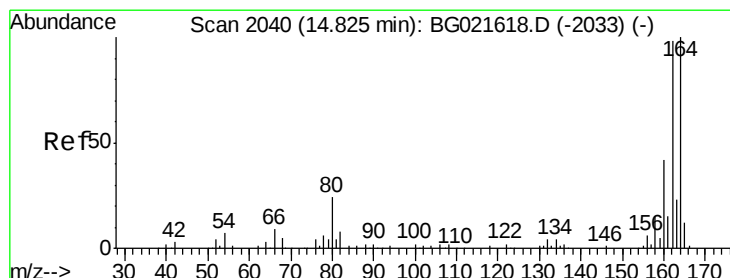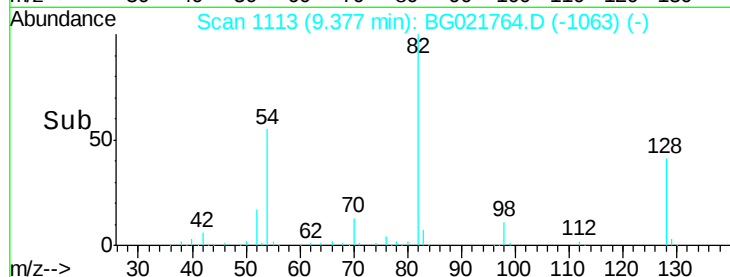
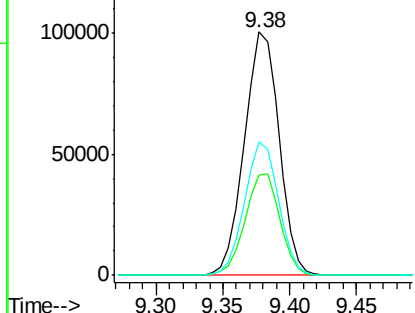



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.82 min Scan# 2040
Delta R.T. -0.00 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57

Tgt Ion	164	Resp	82580
Ion Ratio	100	Lower	Upper
162	100.3	78.0	117.0
160	45.4	32.9	49.3

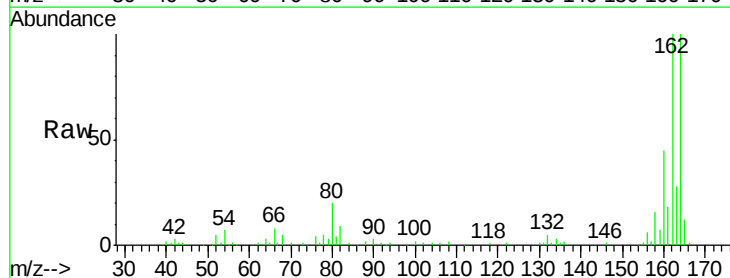

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

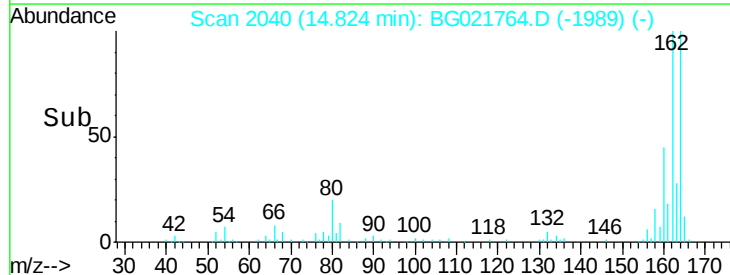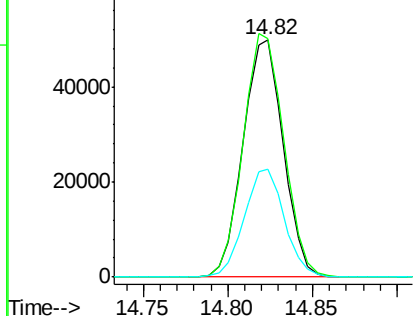


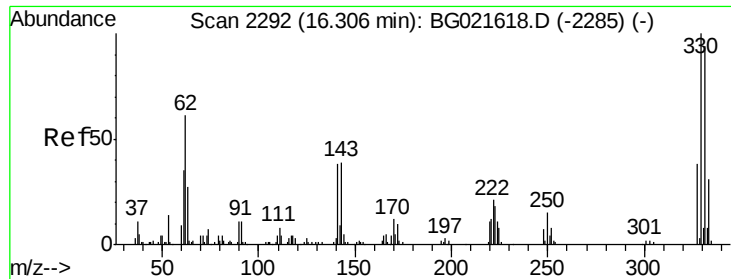




#41
 2,4,6-Tribromophenol
 Concen: 128.18 ng
 RT: 16.30 min Scan# 2292
 Delta R.T. -0.00 min
 Lab File: BG021764.D
 Acq: 19 Apr 2016 20:57

Instrument :
 BNA_G
 ClientSampleId :
 EUT01-TU-B2(9-13)-C

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	78.0	117.0
141	37.6	33.8	50.8

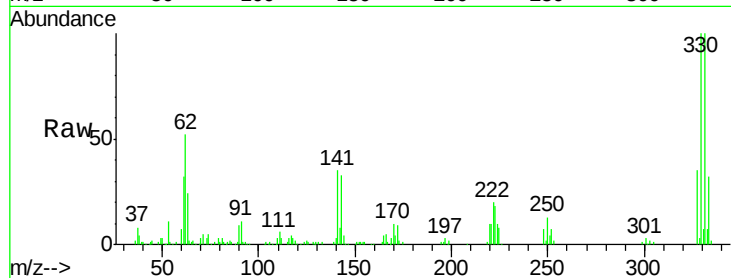


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

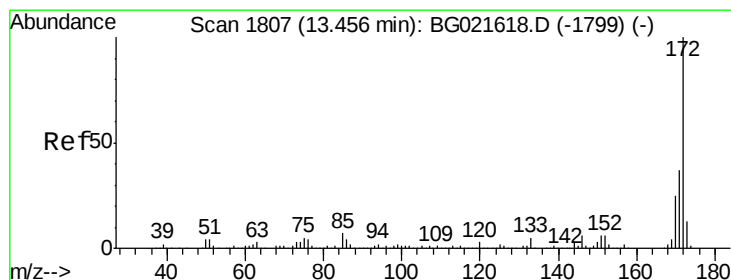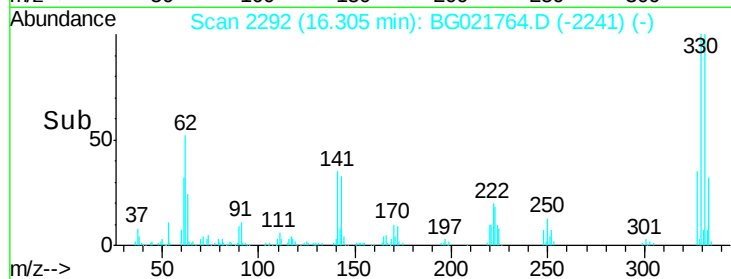
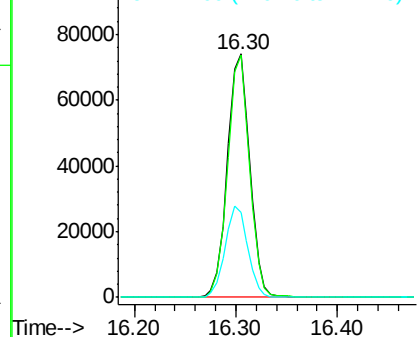



#44
 2-Fluorobiphenyl
 Concen: 75.18 ng
 RT: 13.45 min Scan# 1806
 Delta R.T. -0.01 min
 Lab File: BG021764.D
 Acq: 19 Apr 2016 20:57

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.4	27.8	41.6
170	24.6	19.6	29.4

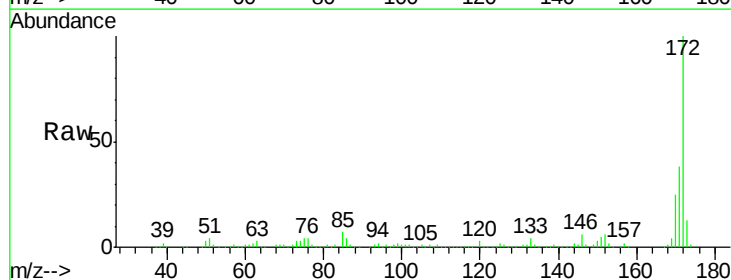

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

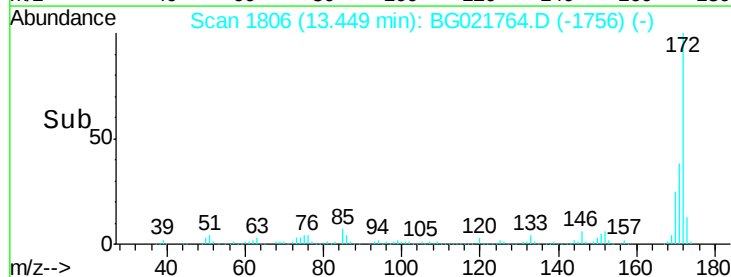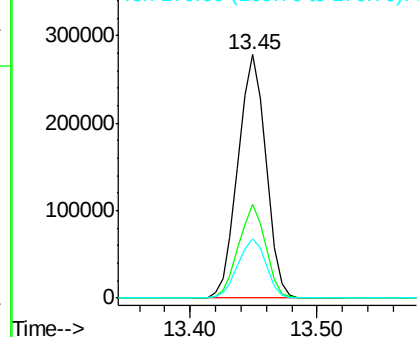

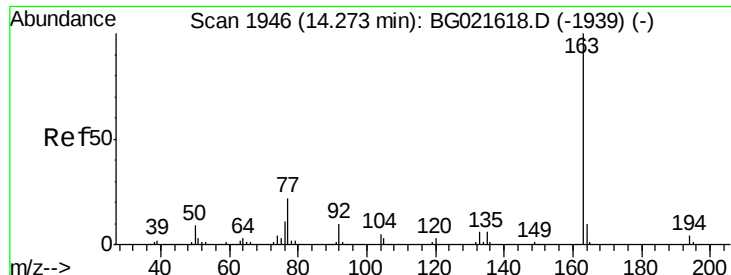

#49

Dimethylphthalate

Concen: 7.29 ng

RT: 14.26 min Scan# 1944

Delta R.T. -0.01 min

Lab File: BG021764.D

Acq: 19 Apr 2016 20:57

Instrument :

BNA_G

ClientSampleId :

EUT01-TU-B2(9-13)-C


Tot Ion:163 Resp: 52017

Ion Ratio Lower Upper

163 100

194 3.3 3.0 4.6




164 9.8 8.1 12.1

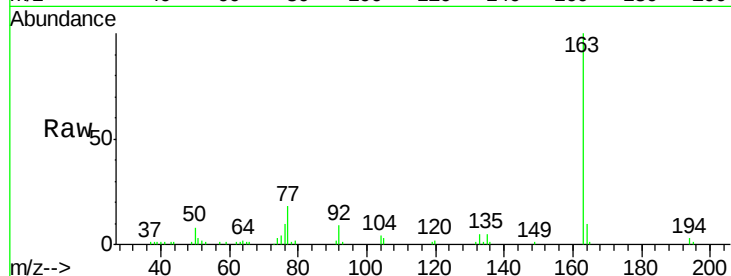

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

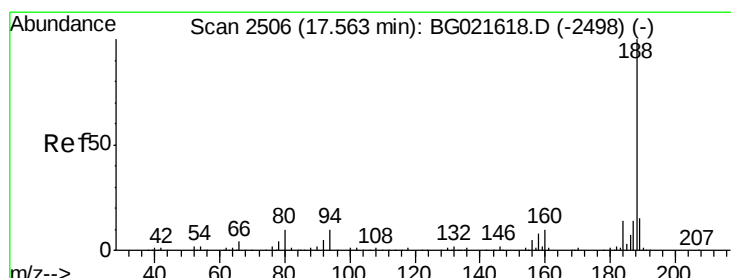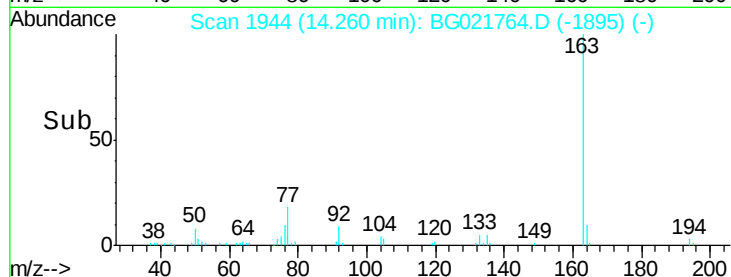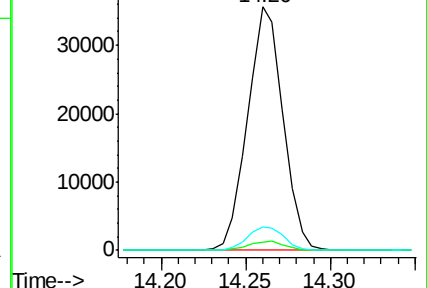

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.56 min Scan# 2505

Delta R.T. -0.01 min

Lab File: BG021764.D

Acq: 19 Apr 2016 20:57


Tgt Ion:188 Resp: 176630

Ion Ratio Lower Upper

188 100

94 8.6 7.5 11.3



80 11.0 8.6 13.0

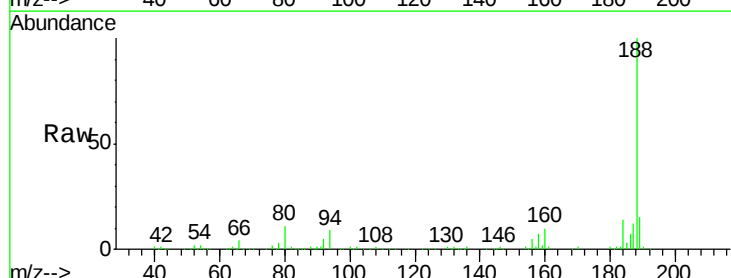


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



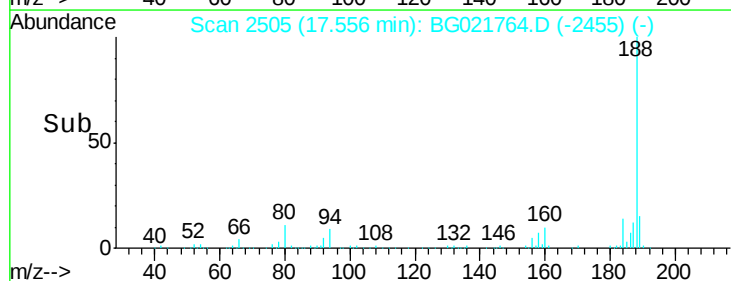
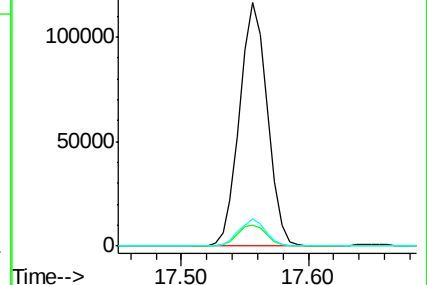


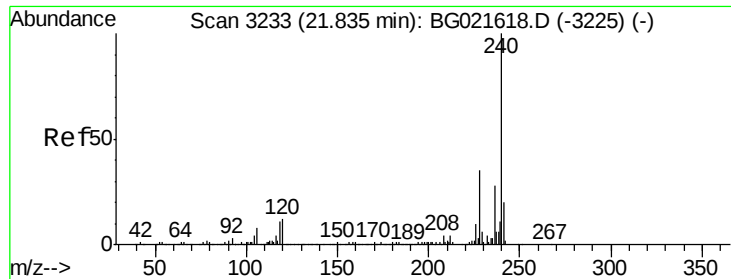

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.83 min Scan# 3232
Delta R.T. -0.01 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57




Instrument :
BNA_G
ClientSampleId :
EUT01-TU-B2(9-13)-C


Tot Ion:240 Resp: 194326
Ion Ratio Lower Upper
240 100
120 10.1 8.4 12.6
236 26.5 19.6 29.4

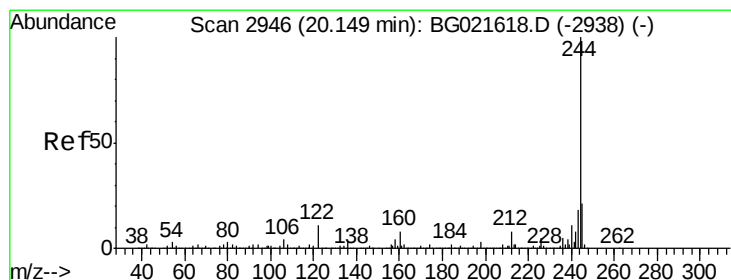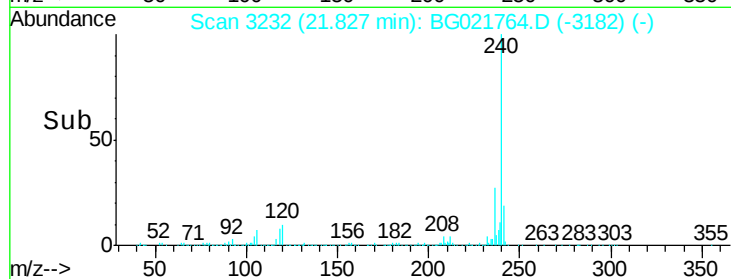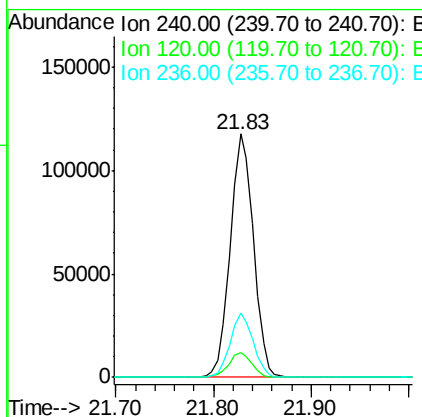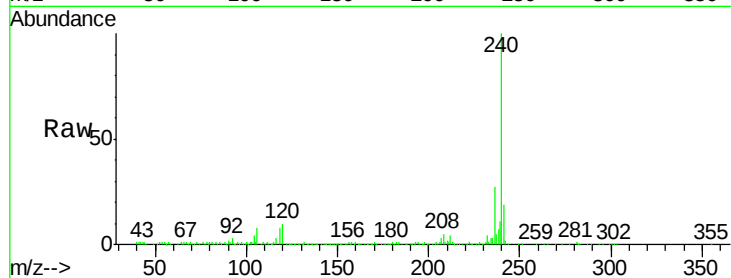

#78
Terphenyl-d14
Concen: 68.56 ng
RT: 20.14 min Scan# 2945
Delta R.T. -0.01 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57

Tgt Ion:244 Resp: 533973
Ion Ratio Lower Upper
244 100
212 8.3 6.5 9.7
122 10.6 8.6 12.8

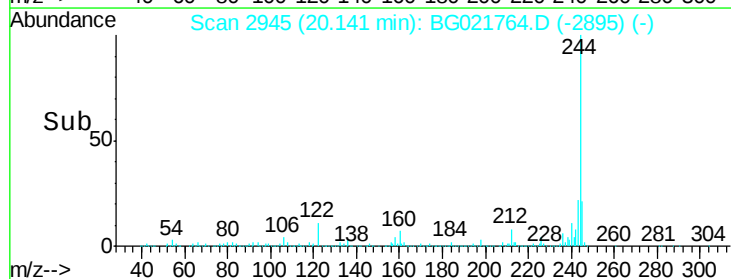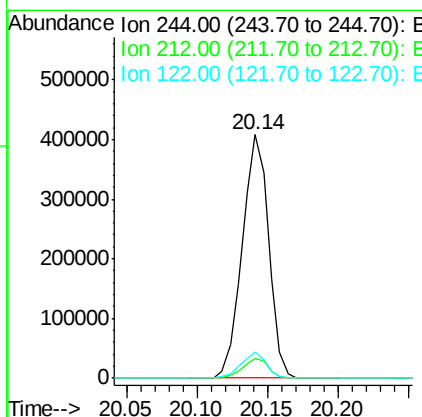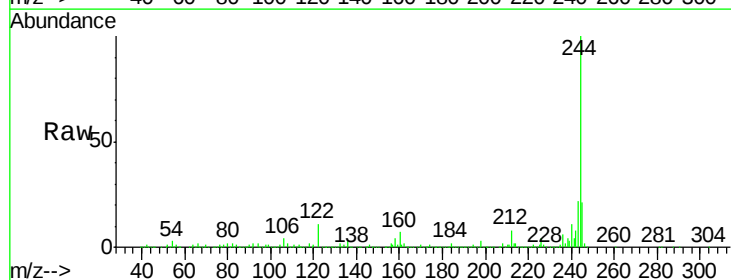


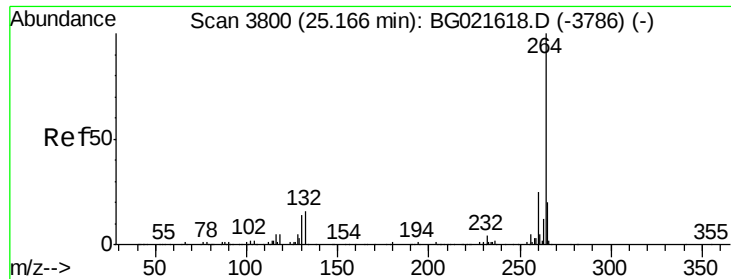

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.16 min Scan# 3800
Delta R.T. -0.00 min
Lab File: BG021764.D
Acq: 19 Apr 2016 20:57

Instrument :
BNA_G
ClientSampleId :
EUT01-TU-B2(9-13)-C

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	20.2	30.4
265	20.8	17.8	26.8

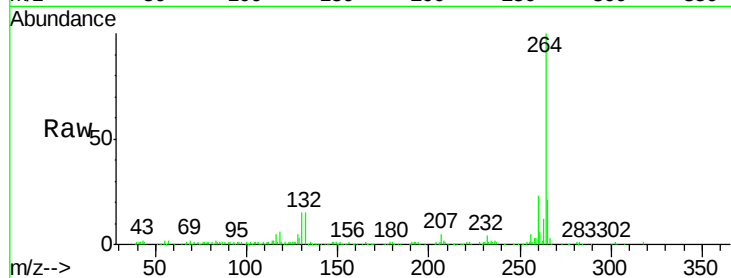

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

