
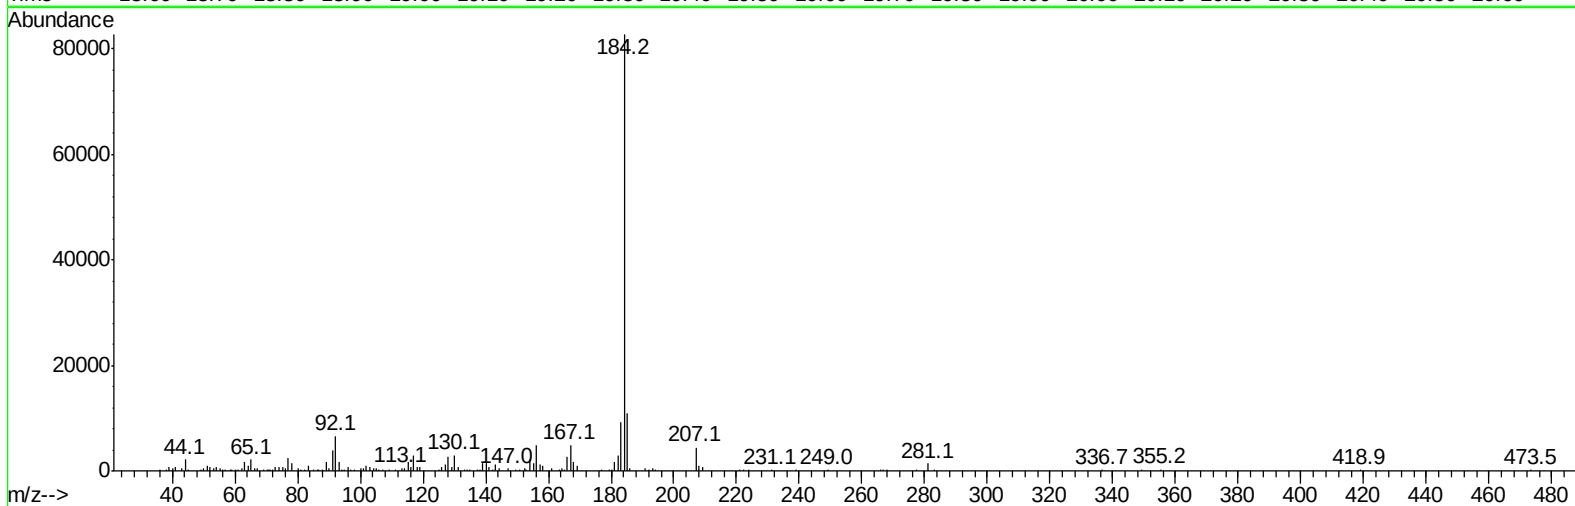


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042017\
Data File : BG026677.D
Acq On : 20 Apr 2017 15:26
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:19:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

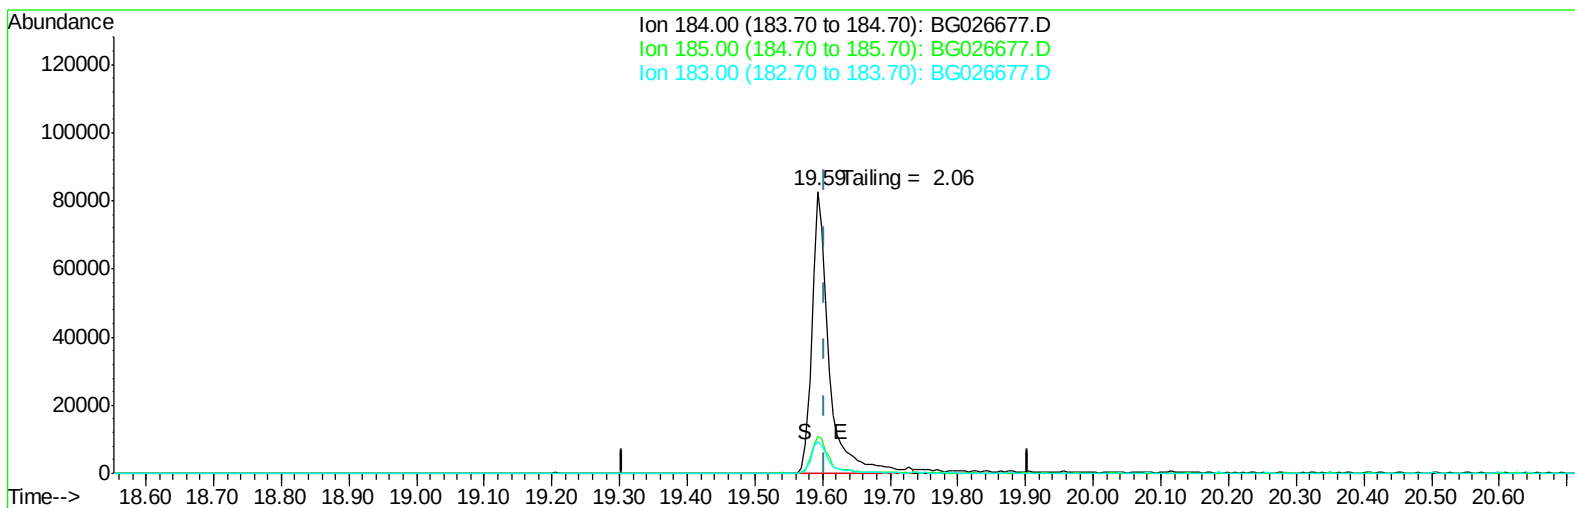

TIC: BG026677.D

(76) Benzidine



19.593min (-0.011) 82471.46ng

response 145410

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.27
183.00	13.80	11.16
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA G\DATA\BG042017\  
Data File : BG026677.D  
Acq On    : 20 Apr 2017  15:26  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Apr 21 05:19:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

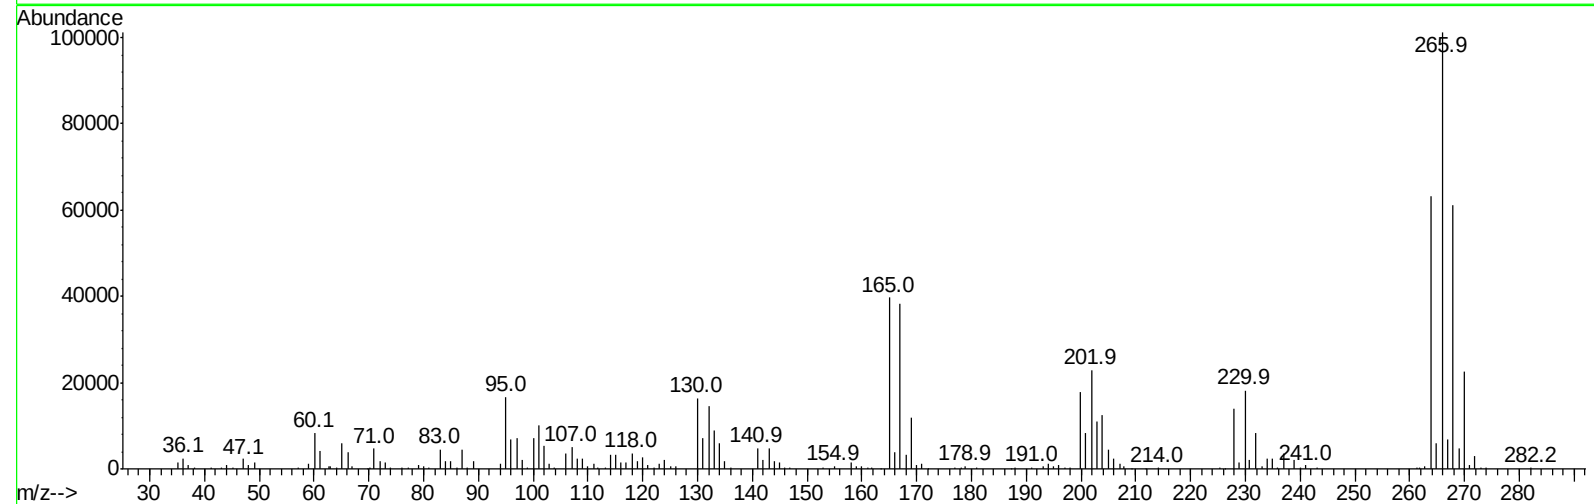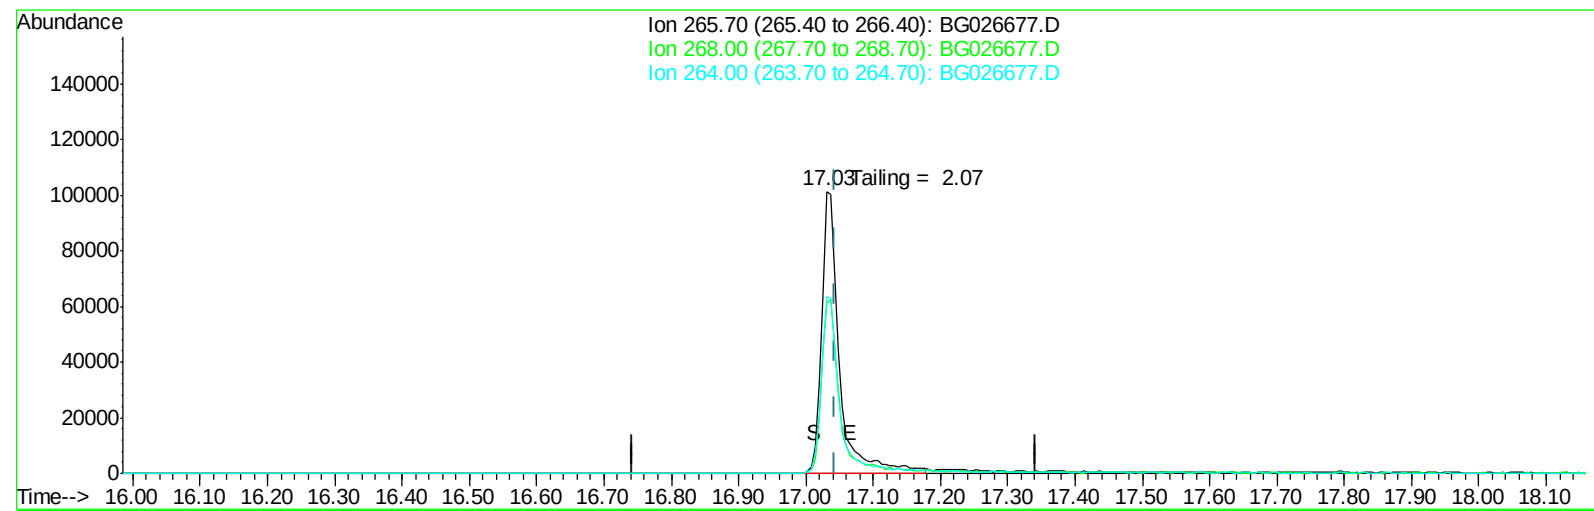

TIC: BG026677.D

(69) Pentachlorophenol (C)

17.031min (-0.012) 0.00ng

response 188667

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	60.53
264.00	62.60	62.52
0.00	0.00	0.00