
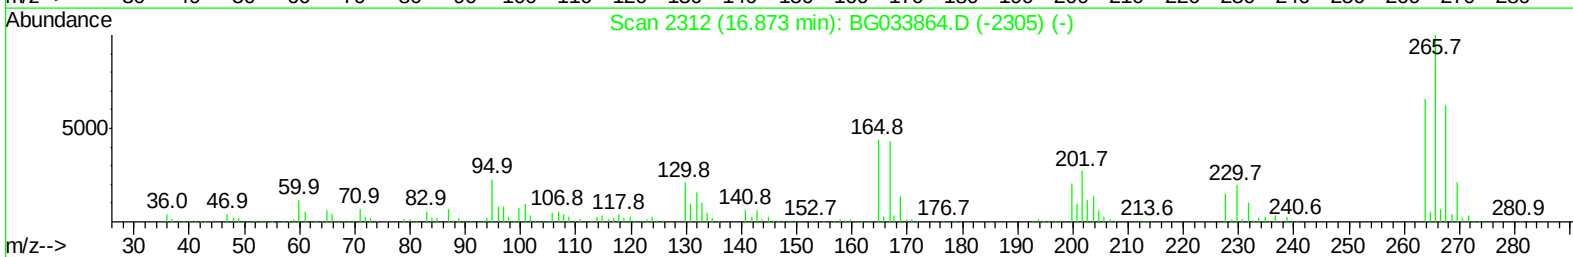
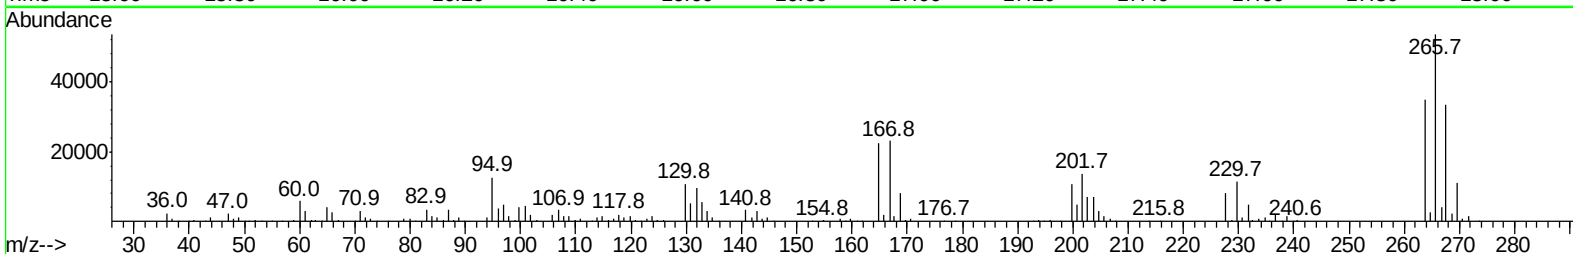


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042018\
Data File : BG033880.D
Acq On : 20 Apr 2018 10:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 03:42:49 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

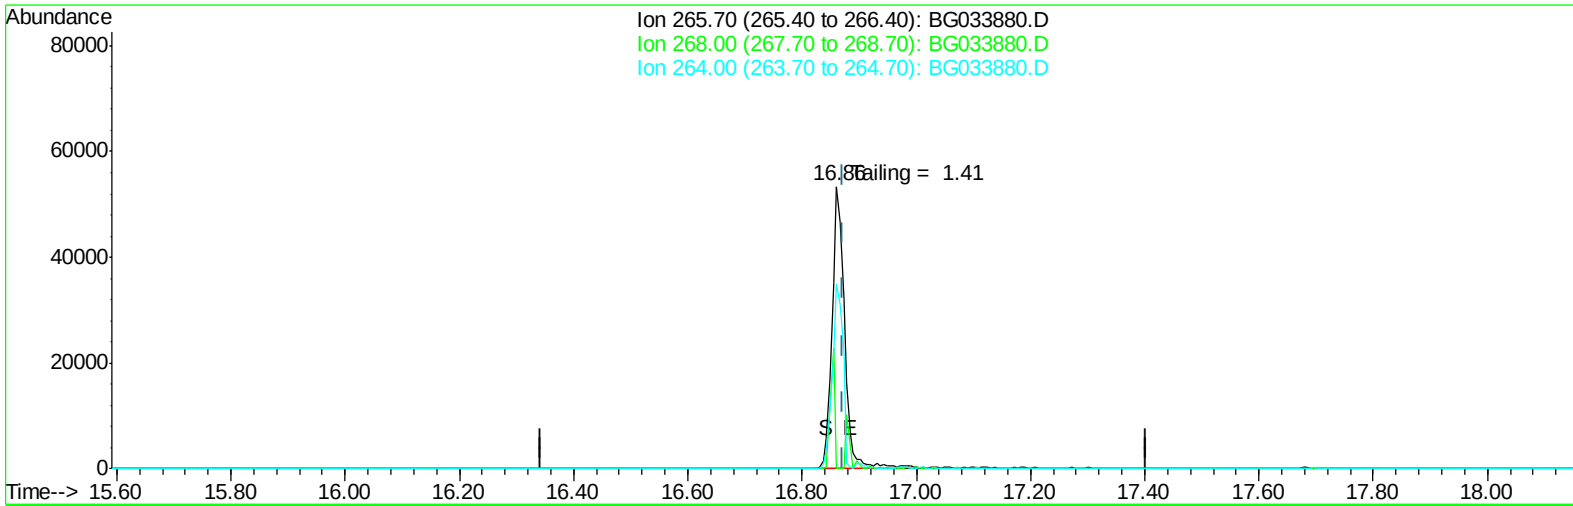

TIC: BG033880.D

(69) Pentachlorophenol (C)




16.861min (-0.012) 46061.49ng

response 78558

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	4.74#
264.00	62.00	70.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042018\
 Data File : BG033880.D
 Acq On : 20 Apr 2018 10:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 03:42:49 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

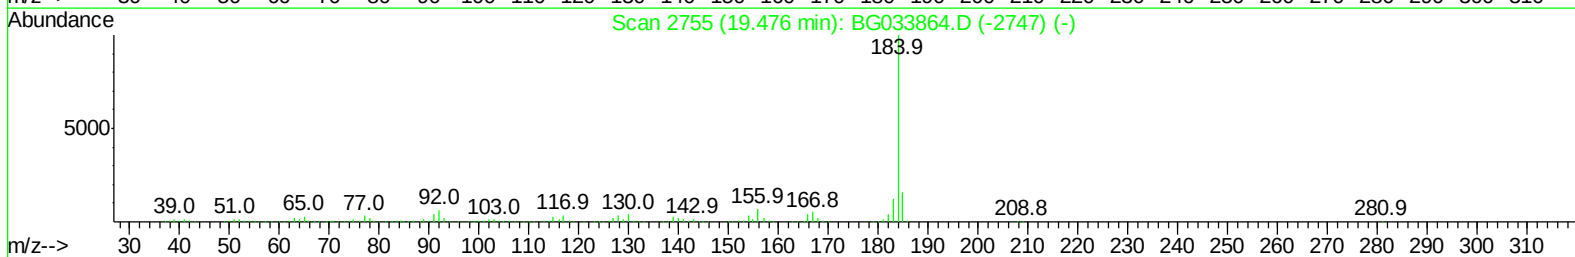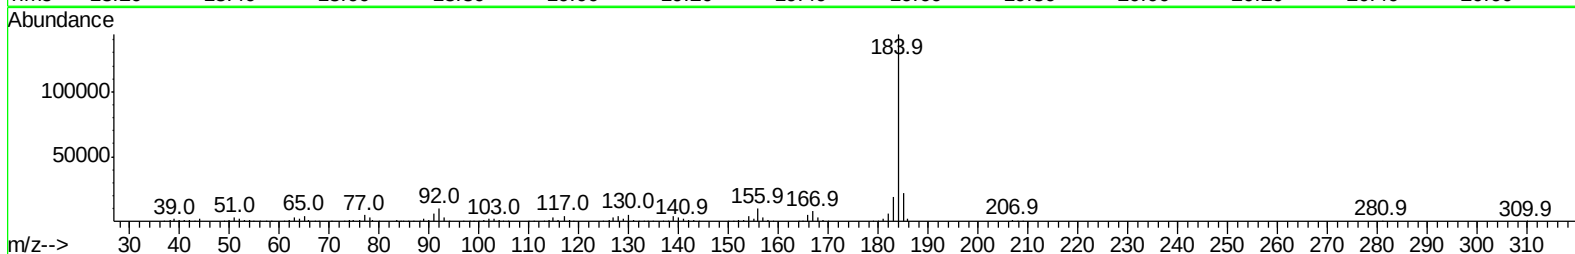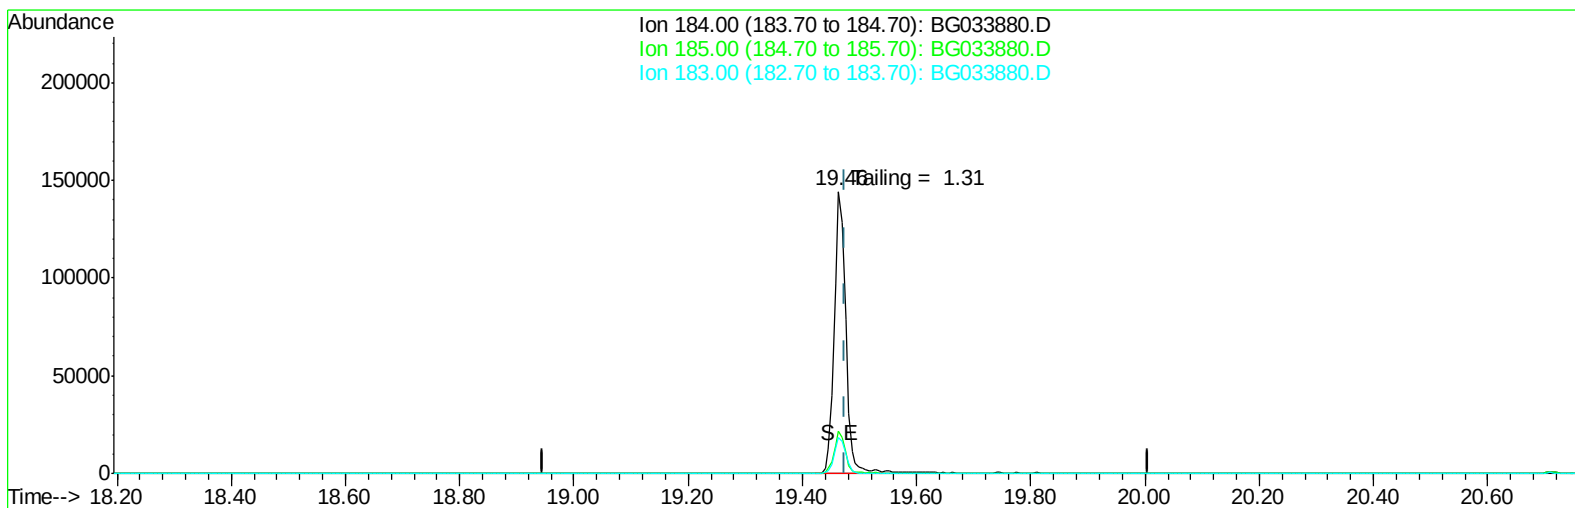

TIC: BG033880.D

(76) Benzidine

19.463min (-0.012) 0.00ng

response 200704

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.17
183.00	13.30	12.87
0.00	0.00	0.00