
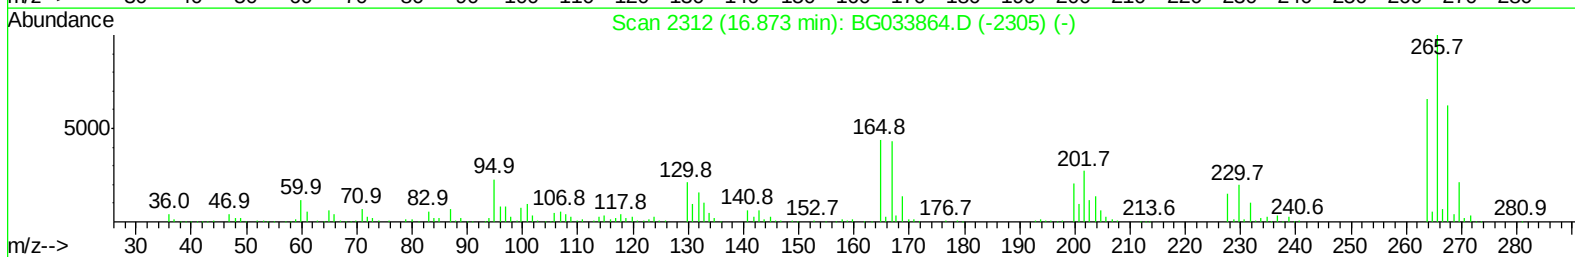
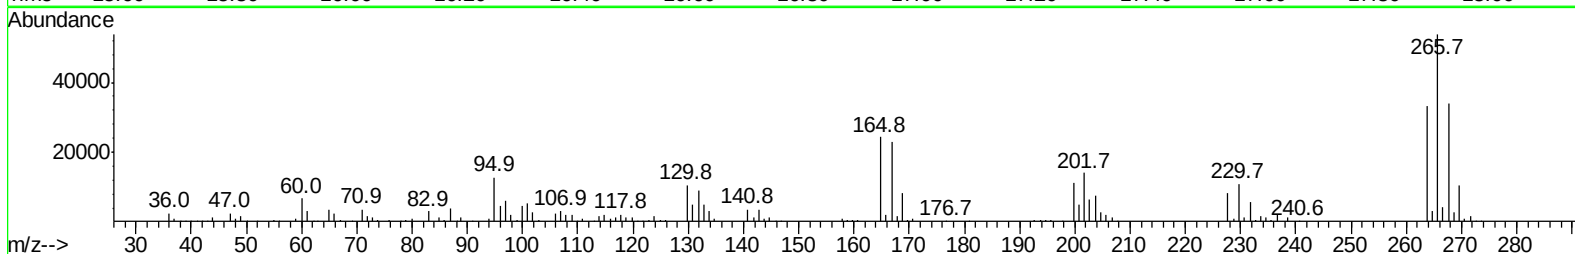


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042018\
Data File : BG033896.D
Acq On : 20 Apr 2018 22:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 03:44:00 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

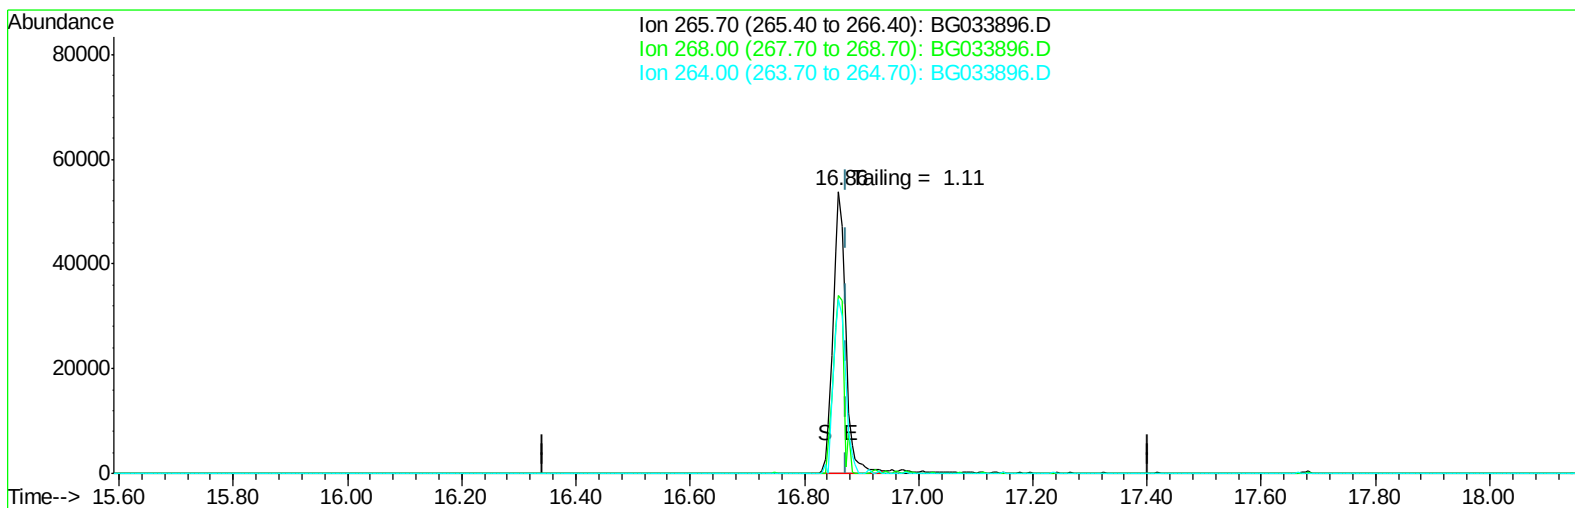

TIC: BG033896.D

(69) Pentachlorophenol (C)




16.860min (-0.013) 28129.48ng

response 82372

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.52
264.00	62.00	67.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042018\
Data File : BG033896.D
Acq On : 20 Apr 2018 22:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 03:44:00 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

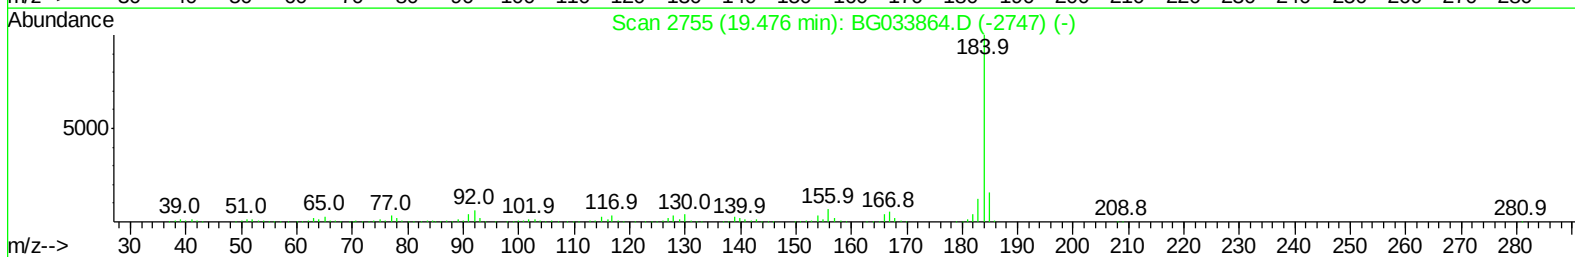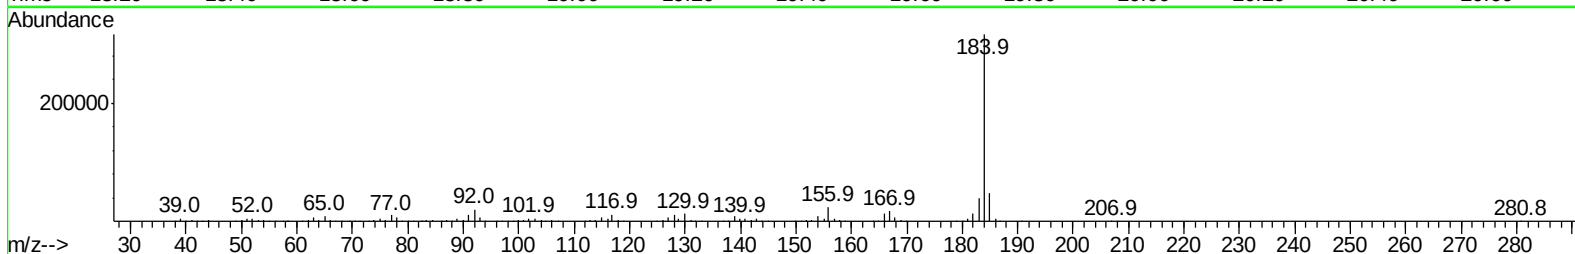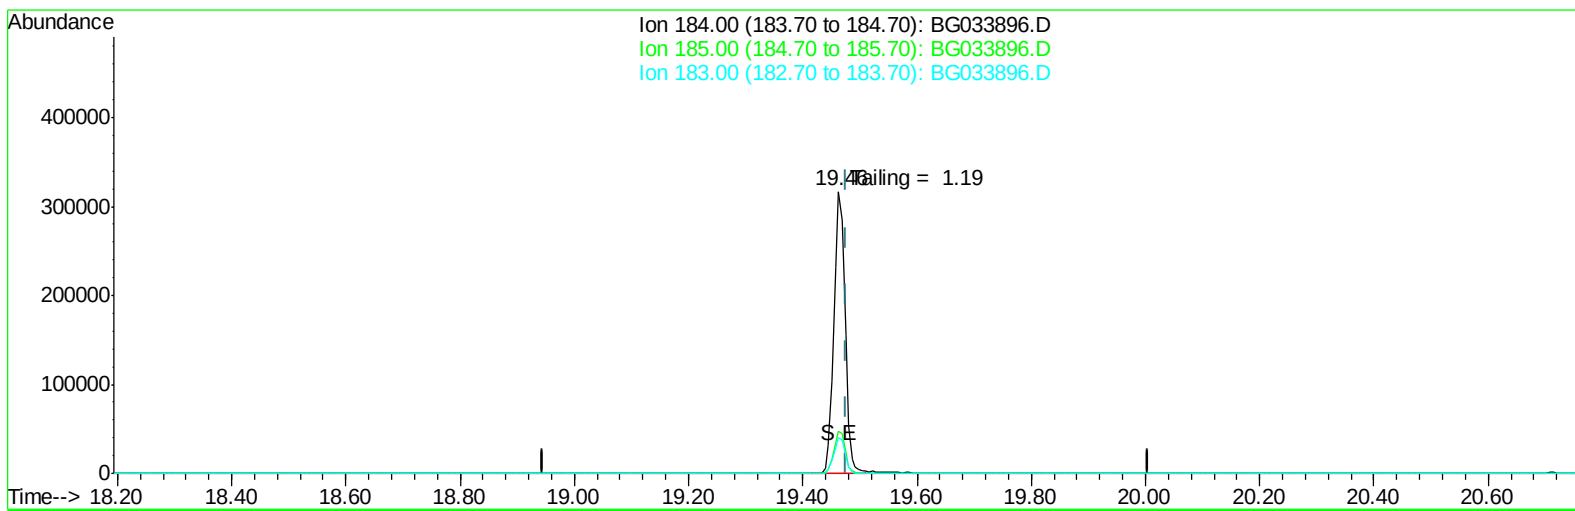

TIC: BG033896.D

(76) Benzidine

19.463min (-0.013) 0.00ng

response 432750

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.04
183.00	13.30	12.72
0.00	0.00	0.00