


Data Path : Z:\HPCHEM1\BNA G\Data\BG042018\
 Data File : BG033896.D
 Acq On : 20 Apr 2018 22:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

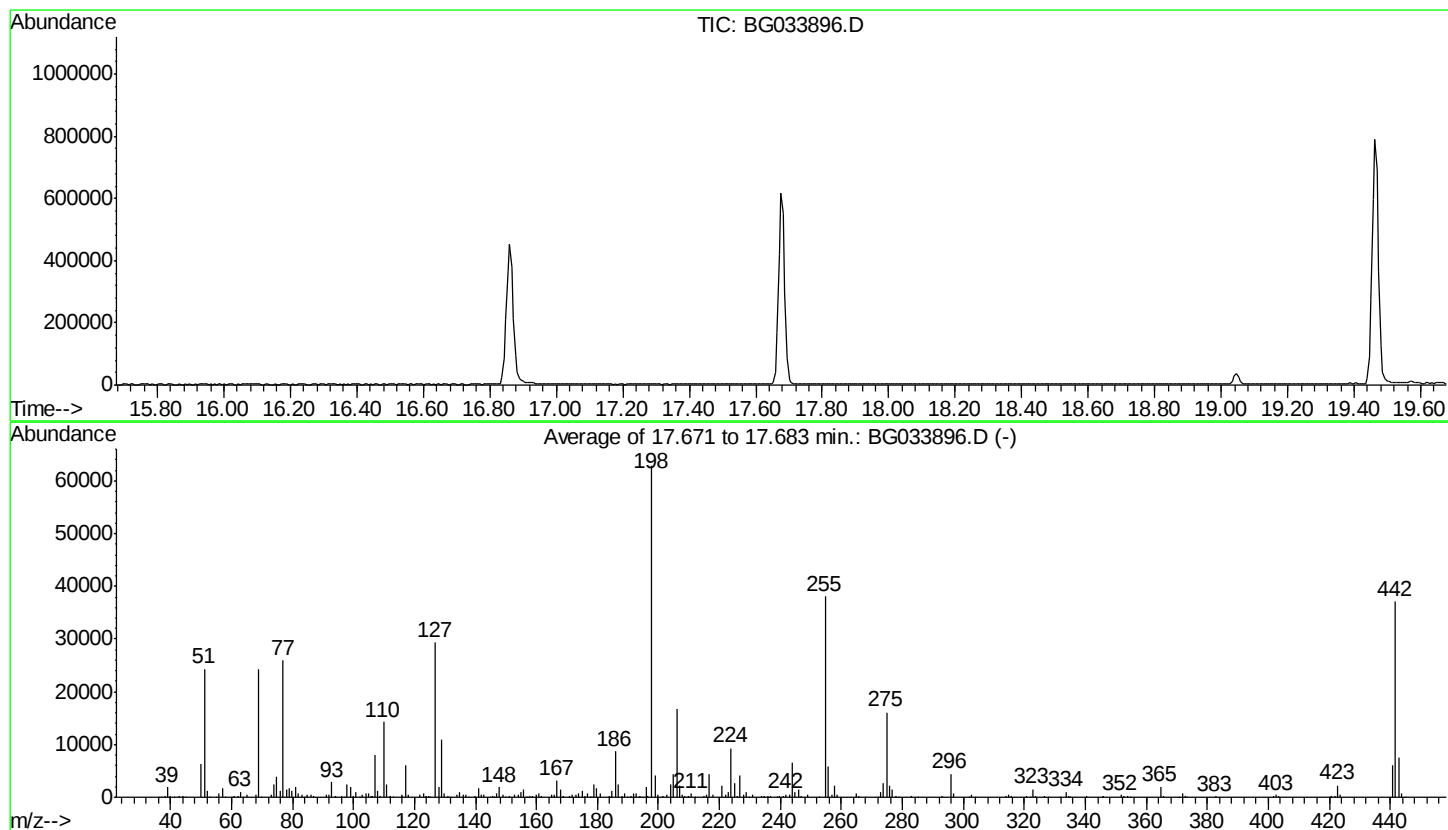

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	24376	PASS
68	69	0.00	2	1.6	392	PASS
69	198	0.00	100	38.6	24282	PASS
70	69	0.00	2	0.5	116	PASS
127	198	10	80	46.6	29280	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62896	PASS
199	198	5	9	6.6	4135	PASS
275	198	10	60	25.6	16108	PASS
365	198	1	100	3.3	2062	PASS
441	443	0.01	100	81.0	6182	PASS
442	198	50	100	58.9	37069	PASS
443	442	15	24	20.6	7631	PASS