
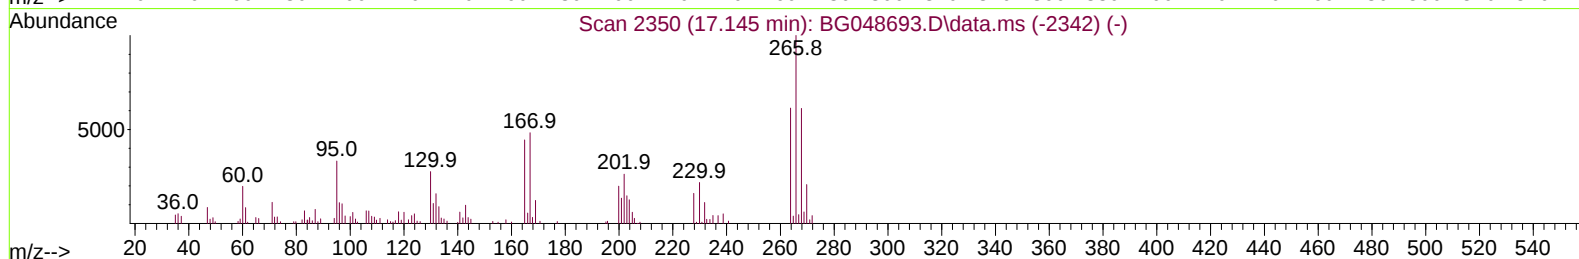
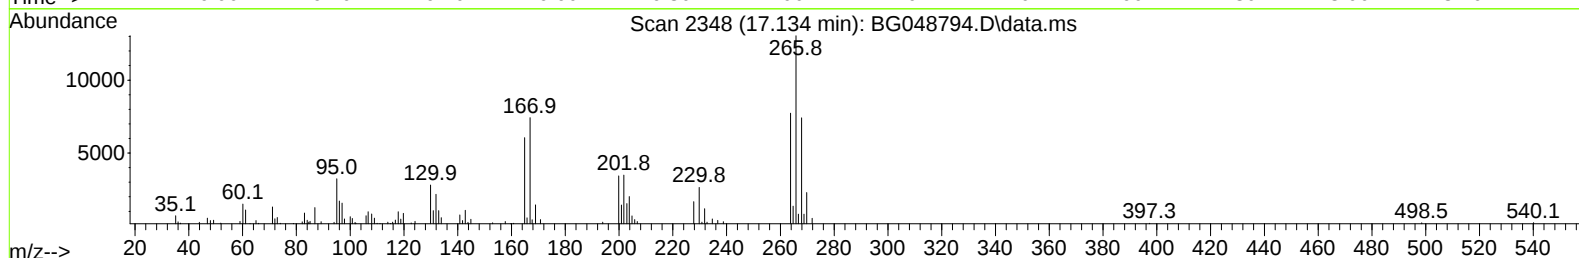


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042021\
Data File : BG048794.D
Acq On : 20 Apr 2021 14:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:57:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

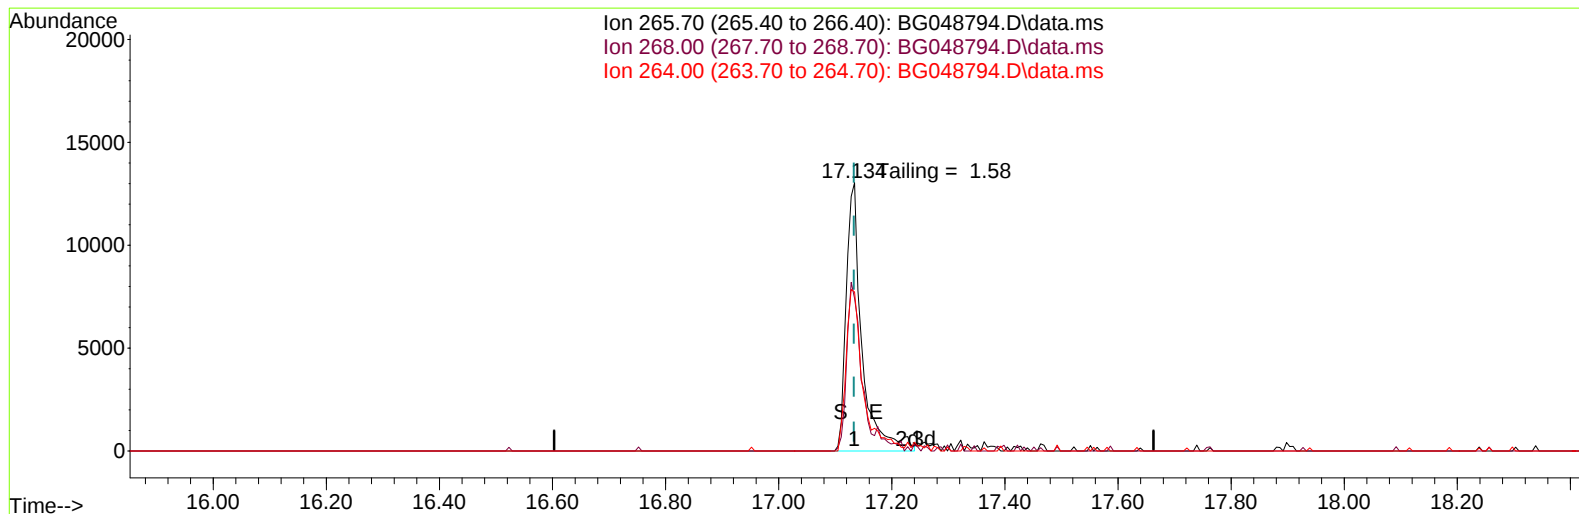

TIC: BG048794.D\data.ms

(70) Pentachlorophenol (C)




17.134min (+ 0.001) 0.00 ng

response 24516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	56.86
264.00	61.30	69.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042021\
 Data File : BG048794.D
 Acq On : 20 Apr 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 05:57:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

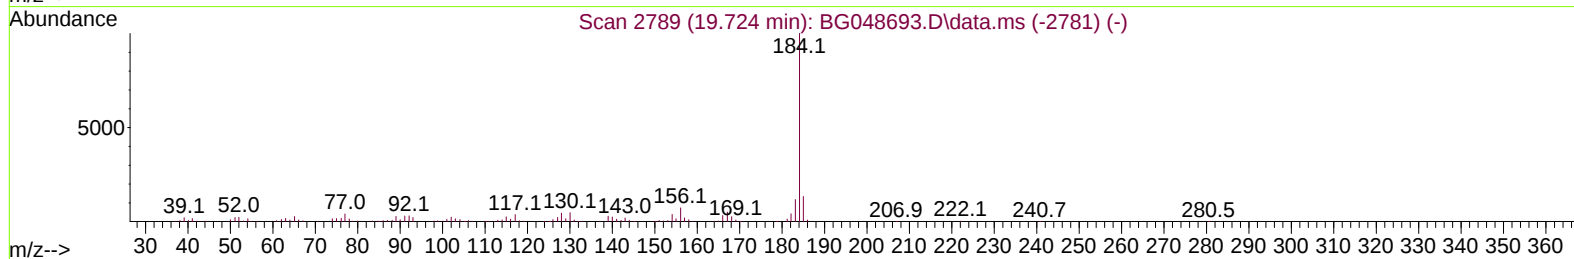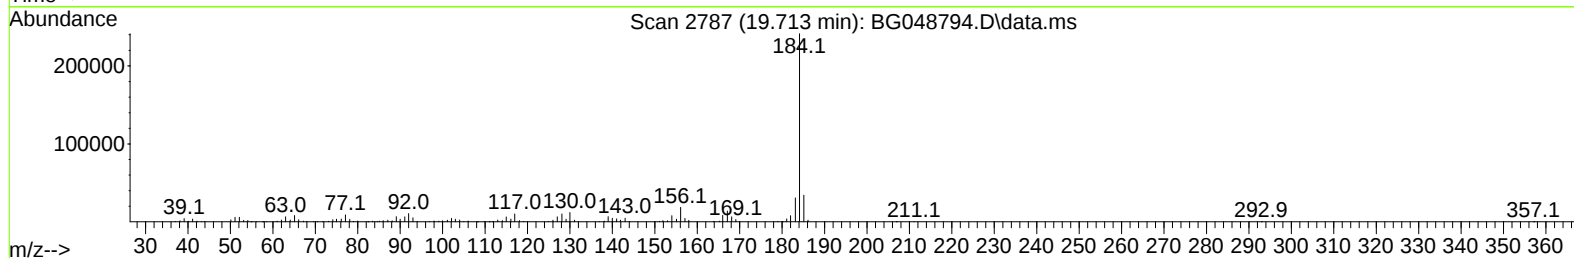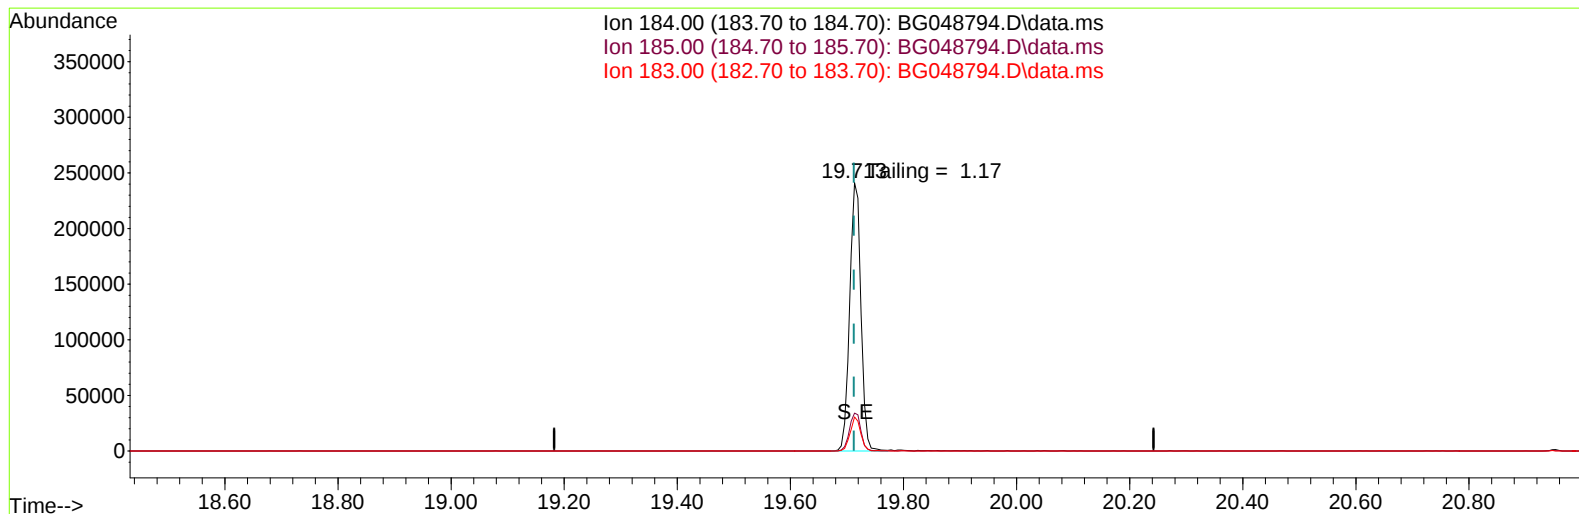

TIC: BG048794.D\data.ms

(77) Benzidine**19.713min (+ 0.001) 53874.62 ng****response 332109**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.16
183.00	11.70	12.71
0.00	0.00	0.00