
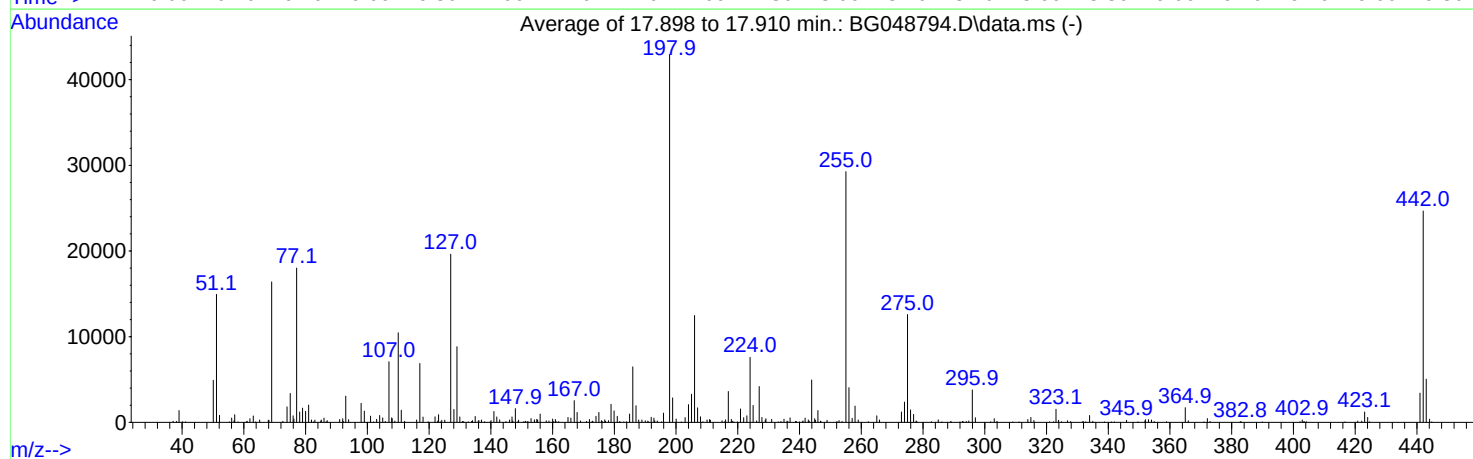


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042021\
 Data File : BG048794.D
 Acq On : 20 Apr 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 17:33:30 2021

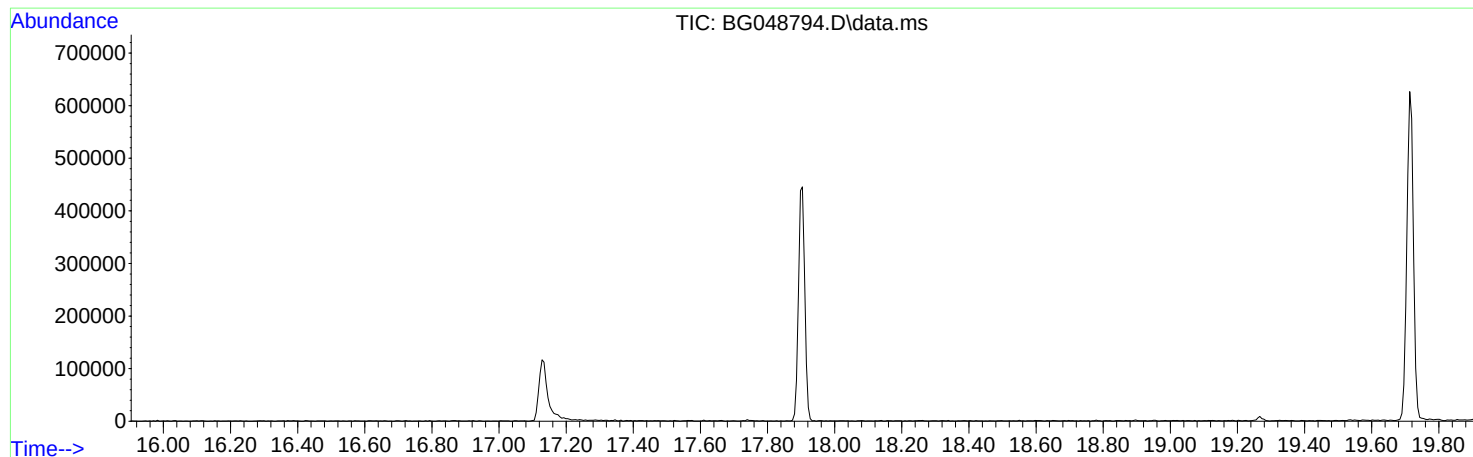


AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	14934	PASS
68	69	0.00	2	1.6	263	PASS
69	198	0.00	100	38.2	16408	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	19639	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42939	PASS
199	198	5	9	6.6	2855	PASS
275	198	10	60	29.3	12584	PASS
365	198	1	100	4.0	1727	PASS
441	198	0.01	100	7.9	3410	PASS
442	198	50	100	57.5	24680	PASS
443	442	15	24	20.4	5045	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042021\
Data File : BG048794.D
Acq On : 20 Apr 2021 14:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 21 05:57:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

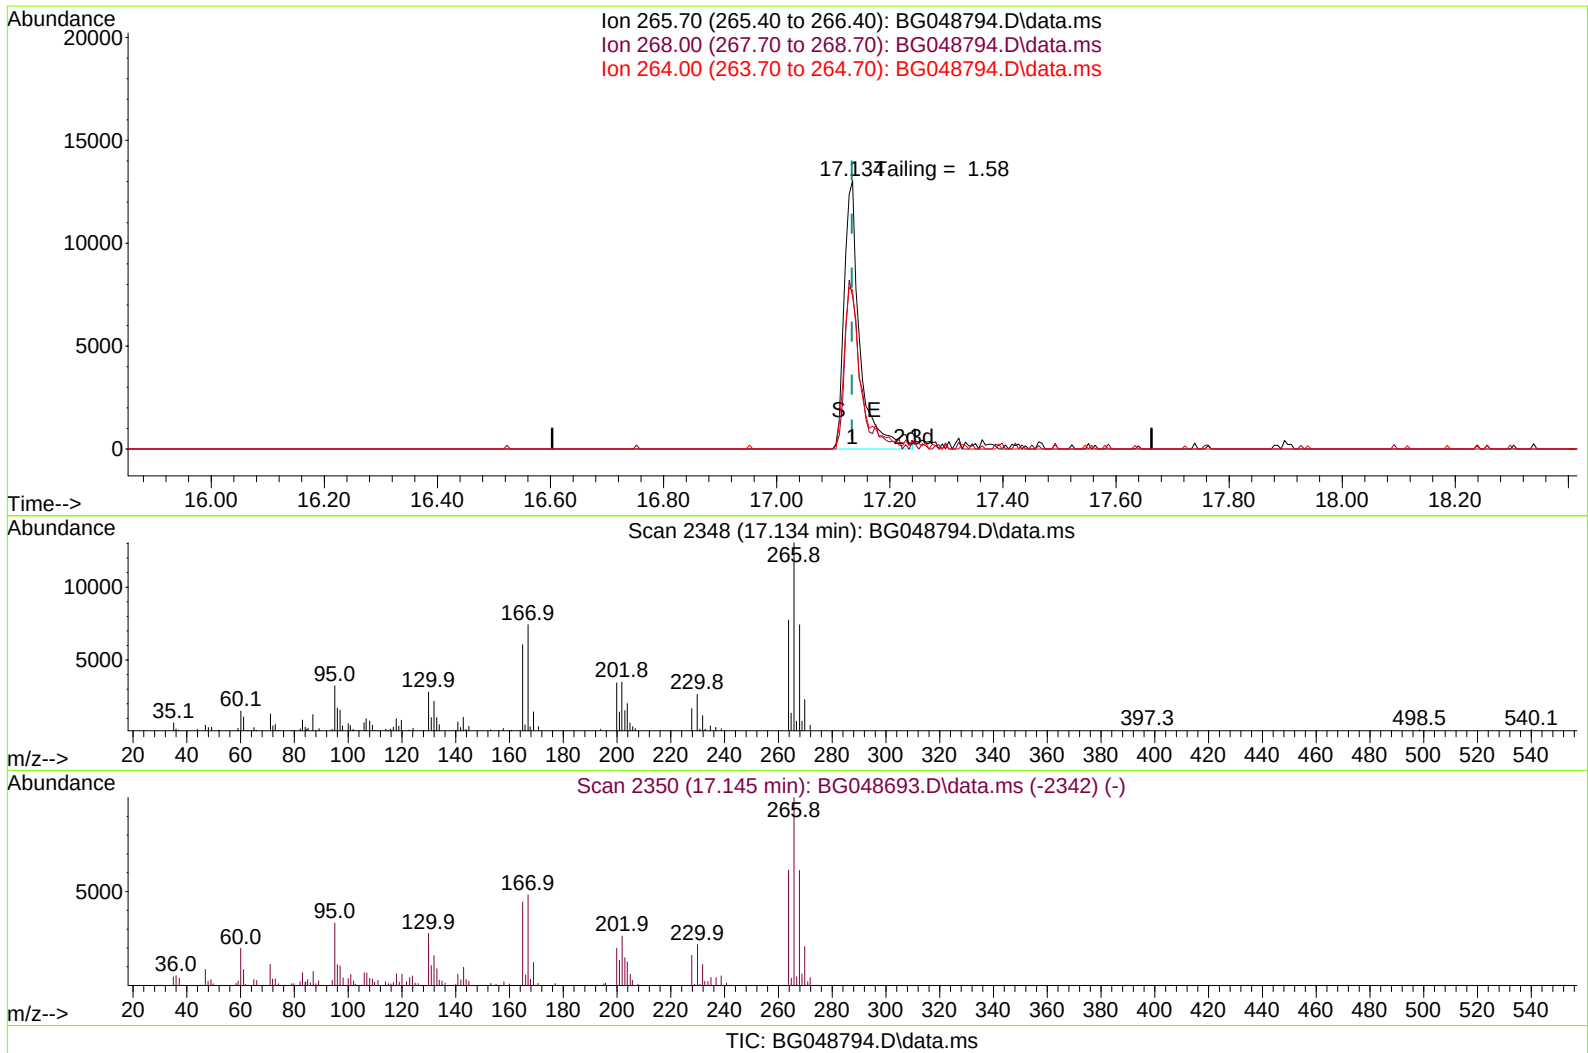

(70) Pentachlorophenol (C)

17.134min (+ 0.001) 0.00 ng




response 24516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	56.86
264.00	61.30	69.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042021\
 Data File : BG048794.D
 Acq On : 20 Apr 2021 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 05:57:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

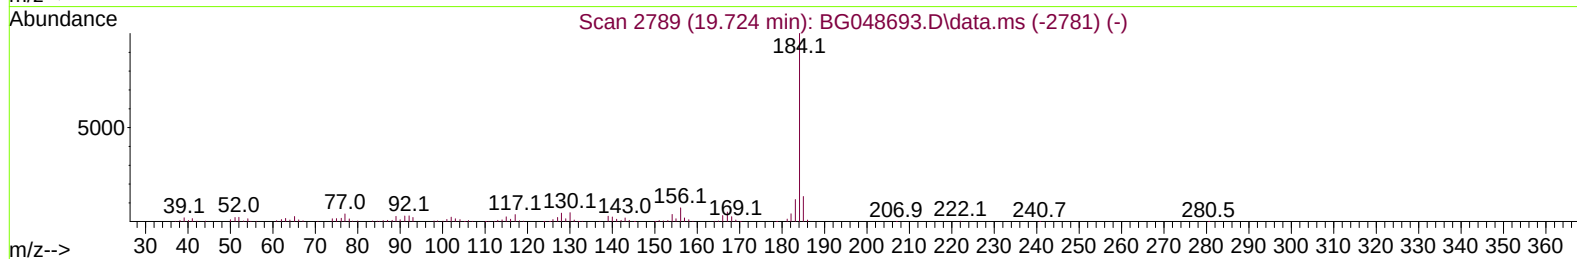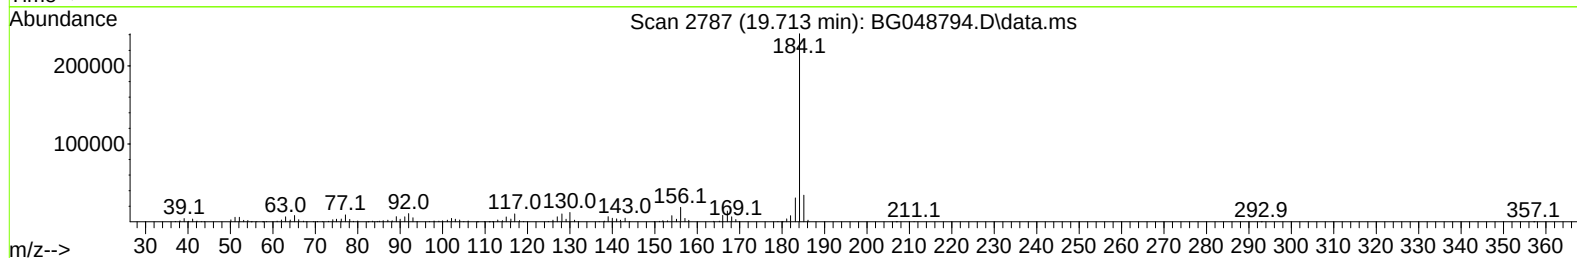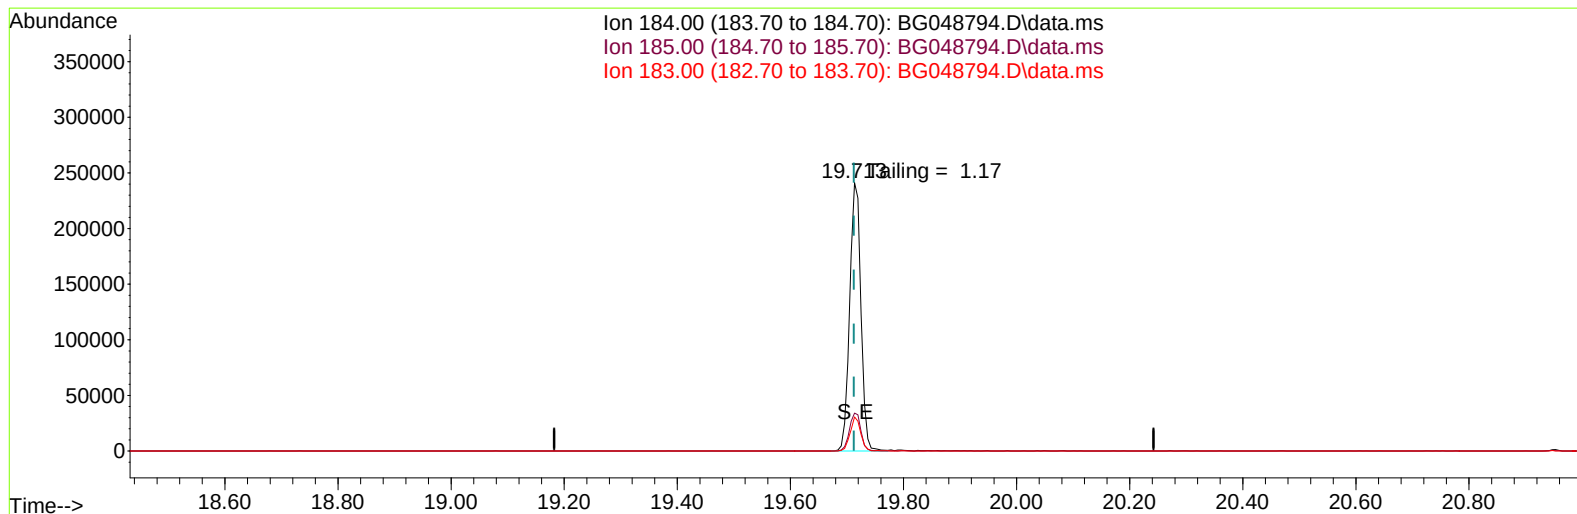

TIC: BG048794.D\data.ms

(77) Benzidine

19.713min (+ 0.001) 53874.62 ng

response 332109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.16
183.00	11.70	12.71
0.00	0.00	0.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/20/2021	BNA_G	<u>BG048794.D</u>
Compound Name	Response	Retention Time
DDT	167420	20.947
DDD	4103	20.501
DDE	476	20.001
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4579	171999	2.66

Instrument :
BNA_G
ClientSampleId :
DFTPP