


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042023\
Data File : BG057140.D
Acq On : 20 Apr 2023 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 21 05:53:40 2023

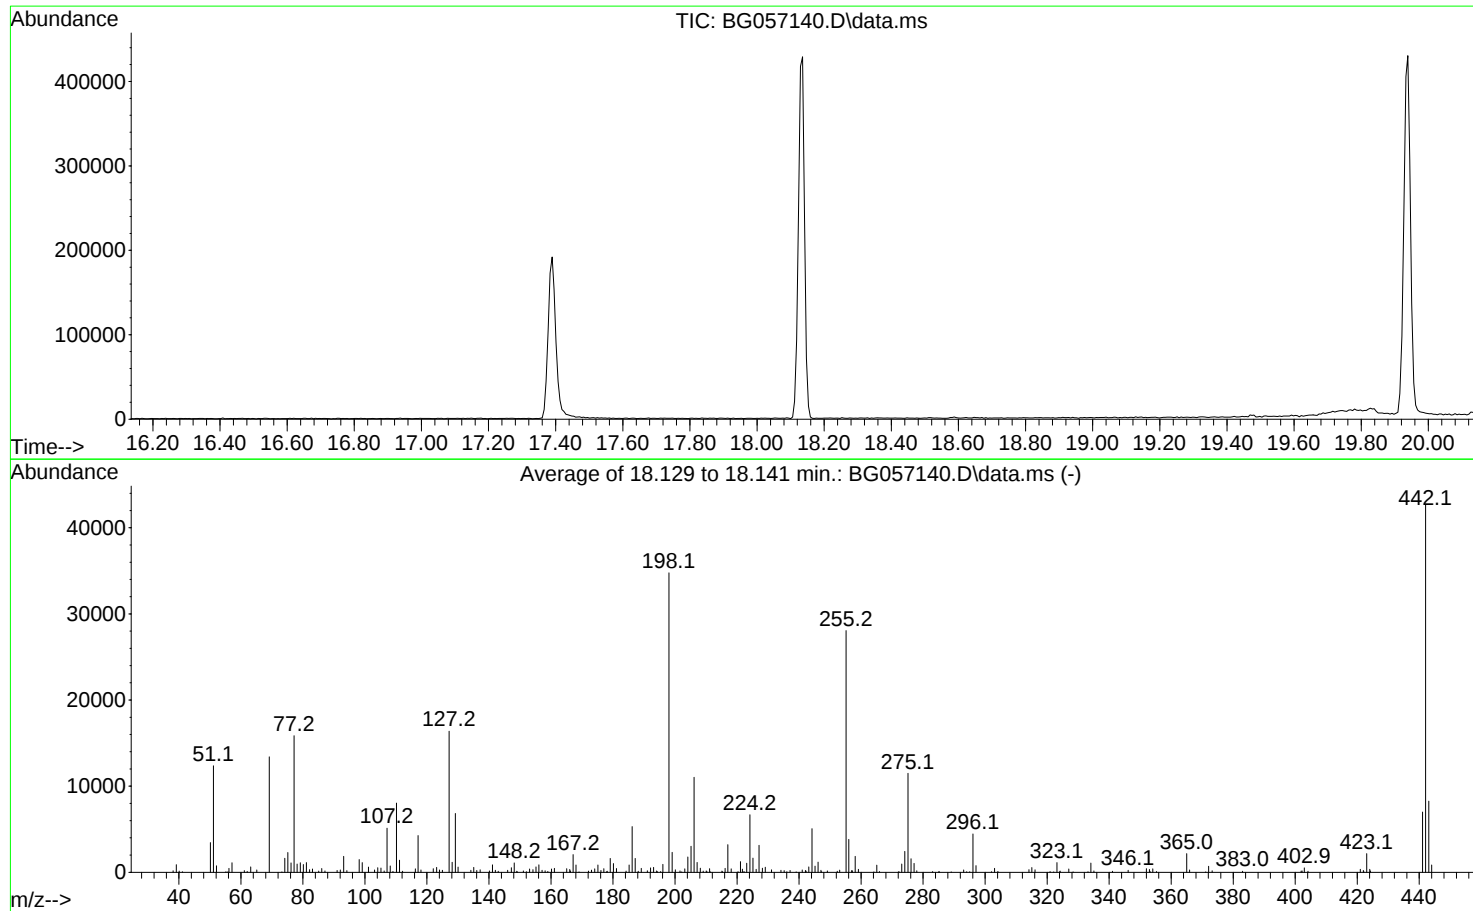

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	12358	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	13410	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	16379	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34760	PASS
199	198	5	9	6.6	2310	PASS
275	198	10	60	33.0	11484	PASS
365	198	1	100	6.2	2164	PASS
441	198	0.01	100	20.1	6996	PASS
442	442	50	100	100.0	42707	PASS
443	442	15	24	19.3	8251	PASS