
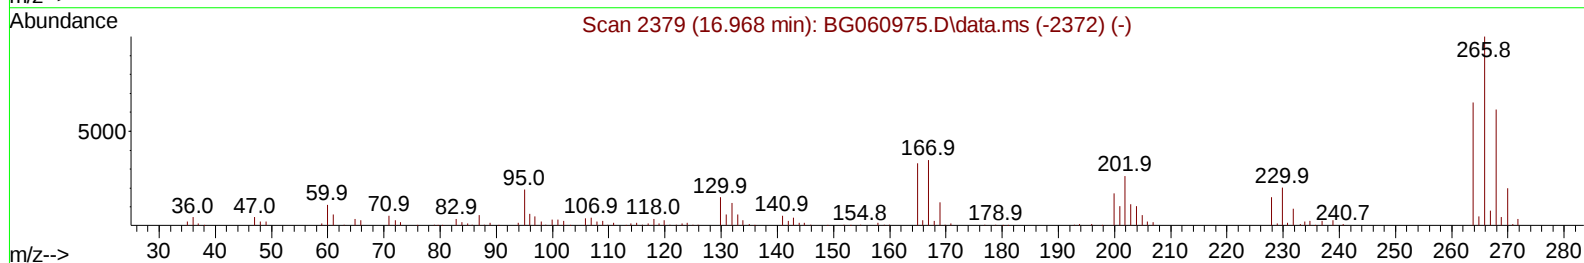
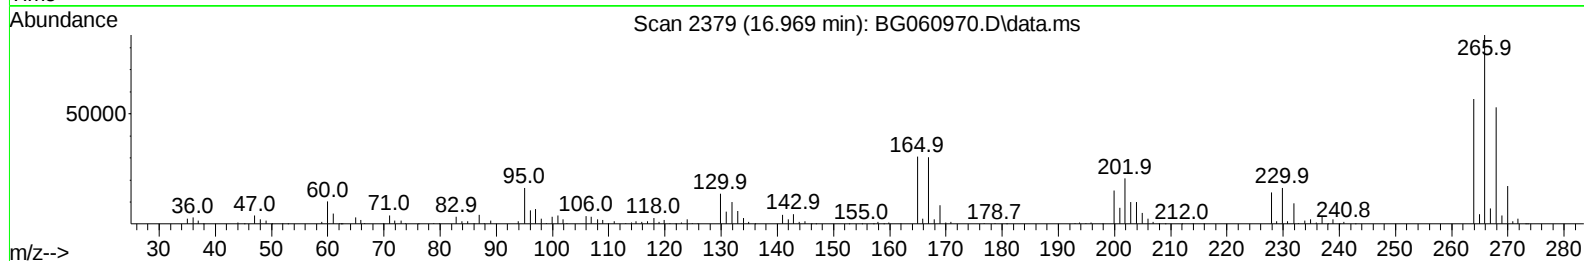


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042024\
Data File : BG060970.D
Acq On : 20 Apr 2024 16:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 04:29:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

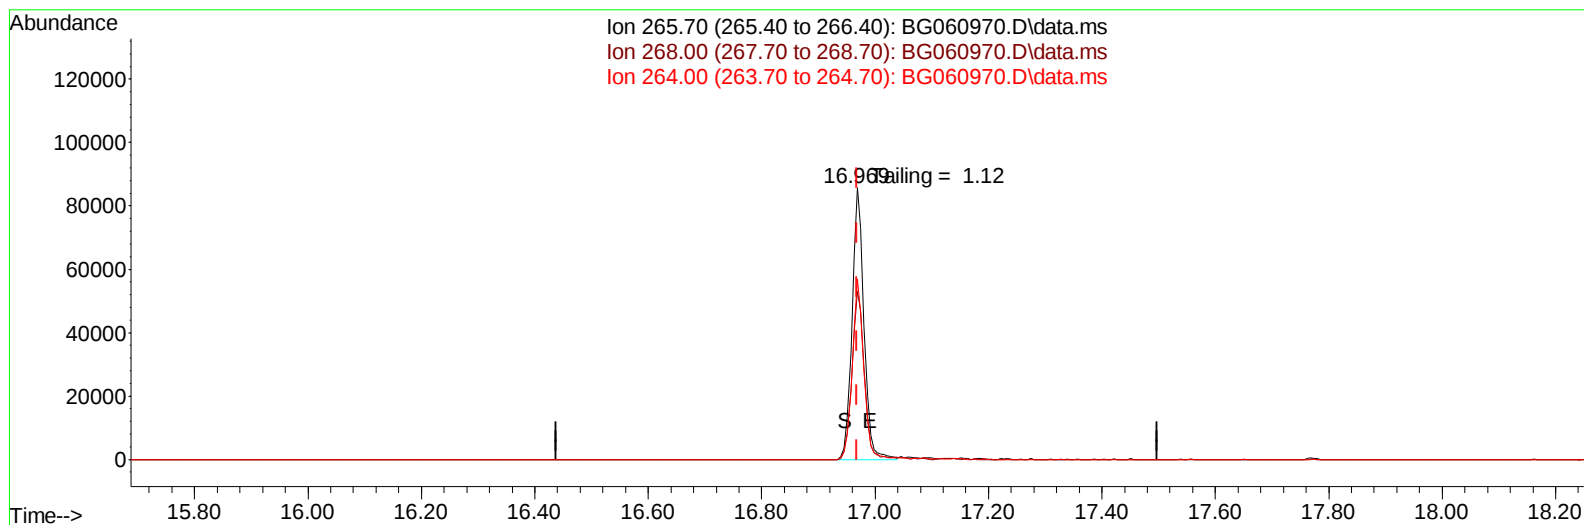




TIC: BG060970.D\data.ms

(70) Pentachlorophenol (C)**16.969min (+ 0.001) 52131.00 ng****response 125576**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	61.80
264.00	65.20	66.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042024\
Data File : BG060970.D
Acq On : 20 Apr 2024 16:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 04:29:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

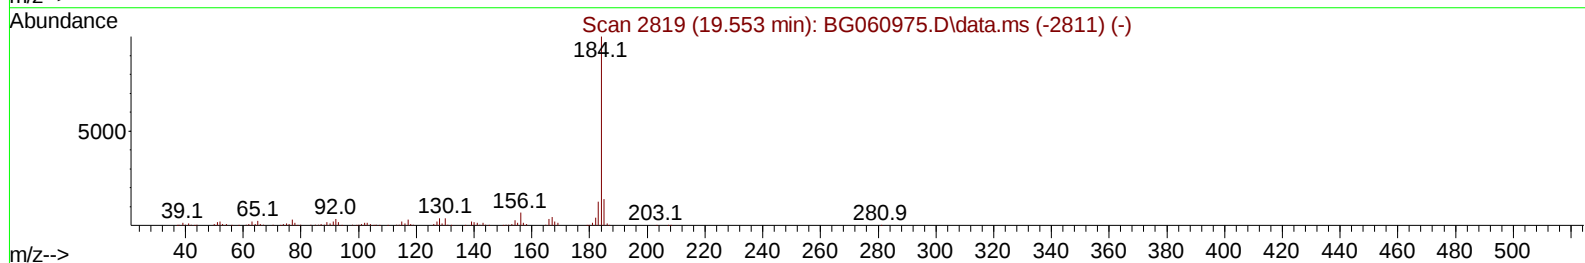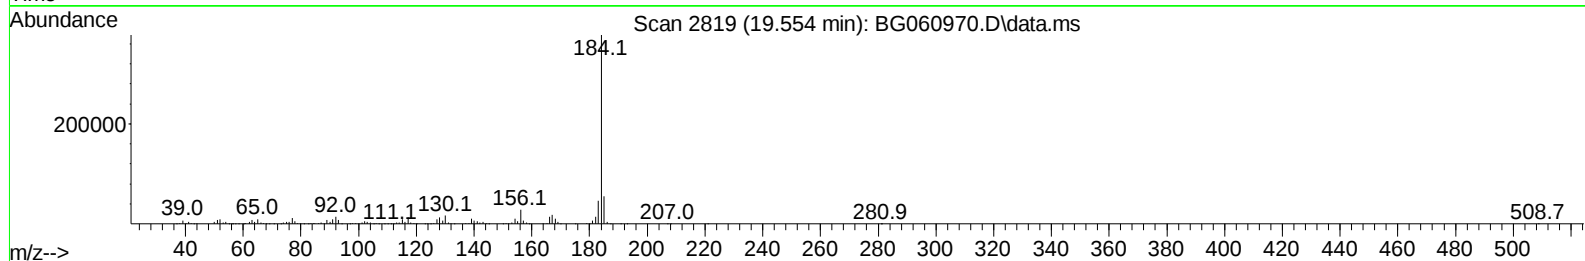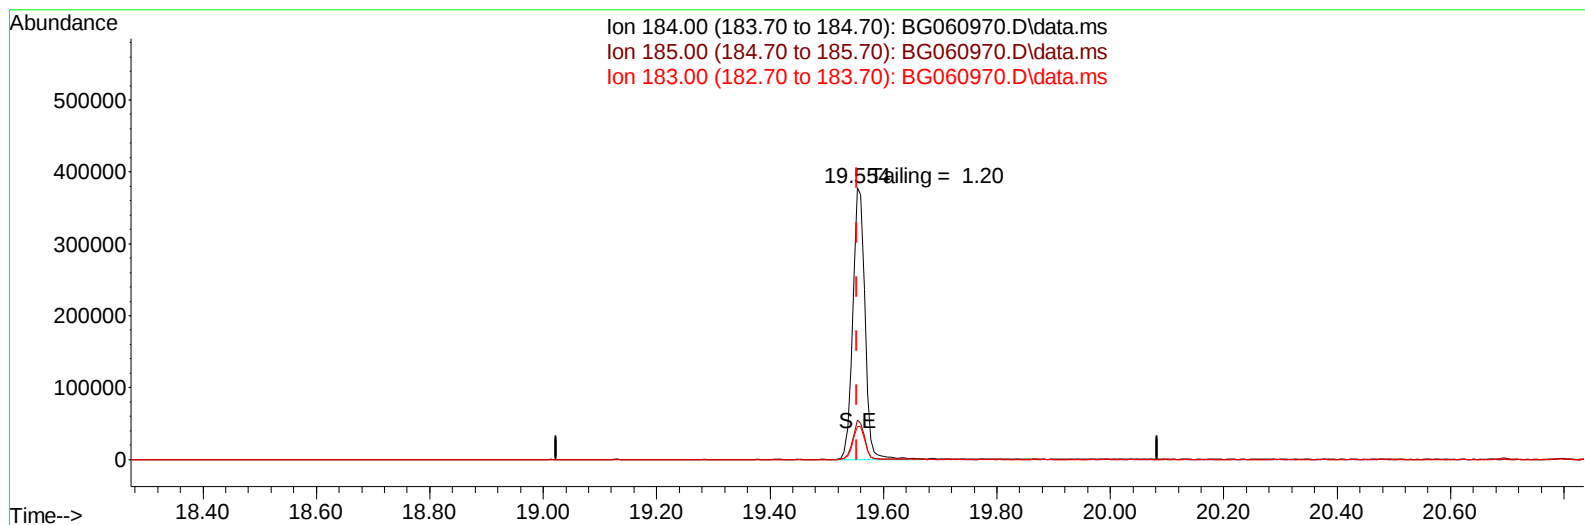

TIC: BG060970.D\data.ms

(77) Benzidine**19.554min (+ 0.001) 29601.97 ng****response 562204**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.49
183.00	12.70	12.18
0.00	0.00	0.00