
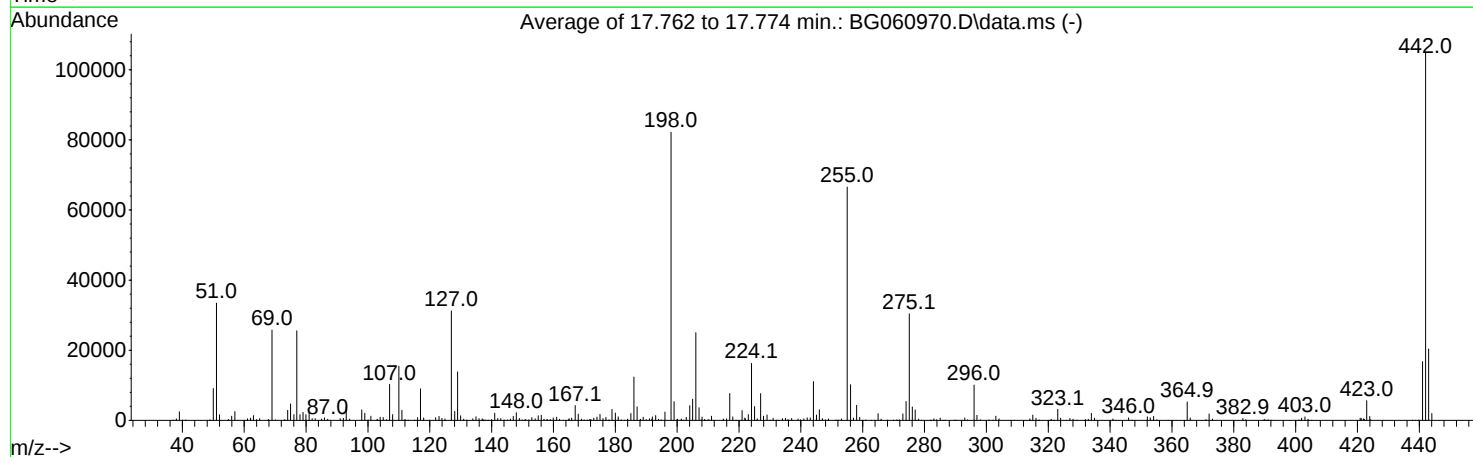


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG042024\  
Data File : BG060970.D  
Acq On : 20 Apr 2024 16:11  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Mon Apr 22 04:22:00 2024

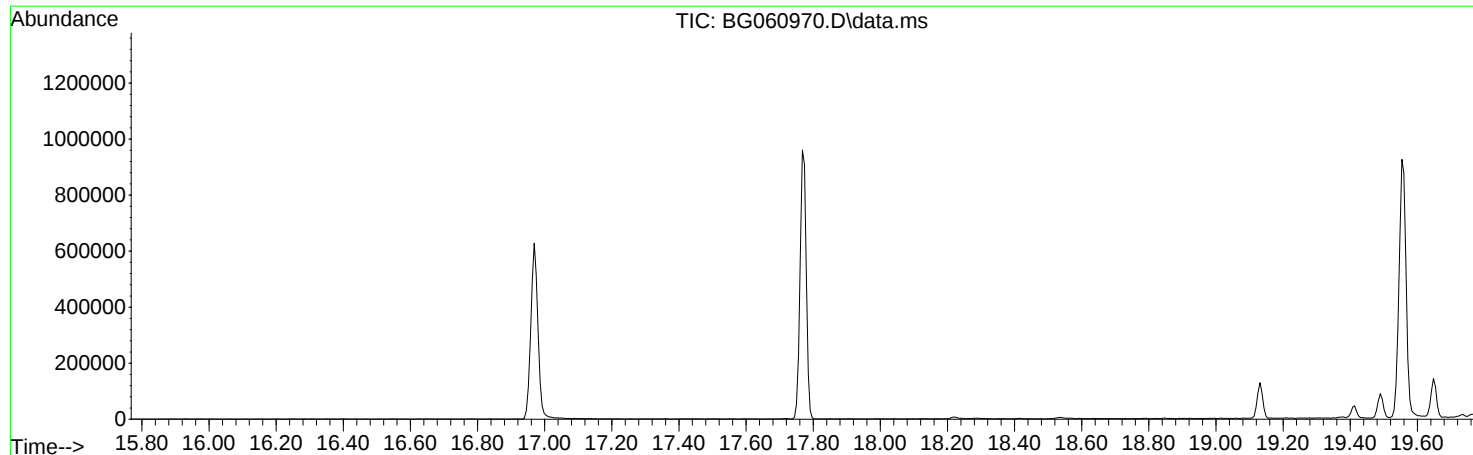




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.7         | 33453      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.0          | 247        | PASS                |
| 69             | 198             | 0.00            | 100             | 31.4         | 25813      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 123        | PASS                |
| 127            | 198             | 10              | 80              | 38.0         | 31229      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 82208      | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 5347       | PASS                |
| 275            | 198             | 10              | 60              | 37.0         | 30421      | PASS                |
| 365            | 198             | 1               | 100             | 6.4          | 5274       | PASS                |
| 441            | 198             | 0.01            | 100             | 20.4         | 16758      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 104936     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 20336      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG042024\  
Data File : BG060970.D  
Acq On : 20 Apr 2024 16:11  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Apr 22 04:29:29 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 22 04:22:00 2024  
Response via : Initial Calibration

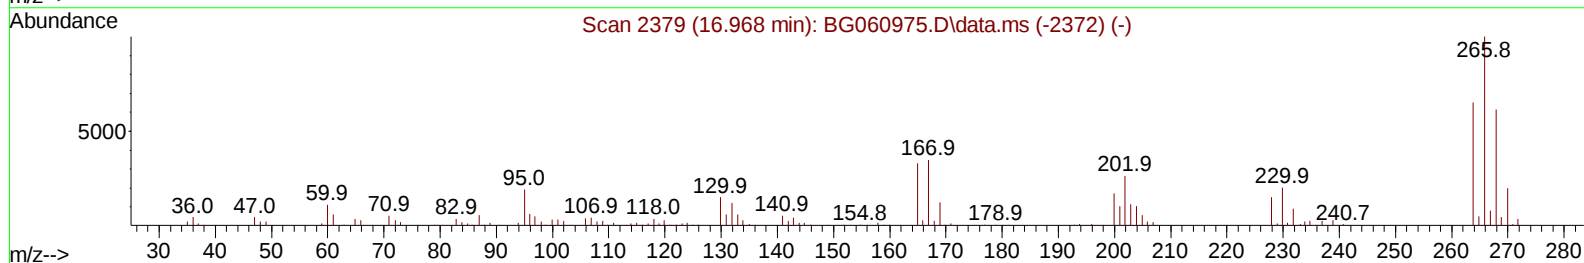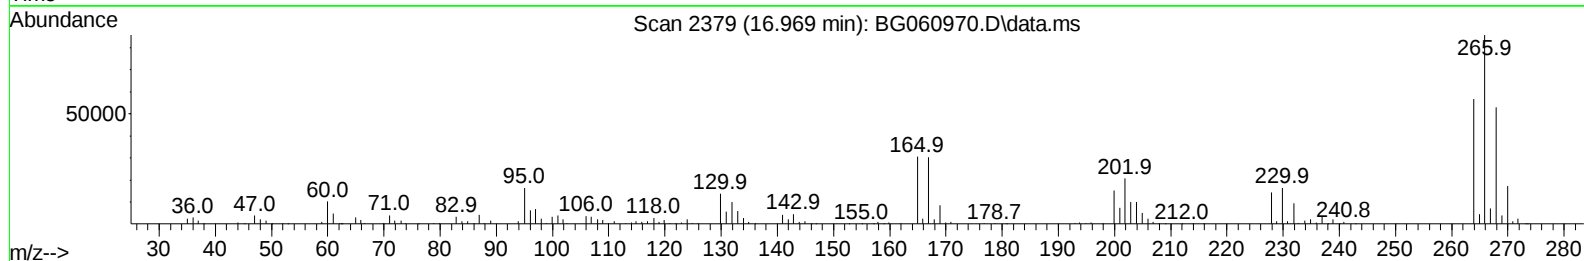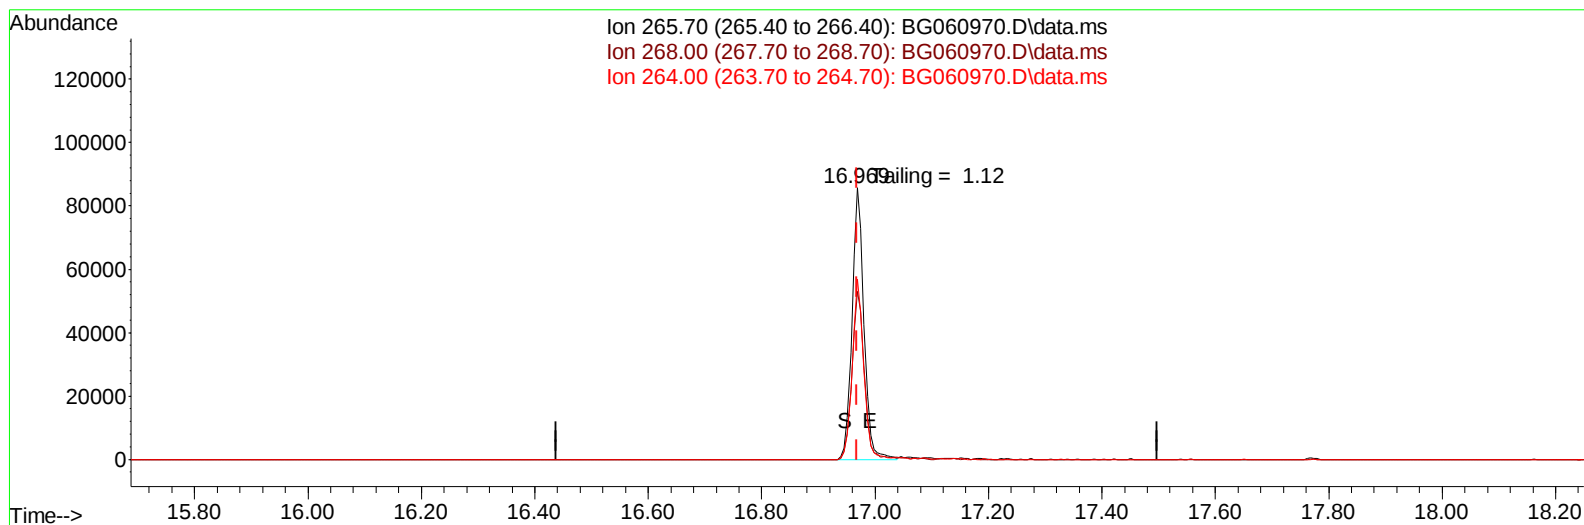

TIC: BG060970.D\data.ms

(70) Pentachlorophenol (C)

16.969min (+ 0.001) 52131.00 ng




response 125576

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.40  | 61.80  |
| 264.00 | 65.20  | 66.33  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG042024\  
Data File : BG060970.D  
Acq On : 20 Apr 2024 16:11  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Apr 22 04:29:29 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 22 04:22:00 2024  
Response via : Initial Calibration

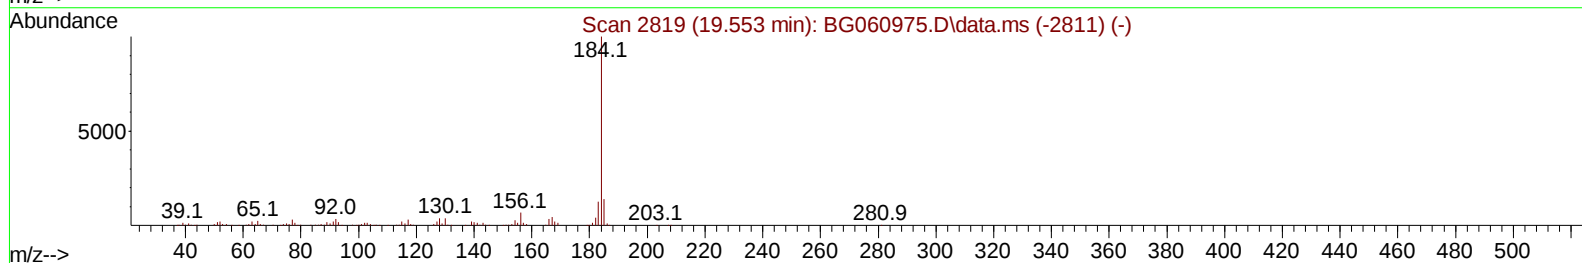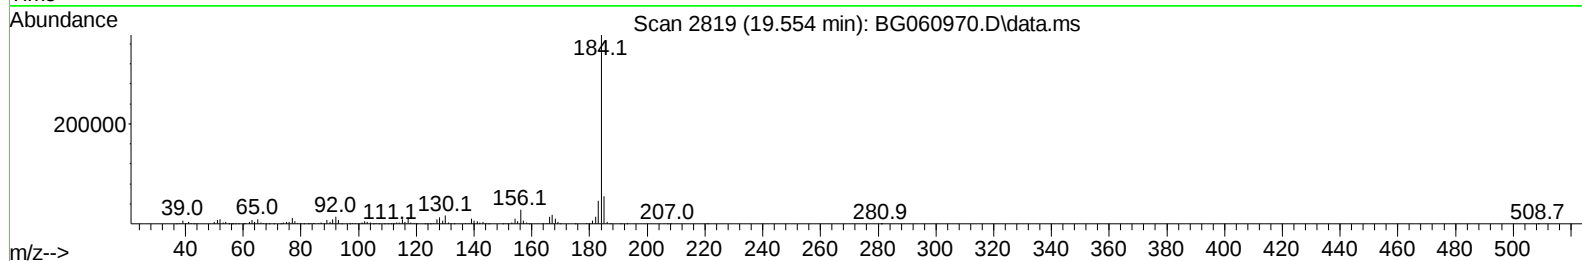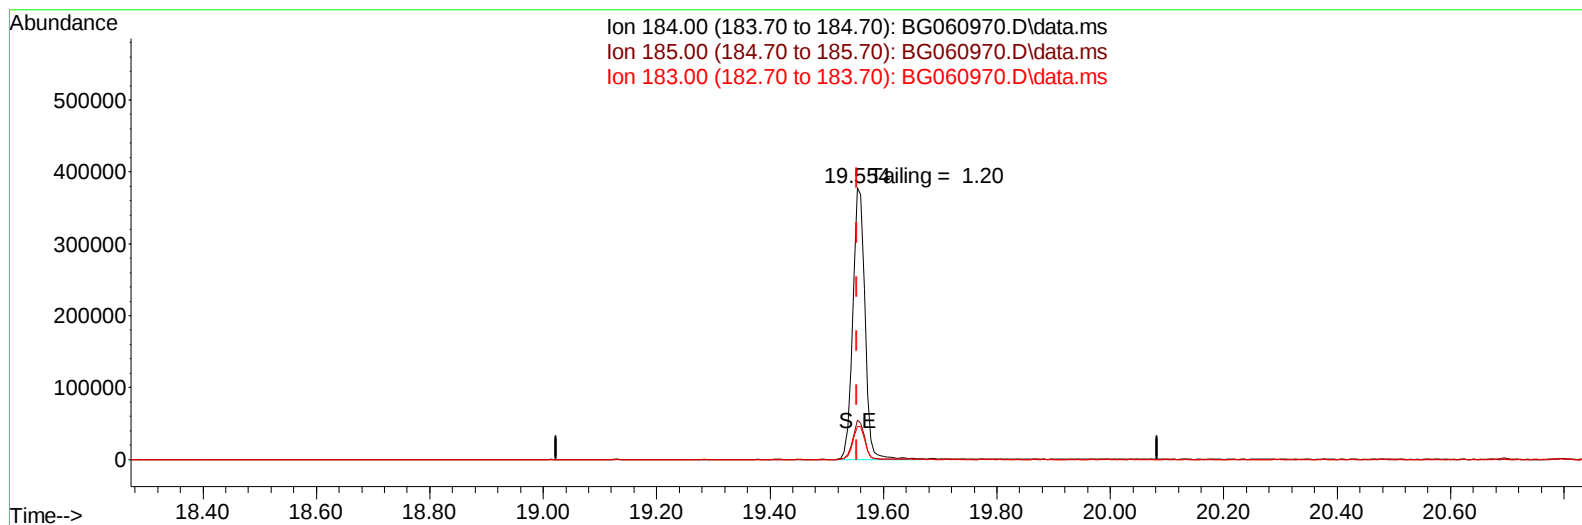

TIC: BG060970.D\data.ms

(77) Benzidine

19.554min (+ 0.001) 29601.97 ng

response 562204

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.49  |
| 183.00 | 12.70  | 12.18  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/20/2024     | BNA_G            | <u>BG060970.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 347219           | 20.794             |
| DDD           | 12177            | 20.353             |
| DDE           | 586              | 19.848             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 12763         | 359982           | 3.55               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP