

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
 Data File : BG016602.D
 Acq On : 22 Apr 2015 3:21
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Quant Time: Apr 22 04:21:51 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 22 02:10:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	47639	20.00	ng	0.00
21) Naphthalene-d8	10.42	136	221151	20.00	ng	0.00
38) Acenaphthene-d10	14.28	164	131840	20.00	ng	0.00
63) Phenanthrene-d10	17.02	188	305343	20.00	ng	0.00
75) Chrysene-d12	21.21	240	297504	20.00	ng	0.00
86) Perylene-d12	23.42	264	279583	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.22	112	243603	81.96	ng	0.00
7) Phenol-d6	6.83	99	348952	84.03	ng	0.00
23) Nitrobenzene-d5	8.79	82	297531	82.84	ng	0.00
41) 2,4,6-Tribromophenol	15.77	330	81801	91.35	ng	0.00
44) 2-Fluorobiphenyl	12.90	172	639365	80.32	ng	0.00
78) Terphenyl-d14	19.65	244	1012663	82.00	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.10	88	54050	40.43	ng	97
3) Pyridine	3.50	79	155140	41.96	ng	99
4) n-Nitrosodimethylamine	3.42	42	45143	40.78	ng	99
6) Aniline	6.97	93	236947	41.31	ng	99
8) 2-Chlorophenol	7.20	128	147217	41.49	ng	98
9) Benzaldehyde	6.78	77	67089	35.50	ng	95
10) Phenol	6.85	94	183661	41.81	ng	97
11) bis(2-Chloroethyl)ether	7.07	93	138319	40.22	ng	100
12) 1,3-Dichlorobenzene	7.53	146	151160	40.80	ng	98
13) 1,4-Dichlorobenzene	7.67	146	154278	40.91	ng	97
14) 1,2-Dichlorobenzene	7.98	146	147301	41.06	ng	99
15) Benzyl Alcohol	7.88	79	110068	41.65	ng	97
16) 2,2'-oxybis(1-Chloropropan	8.17	45	134039	40.25	ng	98
17) 2-Methylphenol	8.10	107	124017	41.89	ng	97
18) Hexachloroethane	8.70	117	55168	40.74	ng	98
19) n-Nitroso-di-n-propylamine	8.44	70	110250	41.06	ng	97
20) 3+4-Methylphenols	8.42	107	171530	42.07	ng	99
22) Acetophenone	8.46	105	203603	41.33	ng	# 99
24) Nitrobenzene	8.84	77	155482	41.59	ng	99
25) Isophorone	9.35	82	304861	41.46	ng	99
26) 2-Nitrophenol	9.54	139	88129	42.70	ng	96
27) 2,4-Dimethylphenol	9.61	122	148410	42.29	ng	99
28) bis(2-Chloroethoxy)methane	9.84	93	182023	41.28	ng	98
29) 2,4-Dichlorophenol	10.08	162	123977	42.73	ng	98
30) 1,2,4-Trichlorobenzene	10.29	180	126631	41.04	ng	94
31) Naphthalene	10.47	128	474163	41.07	ng	99
32) Benzoic acid	9.78	122	34527	32.89	ng	92
33) 4-Chloroaniline	10.59	127	224003	42.43	ng	99
34) Hexachlorobutadiene	10.75	225	55978	40.83	ng	96
35) Caprolactam	11.36	113	74910	44.58	ng	97
36) 4-Chloro-3-methylphenol	11.73	107	149307	42.61	ng	96
37) 2-Methylnaphthalene	12.09	142	342671	41.46	ng	99
39) 1,2,4,5-Tetrachlorobenzene	12.46	216	121963	40.21	ng	99
40) Hexachlorocyclopentadiene	12.44	237	35948	38.90	ng	94

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
 Data File : BG016602.D
 Acq On : 22 Apr 2015 3:21
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Quant Time: Apr 22 04:21:51 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 22 02:10:07 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) 2,4,6-Trichlorophenol	12.71	196	89123	41.50	ng	97
43) 2,4,5-Trichlorophenol	12.79	196	96005	41.93	ng	97
45) 1,1'-Biphenyl	13.11	154	411423	40.52	ng	99
46) 2-Chloronaphthalene	13.15	162	315302	40.55	ng	99
47) 2-Nitroaniline	13.37	65	100694	44.39	ng	94
48) Acenaphthylene	14.00	152	577425	41.83	ng	99
49) Dimethylphthalate	13.75	163	414539	42.52	ng	99
50) 2,6-Dinitrotoluene	13.86	165	103888	43.39	ng	97
51) Acenaphthene	14.35	154	339149	41.17	ng	99
52) 3-Nitroaniline	14.20	138	136262	46.08	ng	99
53) 2,4-Dinitrophenol	14.41	184	35979	37.39	ng	98
54) Dibenzofuran	14.68	168	482372	41.60	ng	100
55) 4-Nitrophenol	14.53	139	103690	46.33	ng	98
56) 2,4-Dinitrotoluene	14.66	165	153270	46.52	ng	97
57) Fluorene	15.33	166	434580	42.53	ng	100
58) 2,3,4,6-Tetrachlorophenol	14.92	232	77490	44.85	ng	98
59) Diethylphthalate	15.11	149	447744	43.11	ng	100
60) 4-Chlorophenyl-phenylether	15.33	204	173583	41.37	ng	97
61) 4-Nitroaniline	15.36	138	163090	48.14	ng	97
62) Azobenzene	15.62	77	417759	43.34	ng	97
64) 4,6-Dinitro-2-methylphenol	15.42	198	80364	39.08	ng	99
65) n-Nitrosodiphenylamine	15.55	169	409201	39.97	ng	99
66) 4-Bromophenyl-phenylether	16.22	248	96032	39.95	ng	97
67) Hexachlorobenzene	16.33	284	100660	40.09	ng	96
68) Atrazine	16.50	200	120035	41.94	ng	99
69) Pentachlorophenol	16.68	266	44604	37.87	ng	98
70) Phenanthrene	17.07	178	709544	40.82	ng	99
71) Anthracene	17.15	178	720612	41.72	ng	99
72) Carbazole	17.43	167	756923	42.95	ng	99
73) Di-n-butylphthalate	18.00	149	918518	42.83	ng	100
74) Fluoranthene	19.08	202	795104	42.46	ng	98
76) Benzidine	19.28	184	456324	41.48	ng	99
77) Pyrene	19.45	202	822798	41.18	ng	100
79) Butylbenzylphthalate	20.35	149	443061	42.36	ng	99
80) Benzo(a)anthracene	21.19	228	725234	40.42	ng	100
81) 3,3'-Dichlorobenzidine	21.13	252	243568	41.01	ng	97
82) Chrysene	21.24	228	694527	40.32	ng	99
83) Bis(2-ethylhexyl)phthalate	21.12	149	604797	42.12	ng	99
84) Di-n-octyl phthalate	21.98	149	1002823	42.06	ng	100
85) Indeno(1,2,3-cd)pyrene	25.68	276	781354	41.34	ng	99
87) Benzo(b)fluoranthene	22.75	252	689129	41.31	ng	99
88) Benzo(k)fluoranthene	22.80	252	683104	41.74	ng	99
89) Benzo(a)pyrene	23.33	252	651393	41.13	ng	99
90) Dibenzo(a,h)anthracene	25.69	278	644366	41.86	ng	99
91) Benzo(g,h,i)perylene	26.37	276	646039	41.60	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
 Data File : BG016602.D
 Acq On : 22 Apr 2015 3:21
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 Client Sample ID :
 SSTDCCC040

Quant Time: Apr 22 04:21:51 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 22 02:10:07 2015
 Response via : Initial Calibration

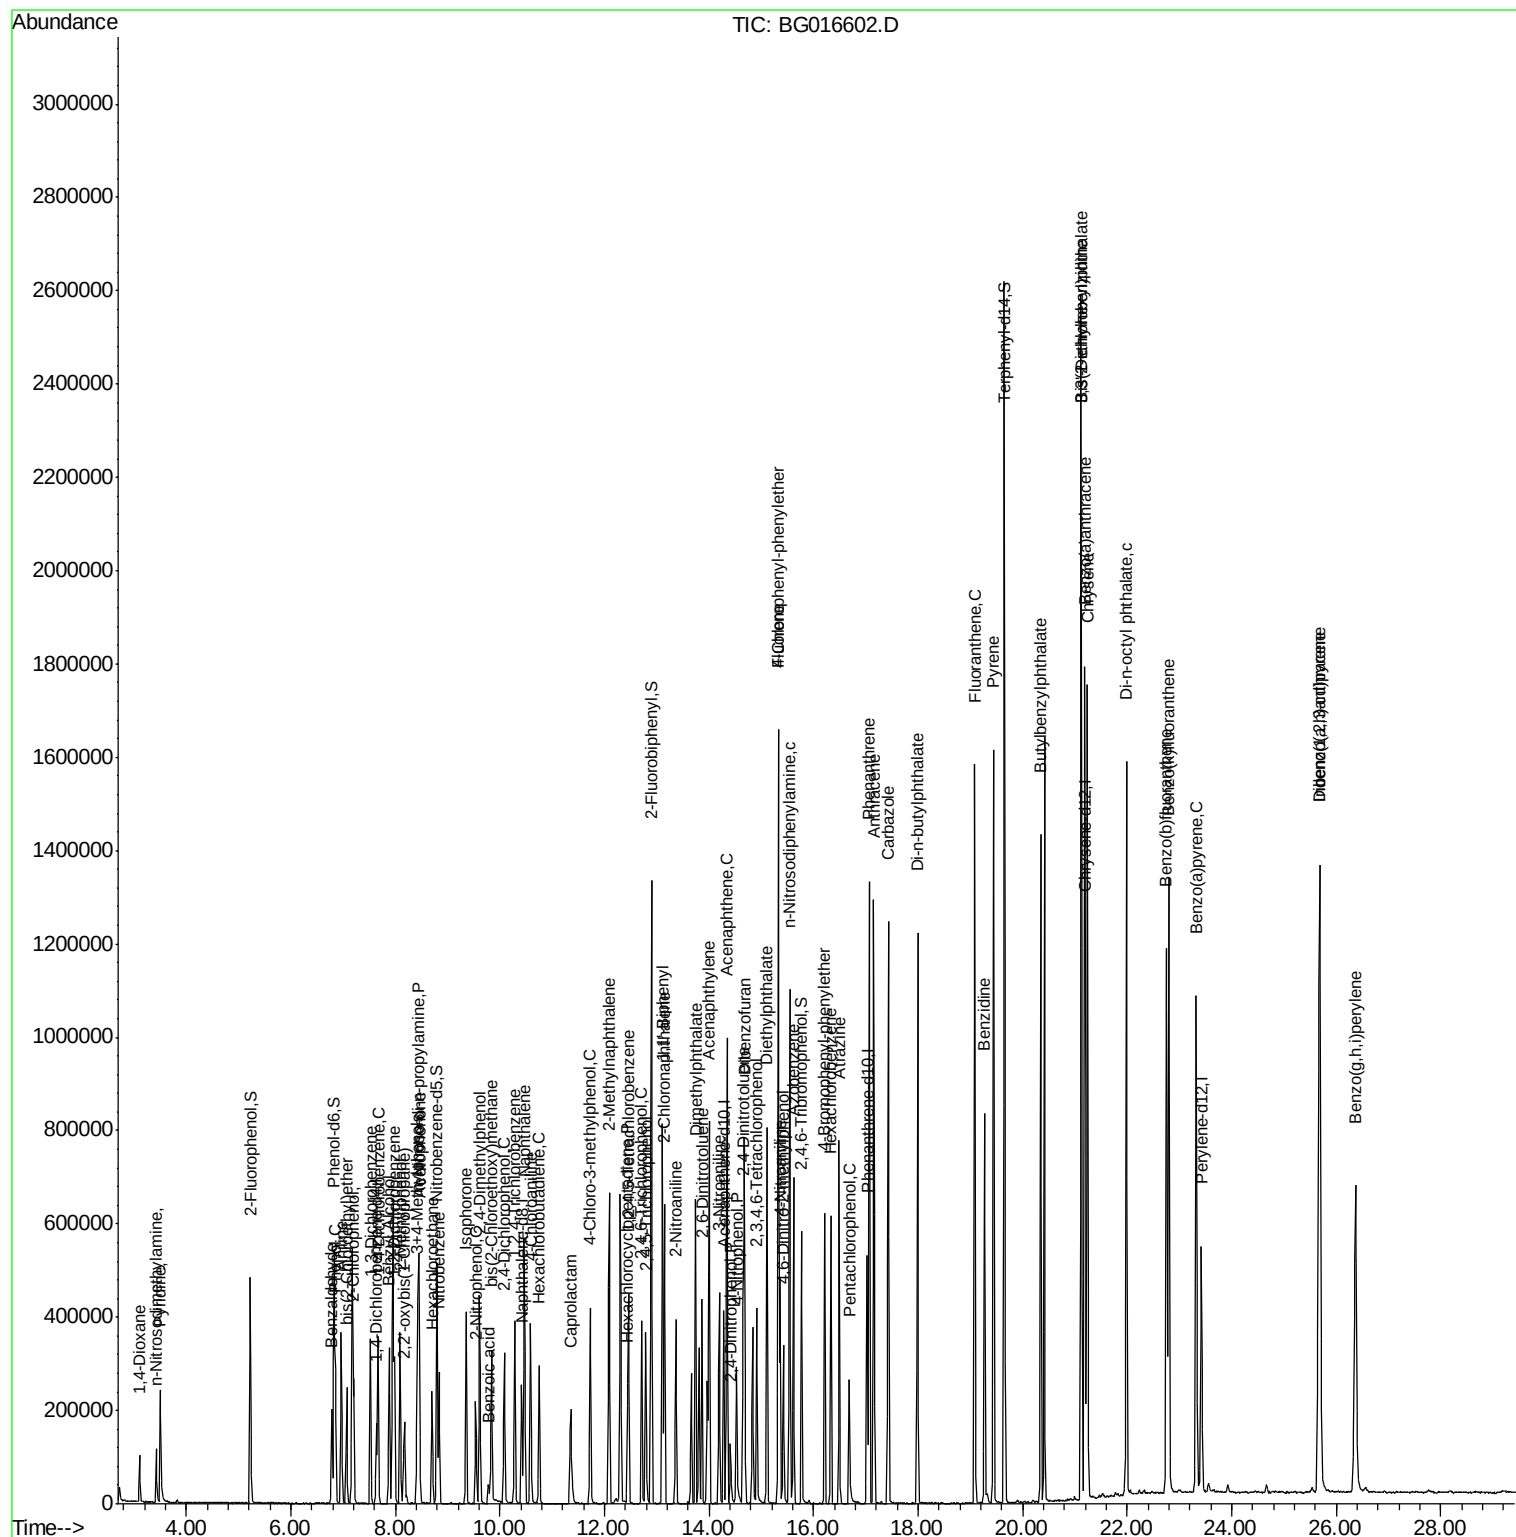

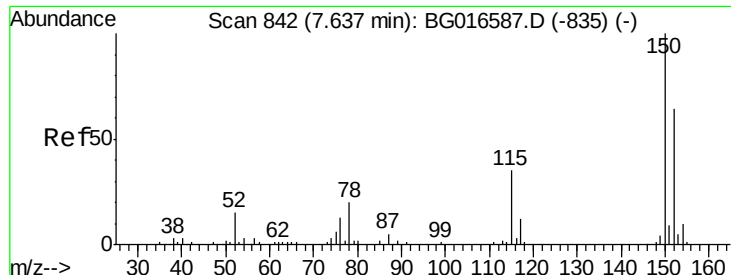

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.64 min Scan# 842

Delta R.T. -0.00 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion:152 Resp: 47639

Ion Ratio Lower Upper

152 100

150 159.8 125.5 188.3




115 56.3 44.5 66.7

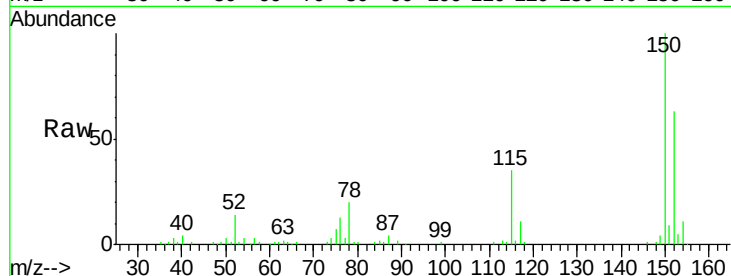

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

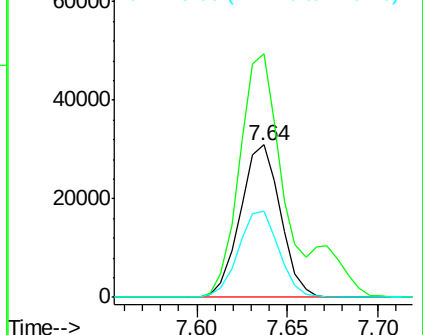

#2

1,4-Dioxane

Concen: 40.43 ng

RT: 3.10 min Scan# 70

Delta R.T. -0.00 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21


Tgt Ion: 88 Resp: 54050

Ion Ratio Lower Upper

88 100

58 59.9 46.0 69.0



43 19.2 16.2 24.4




Abundance Ion 88.00 (87.70 to 88.70): BGC

Ion 58.00 (57.70 to 58.70): BGC

Ion 43.00 (42.70 to 43.70): BGC

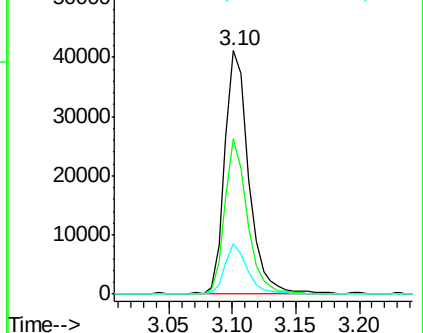

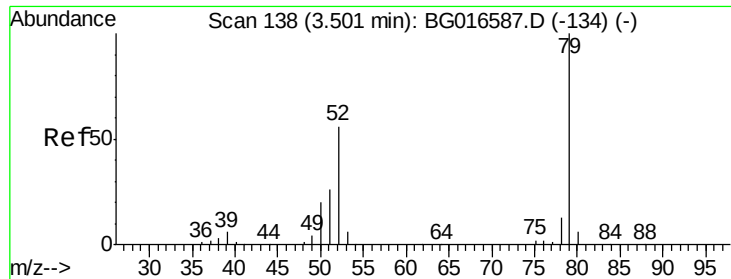

#3

Pyridine

Concen: 41.96 ng

RT: 3.50 min Scan# 138

Delta R.T. -0.00 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 79 Resp: 155140

Ion Ratio Lower Upper

79 100

52 57.2 45.0 67.4




51 26.1 21.4 32.0

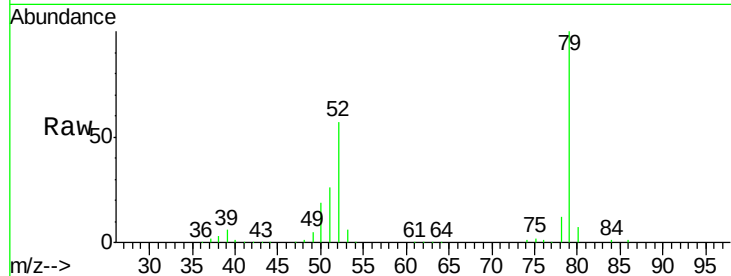

Abundance Ion 79.00 (78.70 to 79.70): BGC

Ion 52.00 (51.70 to 52.70): BGC

Ion 51.00 (50.70 to 51.70): BGC

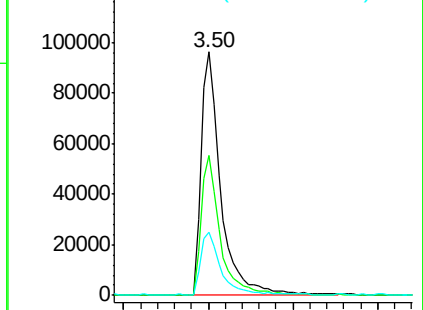

#4

n-Nitrosodimethylamine

Concen: 40.78 ng

RT: 3.42 min Scan# 125

Delta R.T. 0.01 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21


Tgt Ion: 42 Resp: 45143

Ion Ratio Lower Upper

42 100

74 187.6 151.6 227.4



44 6.9 4.9 7.3




Abundance Ion 42.00 (41.70 to 42.70): BGC

Ion 74.00 (73.70 to 74.70): BGC

Ion 44.00 (43.70 to 44.70): BGC

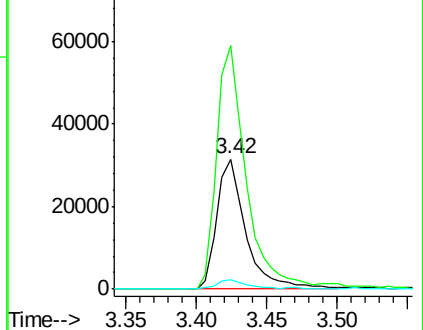



#5

2-Fluorophenol

Concen: 81.96 ng

RT: 5.22 min Scan# 431

Delta R.T. -0.01 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 112 Resp: 243603

Ion Ratio Lower Upper

112 100

64 48.9 38.5 57.7




63 24.1 18.2 27.4



Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): B

Ion 63.00 (62.70 to 63.70): B

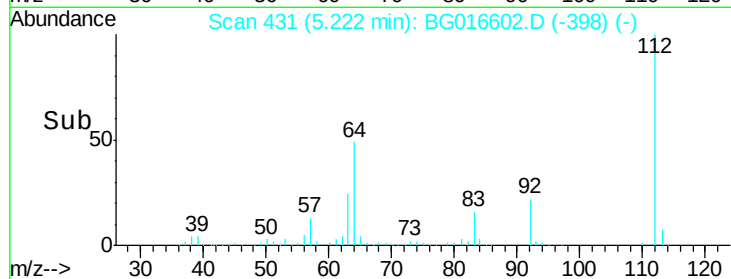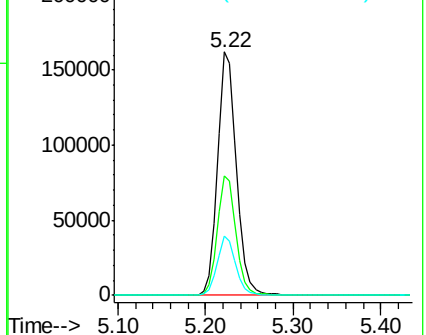

#6

Aniline

Concen: 41.31 ng

RT: 6.97 min Scan# 728

Delta R.T. -0.00 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21


Tgt Ion: 93 Resp: 236947

Ion Ratio Lower Upper

93 100

66 32.7 26.1 39.1



65 17.1 13.0 19.6




Abundance Ion 93.00 (92.70 to 93.70): B

Ion 66.00 (65.70 to 66.70): B

Ion 65.00 (64.70 to 65.70): B

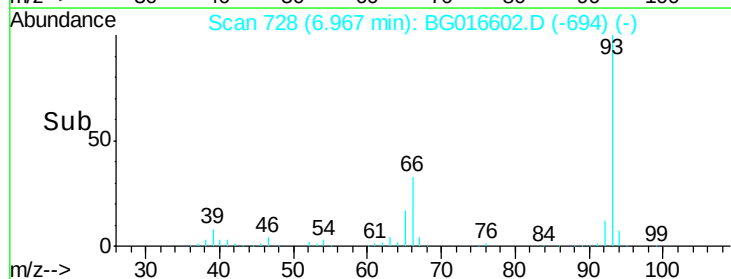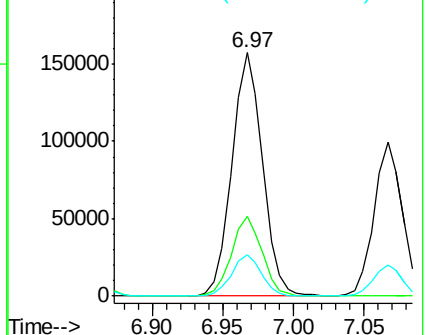

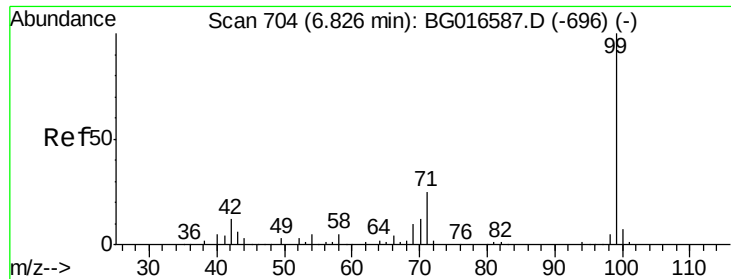

#7

Phenol-d6

Concen: 84.03 ng

RT: 6.83 min Scan# 704

Delta R.T. -0.00 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 99 Resp: 348952

Ion Ratio Lower Upper




99 100

42 11.4 9.5 14.3

71 25.7 20.2 30.2



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

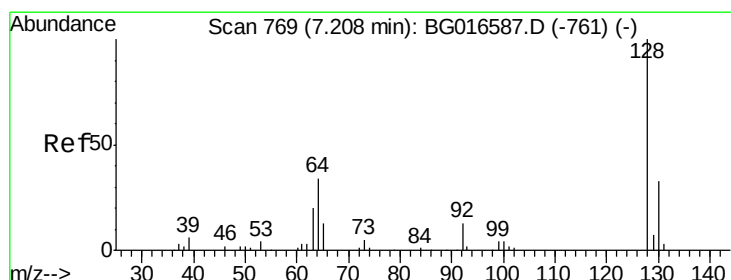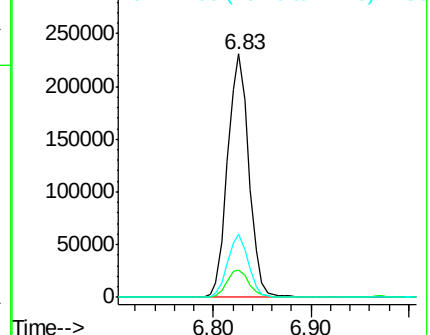

#8

2-Chlorophenol

Concen: 41.49 ng

RT: 7.20 min Scan# 768

Delta R.T. -0.01 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21


Tgt Ion: 128 Resp: 147217

Ion Ratio Lower Upper



128 100


130 31.2 13.5 53.5

64 38.0 17.9 57.9

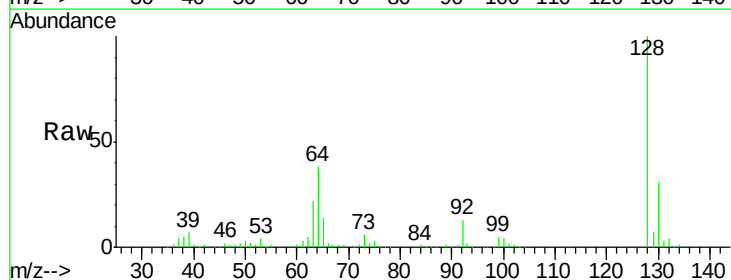

Abundance Ion 128.00 (127.70 to 128.70): BGC
Ion 130.00 (129.70 to 130.70): BGC
Ion 64.00 (63.70 to 64.70): BGC

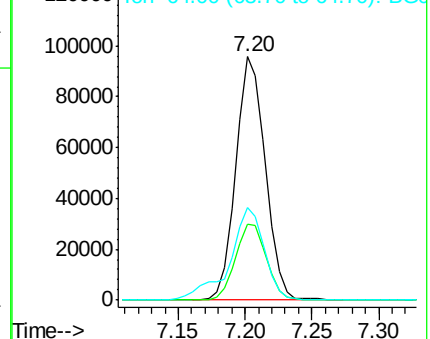

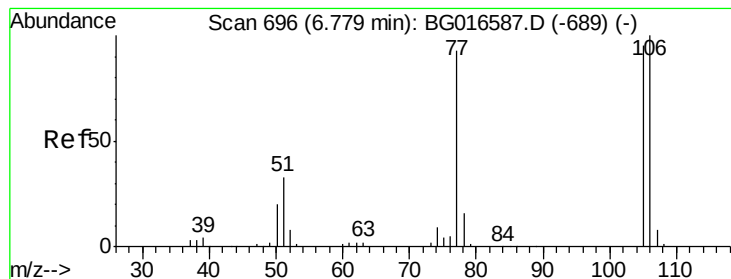

#9

Benzaldehyde

Concen: 35.50 ng

RT: 6.78 min Scan# 696

Delta R.T. -0.00 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040


Tgt Ion: 77 Resp: 67089

Ion Ratio Lower Upper




77 100

105 97.4 81.6 121.6

106 100.9 87.4 127.4



Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 105.00 (104.70 to 105.70): BGC
Ion 106.00 (105.70 to 106.70): BGC

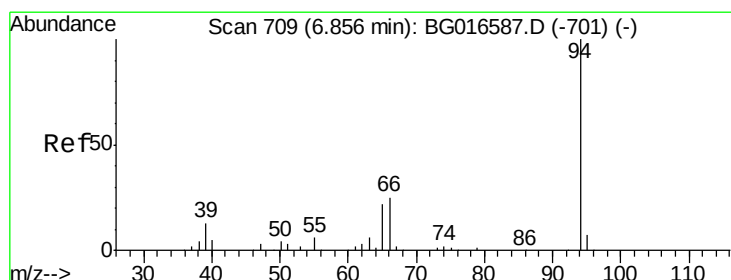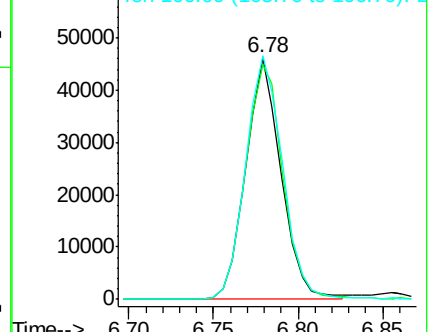

#10

Phenol

Concen: 41.81 ng

RT: 6.85 min Scan# 708

Delta R.T. -0.01 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21


Tgt Ion: 94 Resp: 183661

Ion Ratio Lower Upper



94 100


65 23.7 2.6 42.6

66 28.0 6.3 46.3



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

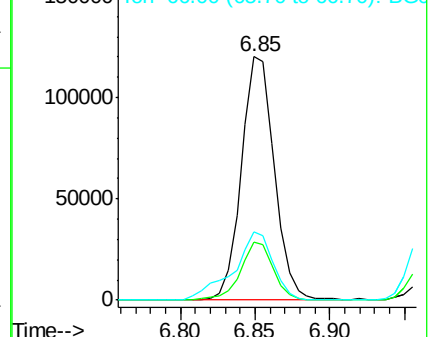


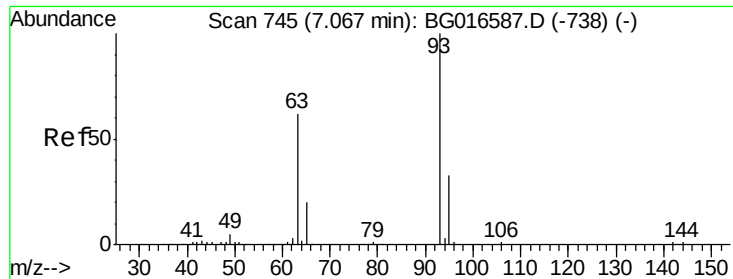




#11
bis(2-Chloroethyl)ether
Concen: 40.22 ng
RT: 7.07 min Scan# 745
Delta R.T. -0.00 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion: 93 Resp: 138319
Ion Ratio Lower Upper
93 100
63 62.0 42.0 82.0
95 32.9 12.6 52.6

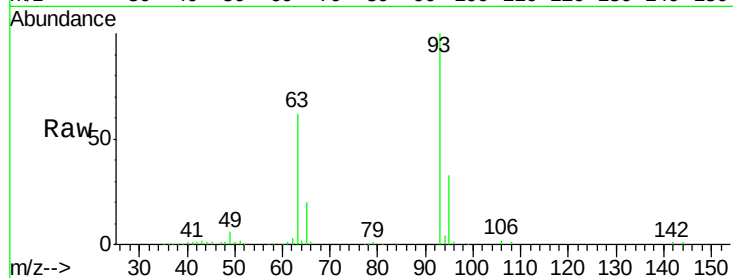


Abundance Ion 93.00 (92.70 to 93.70): BGC
Ion 63.00 (62.70 to 63.70): BGC
Ion 95.00 (94.70 to 95.70): BGC

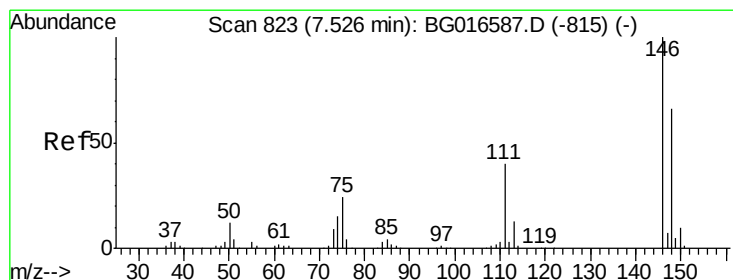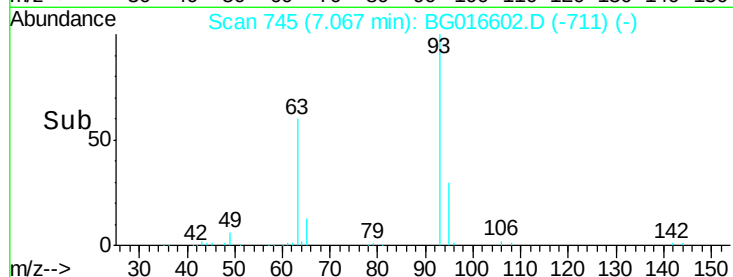
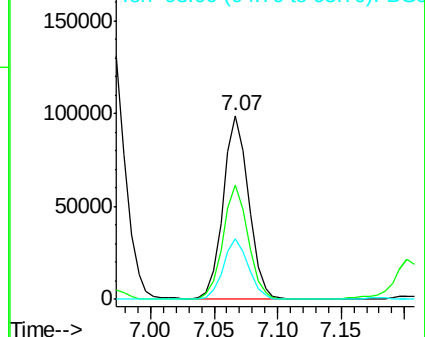



#12
1,3-Dichlorobenzene
Concen: 40.80 ng
RT: 7.53 min Scan# 823
Delta R.T. -0.00 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Tgt Ion: 146 Resp: 151160
Ion Ratio Lower Upper
146 100
148 63.9 52.6 79.0
75 25.0 19.5 29.3

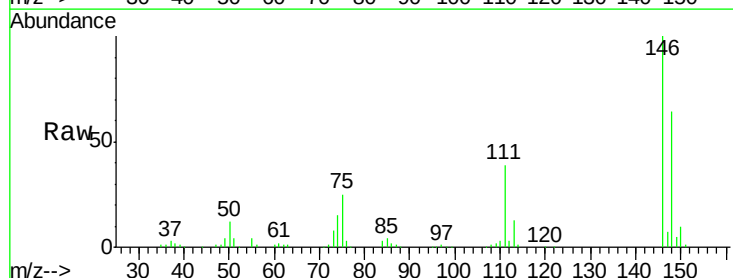

Abundance Ion 146.00 (145.70 to 146.70): BGC
Ion 148.00 (147.70 to 148.70): BGC
Ion 75.00 (74.70 to 75.70): BGC

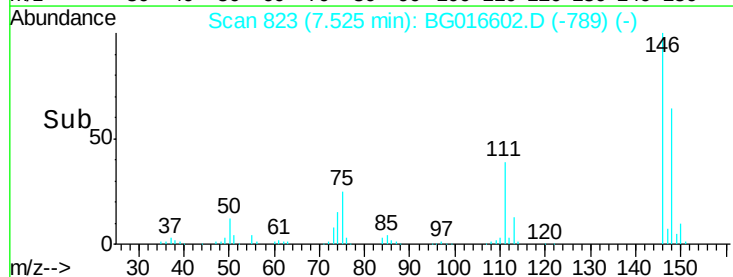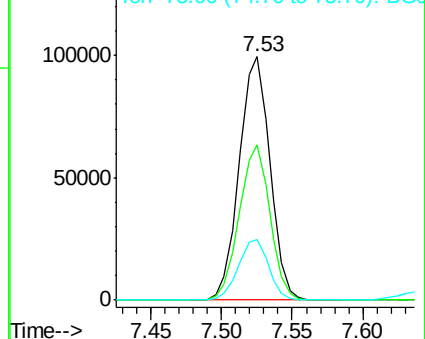


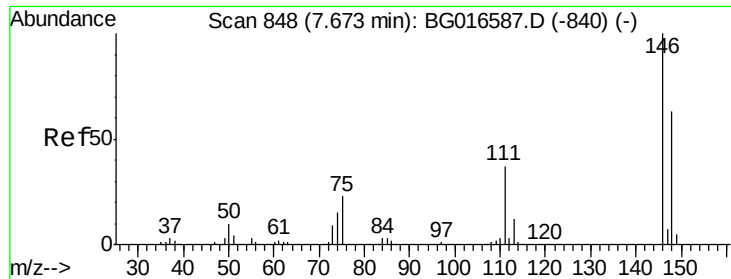




#13
 1,4-Dichlorobenzene
 Concen: 40.91 ng
 RT: 7.67 min Scan# 848
 Delta R.T. -0.00 min
 Lab File: BG016602.D
 Acq: 22 Apr 2015 3:21

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Tgt Ion:146 Resp: 154278
 Ion Ratio Lower Upper
 146 100
 148 65.0 50.5 75.7
 111 38.9 29.6 44.4

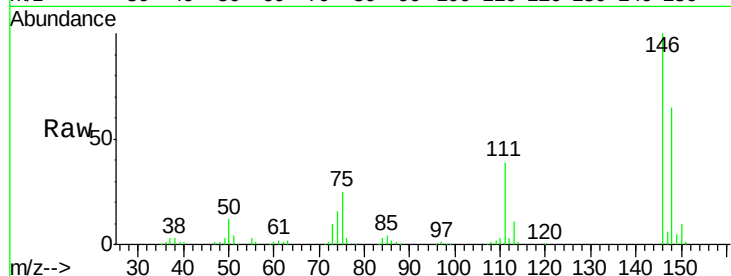


Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E


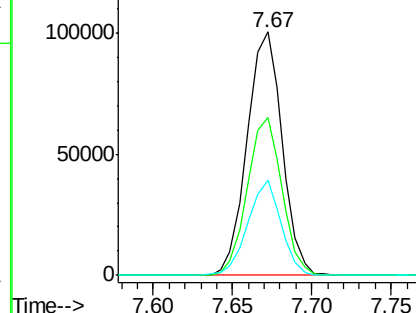



#14
 1,2-Dichlorobenzene
 Concen: 41.06 ng
 RT: 7.98 min Scan# 901
 Delta R.T. -0.00 min
 Lab File: BG016602.D
 Acq: 22 Apr 2015 3:21

Tgt Ion:146 Resp: 147301
 Ion Ratio Lower Upper
 146 100
 148 63.0 51.4 77.2
 111 40.9 32.6 48.8



Abundance Ion 146.00 (145.70 to 146.70): E
 Ion 148.00 (147.70 to 148.70): E
 Ion 111.00 (110.70 to 111.70): E

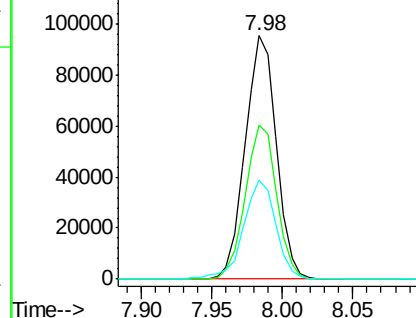



#15

Benzyl Alcohol

Concen: 41.65 ng

RT: 7.88 min Scan# 883

Delta R.T. -0.01 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21

Instrument :

BNA_G

ClientSampleId :

SSTDCCC040





Tgt Ion: 79 Resp: 110068

Ion Ratio Lower Upper

79 100

108 90.0 74.8 112.2

77 63.3 50.0 75.0

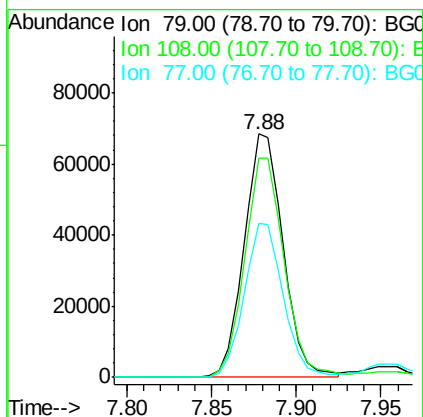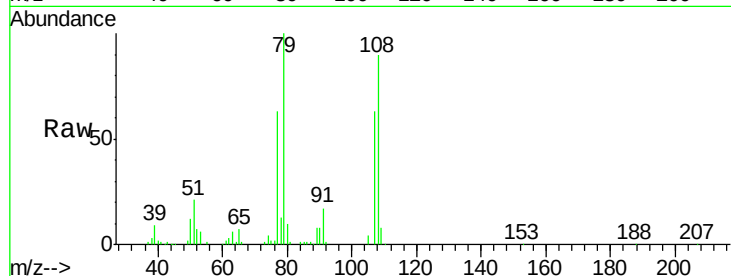

#16

2,2'-oxybis(1-Chloropropane)

Concen: 40.25 ng

RT: 8.17 min Scan# 933

Delta R.T. -0.01 min

Lab File: BG016602.D

Acq: 22 Apr 2015 3:21




Tgt Ion: 45 Resp: 134039


Ion Ratio Lower Upper

45 100

77 17.5 0.0 35.7

79 14.4 0.0 34.3

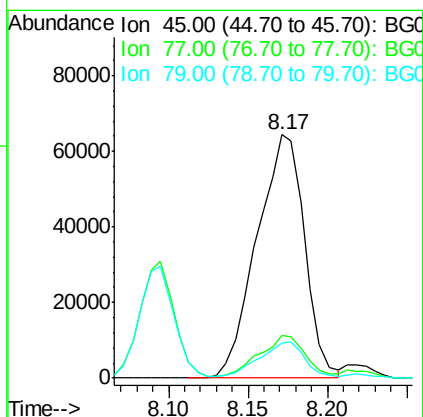


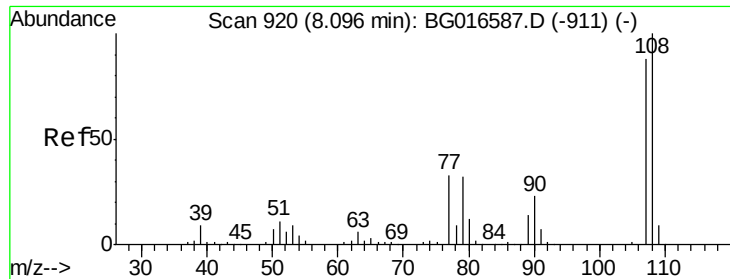




#17
2-Methylphenol
Concen: 41.89 ng
RT: 8.10 min Scan# 920
Delta R.T. -0.00 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion:	107	Resp:	124017
Ion	Ratio	Lower	Upper
107	100		
108	110.0	91.6	137.4
77	38.9	30.2	45.4
79	37.3	29.4	44.2

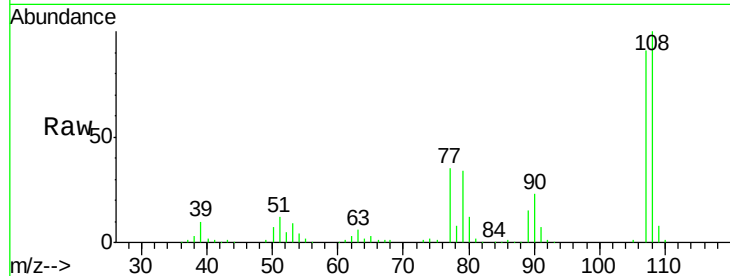


Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BG
Ion 79.00 (78.70 to 79.70): BG

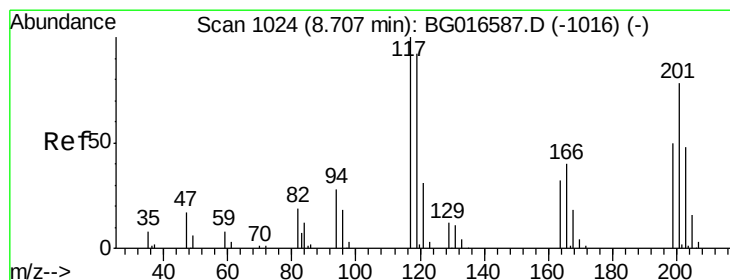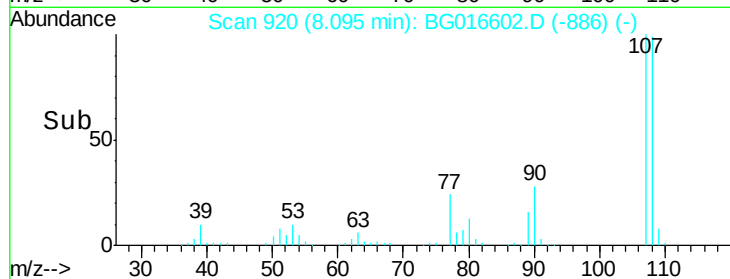
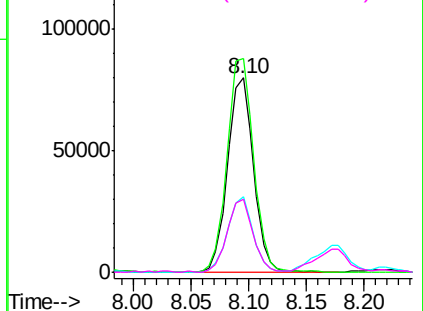



#18
Hexachloroethane
Concen: 40.74 ng
RT: 8.70 min Scan# 1023
Delta R.T. -0.01 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Tgt Ion:	117	Resp:	55168
Ion	Ratio	Lower	Upper
117	100		
119	91.4	73.8	110.8
201	74.3	62.2	93.2

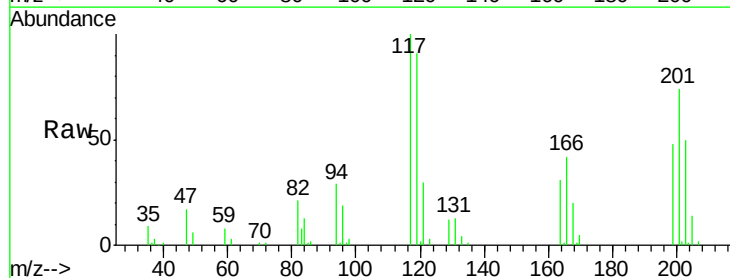

Abundance Ion 117.00 (116.70 to 117.70): E
Ion 119.00 (118.70 to 119.70): E
Ion 201.00 (200.70 to 201.70): E



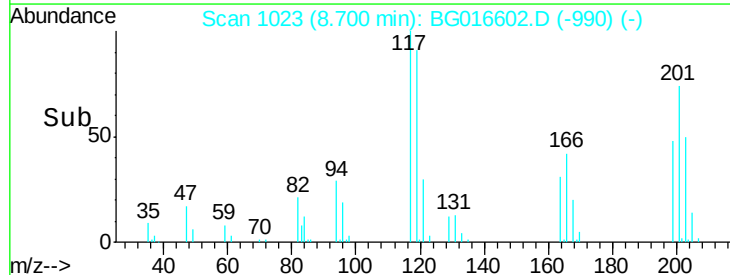
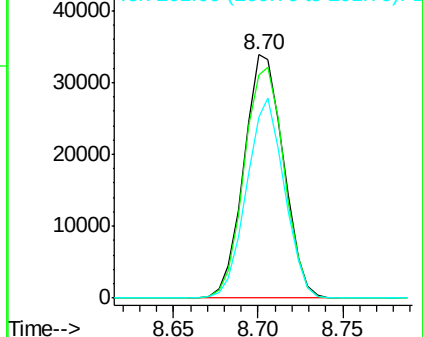


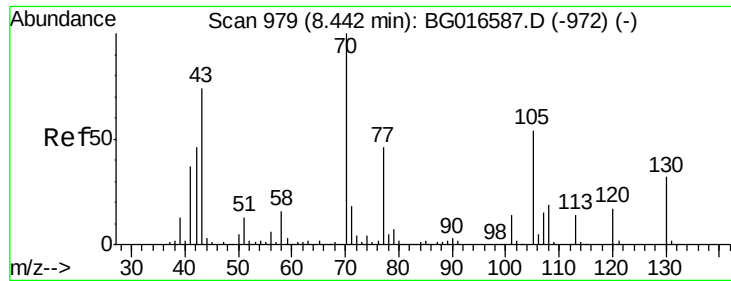

#19
n-Nitroso-di-n-propylamine
Concen: 41.06 ng
RT: 8.44 min Scan# 979
Delta R.T. -0.00 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21




Instrument :
BNA_G
ClientSampleId :
SSTDCCC040


Tgt Ion: 70 Resp: 110250
Ion Ratio Lower Upper
70 100
42 42.2 36.9 55.3
101 13.6 10.8 16.2
130 31.7 25.4 38.2

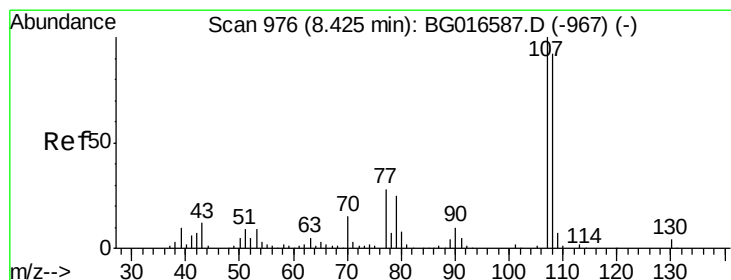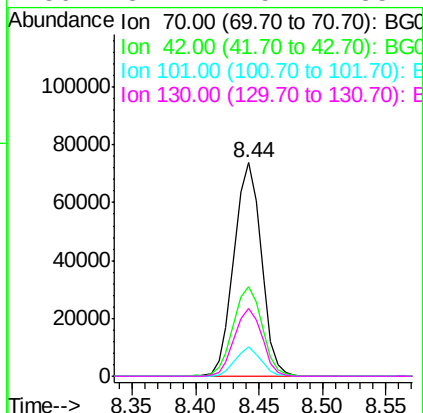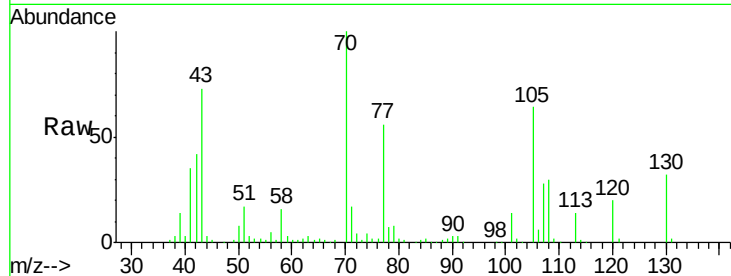

#20
3+4-Methylphenols
Concen: 42.07 ng
RT: 8.42 min Scan# 975
Delta R.T. -0.01 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Tgt Ion: 107 Resp: 171530
Ion Ratio Lower Upper
107 100
108 90.8 71.6 111.6
77 27.0 7.6 47.6
79 23.6 5.1 45.1


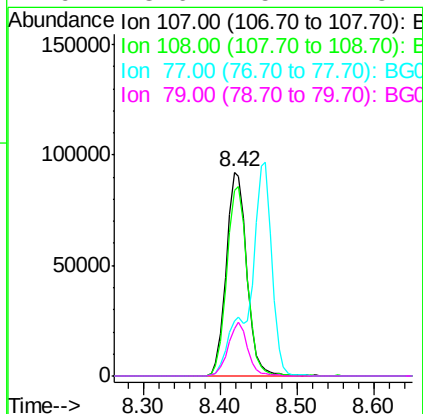




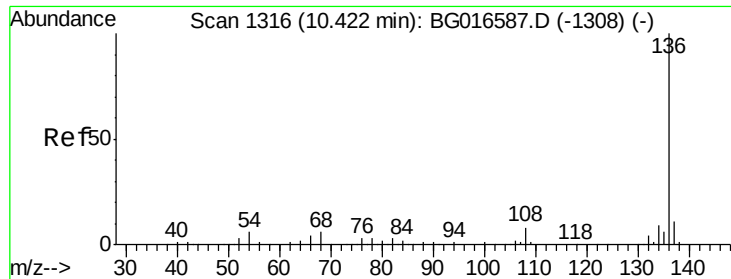

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.42 min Scan# 1315
Delta R.T. -0.01 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion:	136	Resp:	221151
Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.8	13.2
54	6.4	4.9	7.3
68	6.7	4.9	7.3

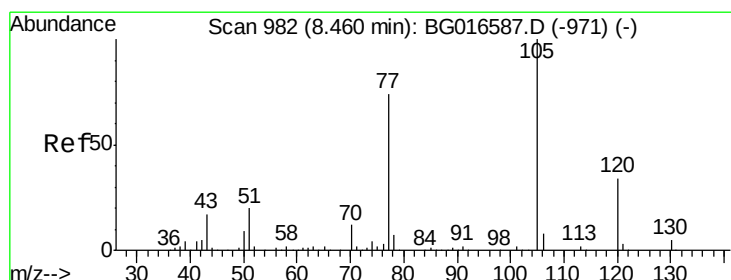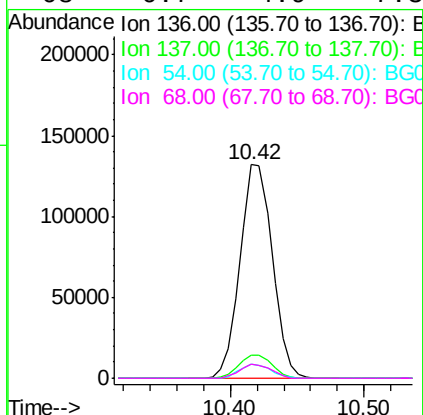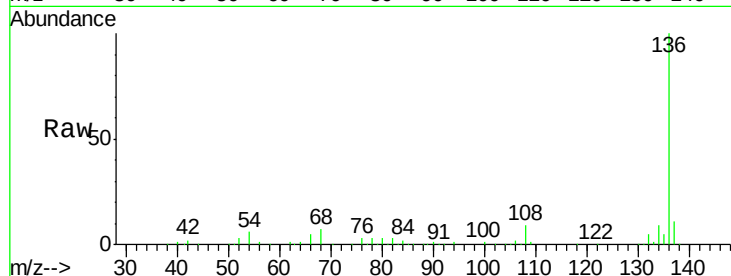

#22
Acetophenone
Concen: 41.33 ng
RT: 8.46 min Scan# 982
Delta R.T. -0.00 min
Lab File: BG016602.D
Acq: 22 Apr 2015 3:21

Tgt Ion:	105	Resp:	203603
Ion	Ratio	Lower	Upper
105	100		
71	1.7	1.8	2.6#
51	21.0	16.5	24.7
120	32.9	26.8	40.2

