


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
 Data File : BG016583.D
 Acq On : 21 Apr 2015 15:00
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 22 02:10:07 2015

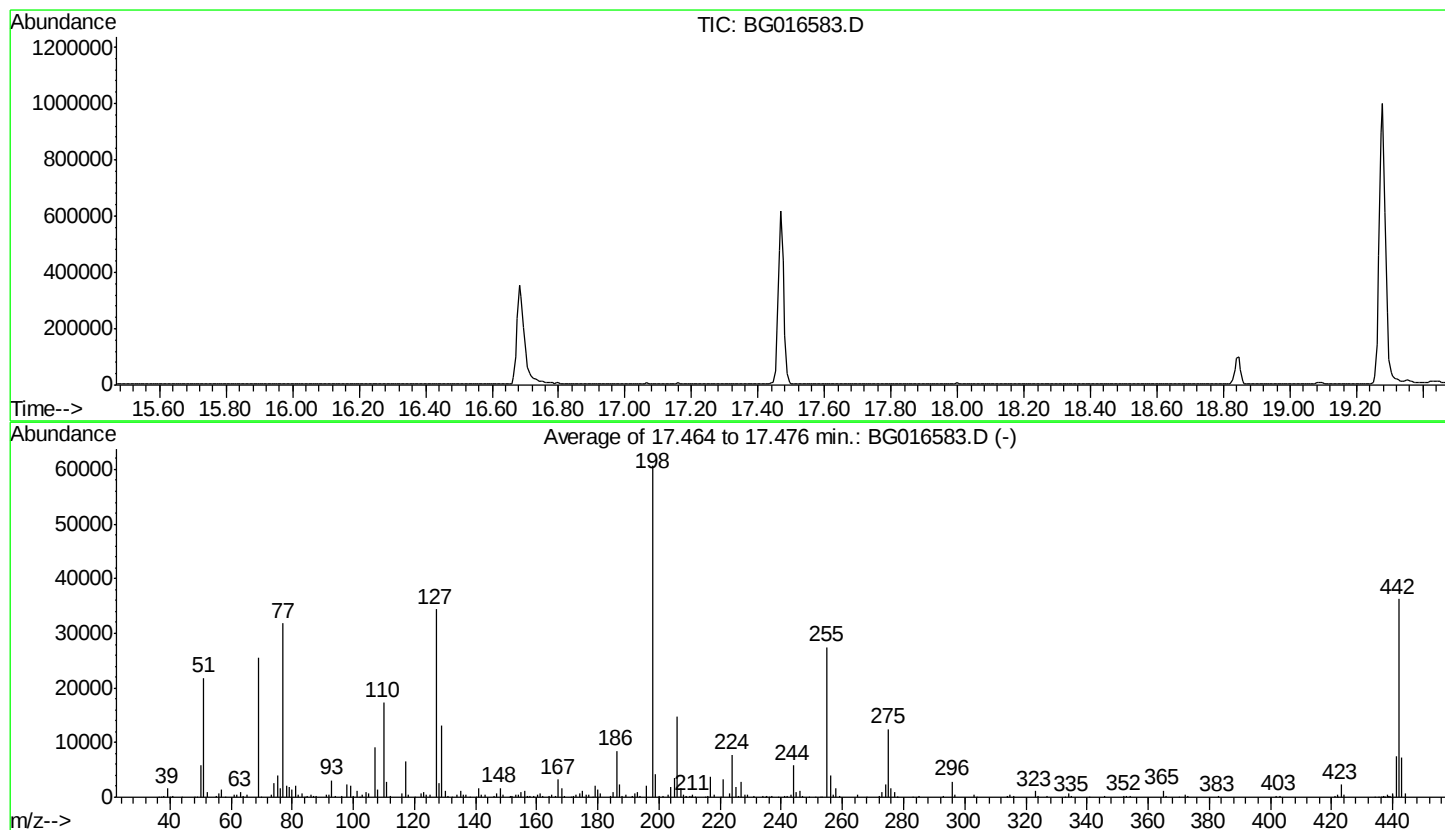

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	21833	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.2	25618	PASS
70	69	0.00	2	0.3	77	PASS
127	198	10	80	56.7	34386	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60696	PASS
199	198	5	9	6.9	4168	PASS
275	198	10	60	20.5	12451	PASS
365	198	1	100	2.0	1220	PASS
441	442	0.01	24	20.4	7418	PASS
442	198	50	100	59.8	36314	PASS
443	442	15	24	19.9	7229	PASS