
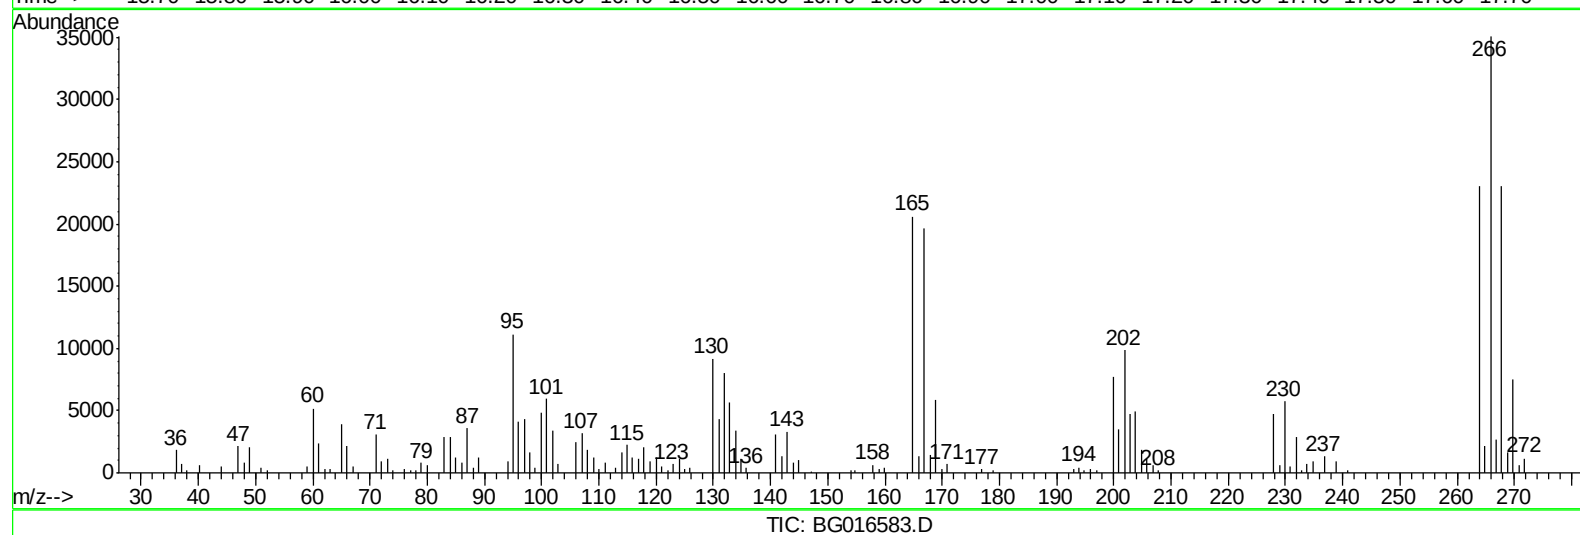


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
Data File : BG016583.D
Acq On : 21 Apr 2015 15:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:06:53 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 02:10:07 2015
Response via : Initial Calibration

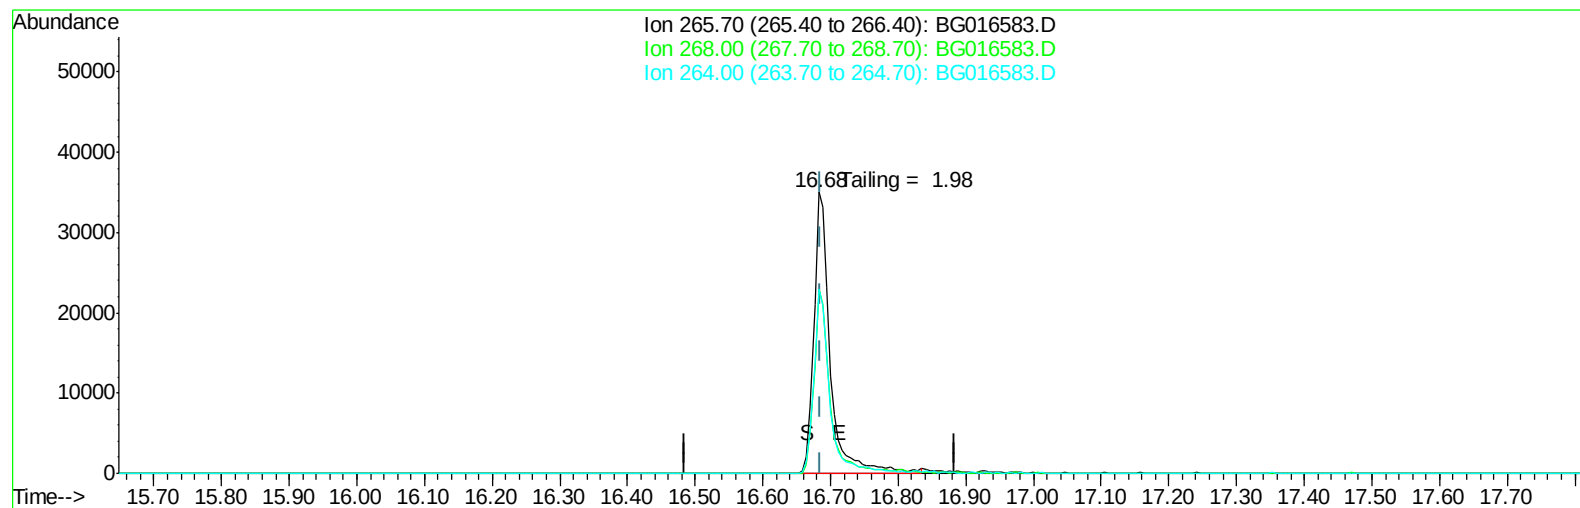

(69) Pentachlorophenol (C)



16.682min (-0.003) 42739.12ng

response 58413

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	65.67
264.00	65.30	65.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
Data File : BG016583.D
Acq On : 21 Apr 2015 15:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:06:53 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 02:10:07 2015
Response via : Initial Calibration

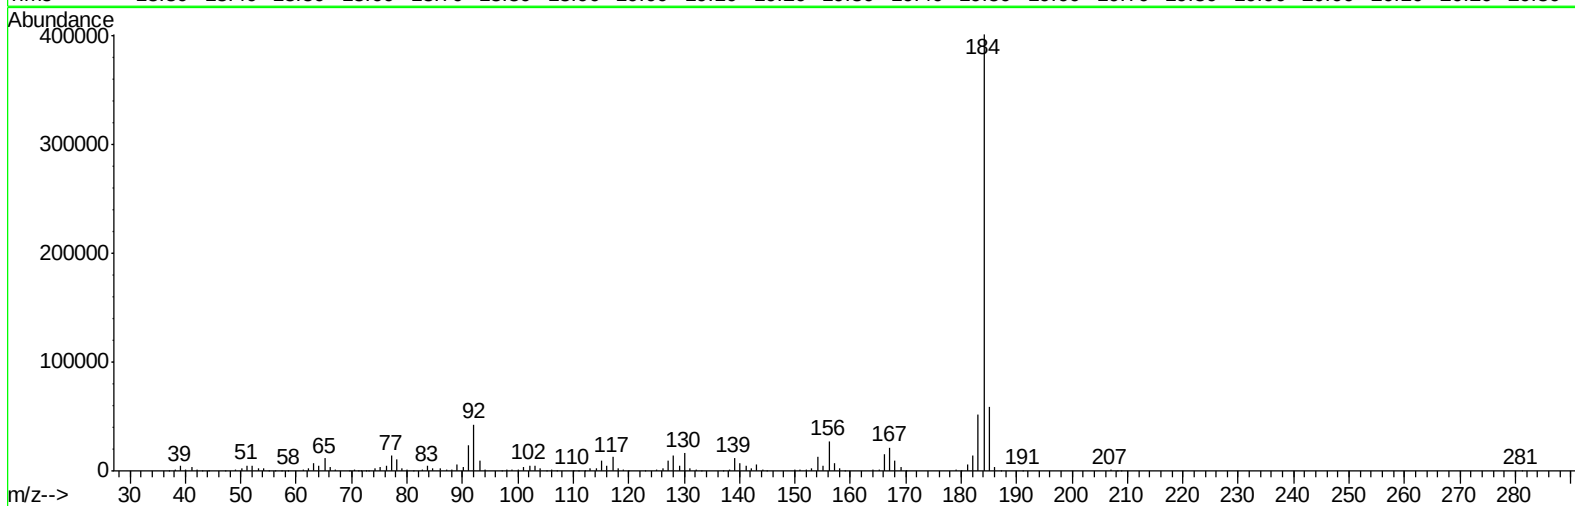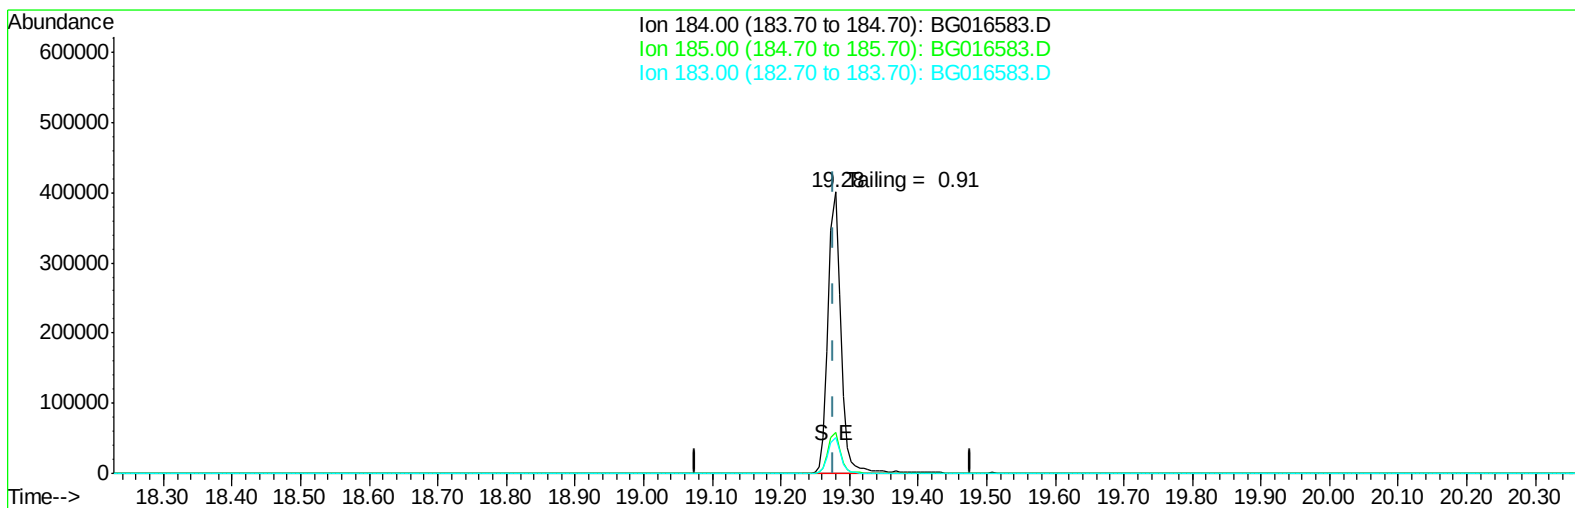

TIC: BG016583.D

(76) Benzidine

19.279min (+0.003) 23486.12ng

response 511489

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.60
183.00	12.90	12.82
0.00	0.00	0.00