
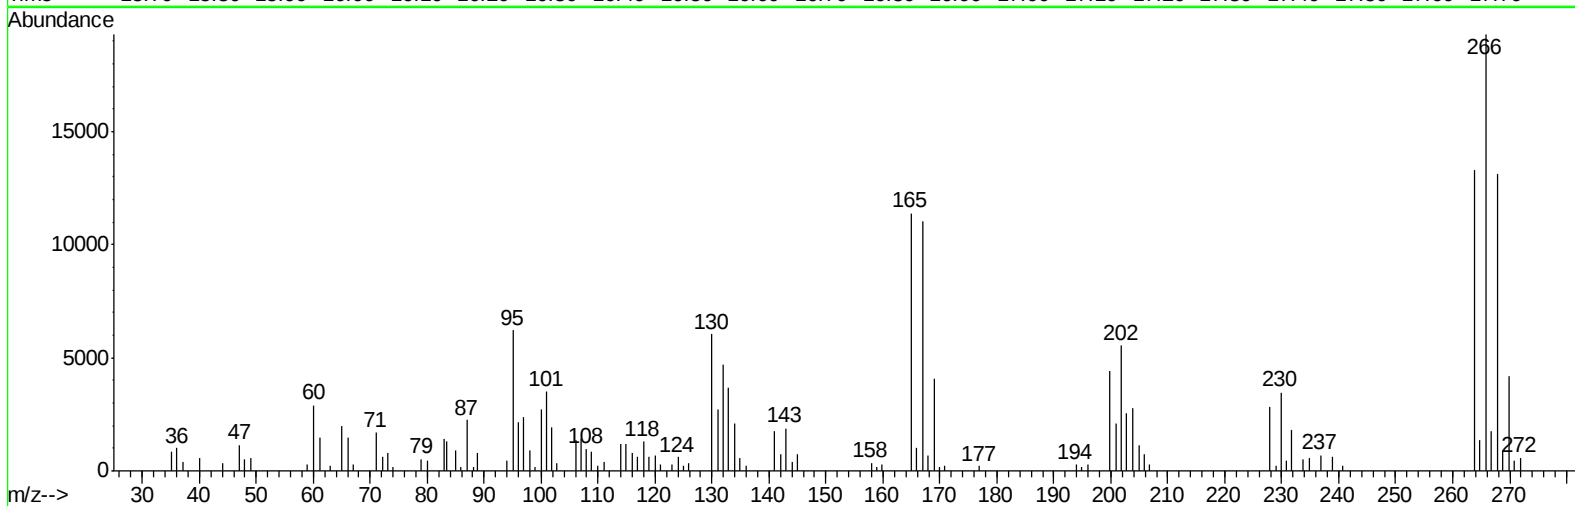


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
Data File : BG016601.D
Acq On : 22 Apr 2015 2:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:09:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 02:10:07 2015
Response via : Initial Calibration

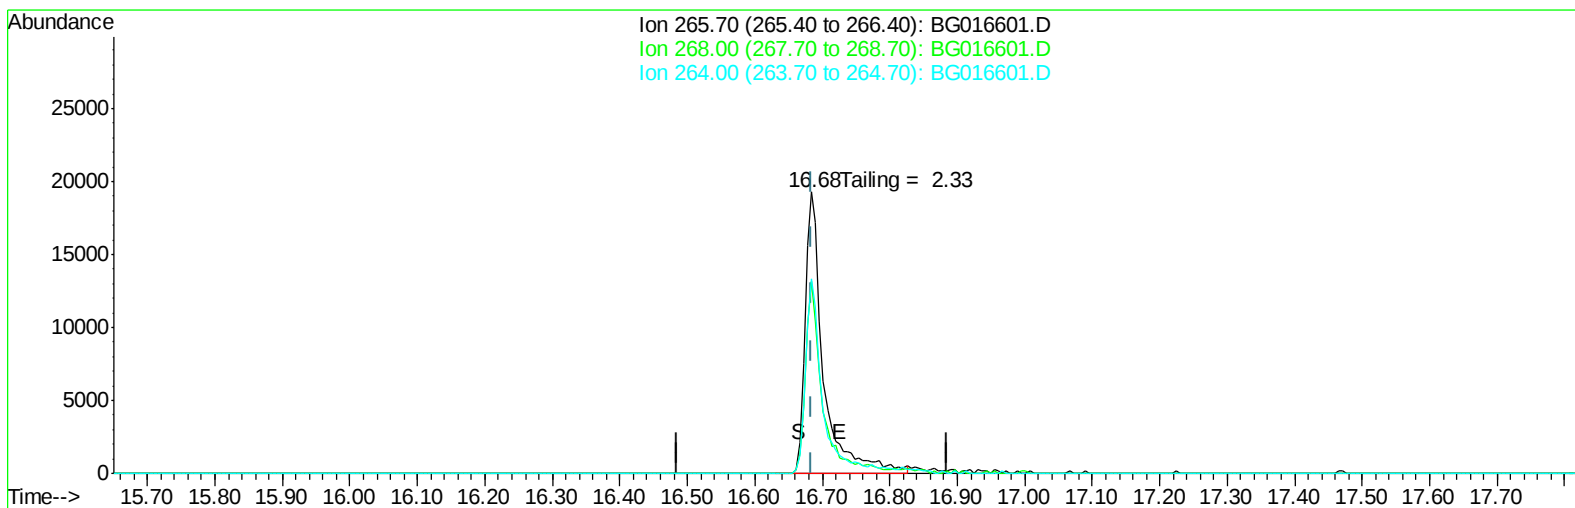

TIC: BG016601.D

(69) Pentachlorophenol (C)



16.684min (-0.001) 34611.53ng

response 36596

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	67.97
264.00	65.30	68.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042115\
Data File : BG016601.D
Acq On : 22 Apr 2015 2:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:09:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 02:10:07 2015
Response via : Initial Calibration

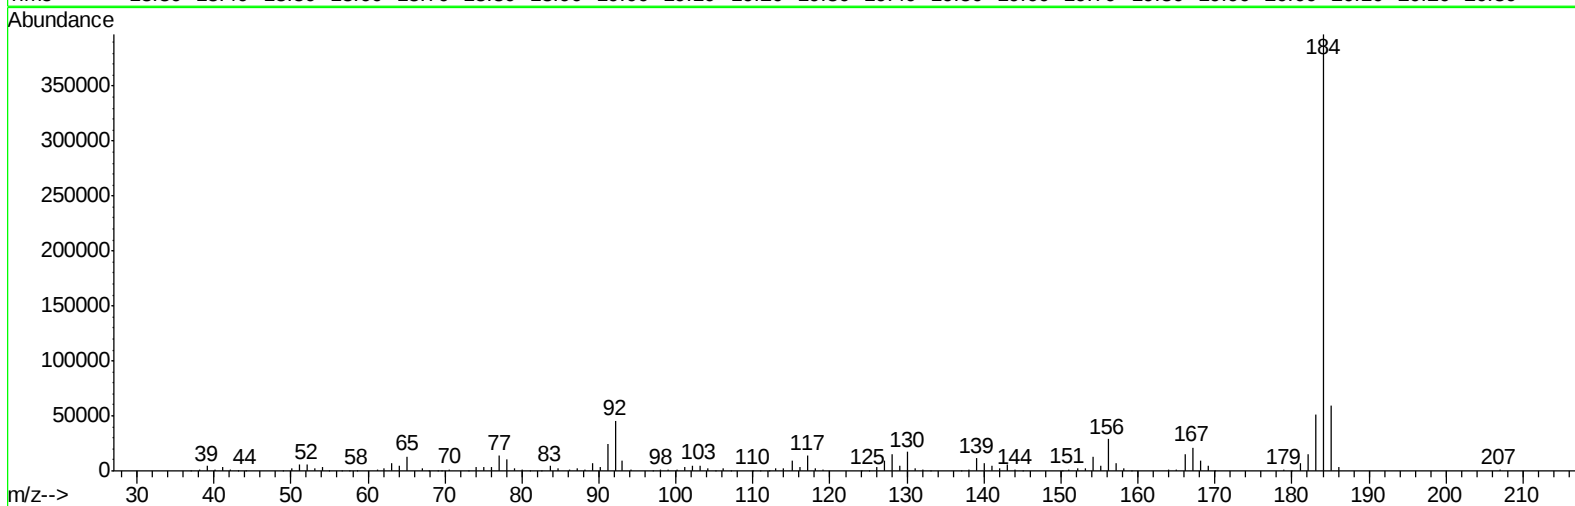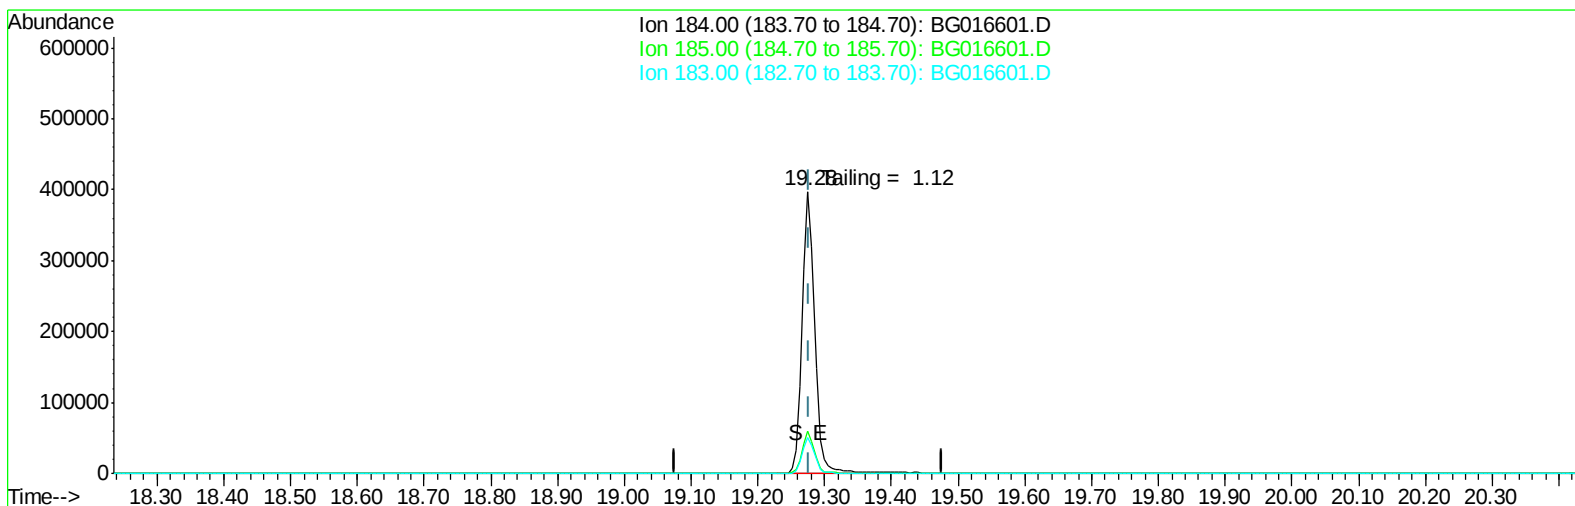

TIC: BG016601.D

(76) Benzidine

19.275min (-0.001) 44264.76ng

response 510649

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.88
183.00	12.90	12.84
0.00	0.00	0.00