

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042115\
 Data File : BG016593.D
 Acq On : 21 Apr 2015 20:58
 Operator : TP/IZ
 Sample : PB82905BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB82905BL

Quant Time: Apr 22 04:43:01 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 22 02:10:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	44775	20.00	ng	0.00
21) Naphthalene-d8	10.42	136	184939	20.00	ng	0.00
38) Acenaphthene-d10	14.28	164	101168	20.00	ng	0.00
63) Phenanthrene-d10	17.02	188	250602	20.00	ng	0.00
75) Chrysene-d12	21.21	240	283193	20.00	ng	0.00
86) Perylene-d12	23.43	264	259244	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	348489	124.74	ng	0.00
7) Phenol-d6	6.82	99	463871	118.85	ng	0.00
23) Nitrobenzene-d5	8.79	82	227978	75.90	ng	0.00
41) 2,4,6-Tribromophenol	15.77	330	86779	126.29	ng	0.00
44) 2-Fluorobiphenyl	12.90	172	513282	84.03	ng	0.00
78) Terphenyl-d14	19.66	244	903246	76.84	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042115\
Data File : BG016593.D
Acq On : 21 Apr 2015 20:58
Operator : TP/IZ
Sample : PB82905BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82905BL

Quant Time: Apr 22 04:43:01 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 02:10:07 2015
Response via : Initial Calibration

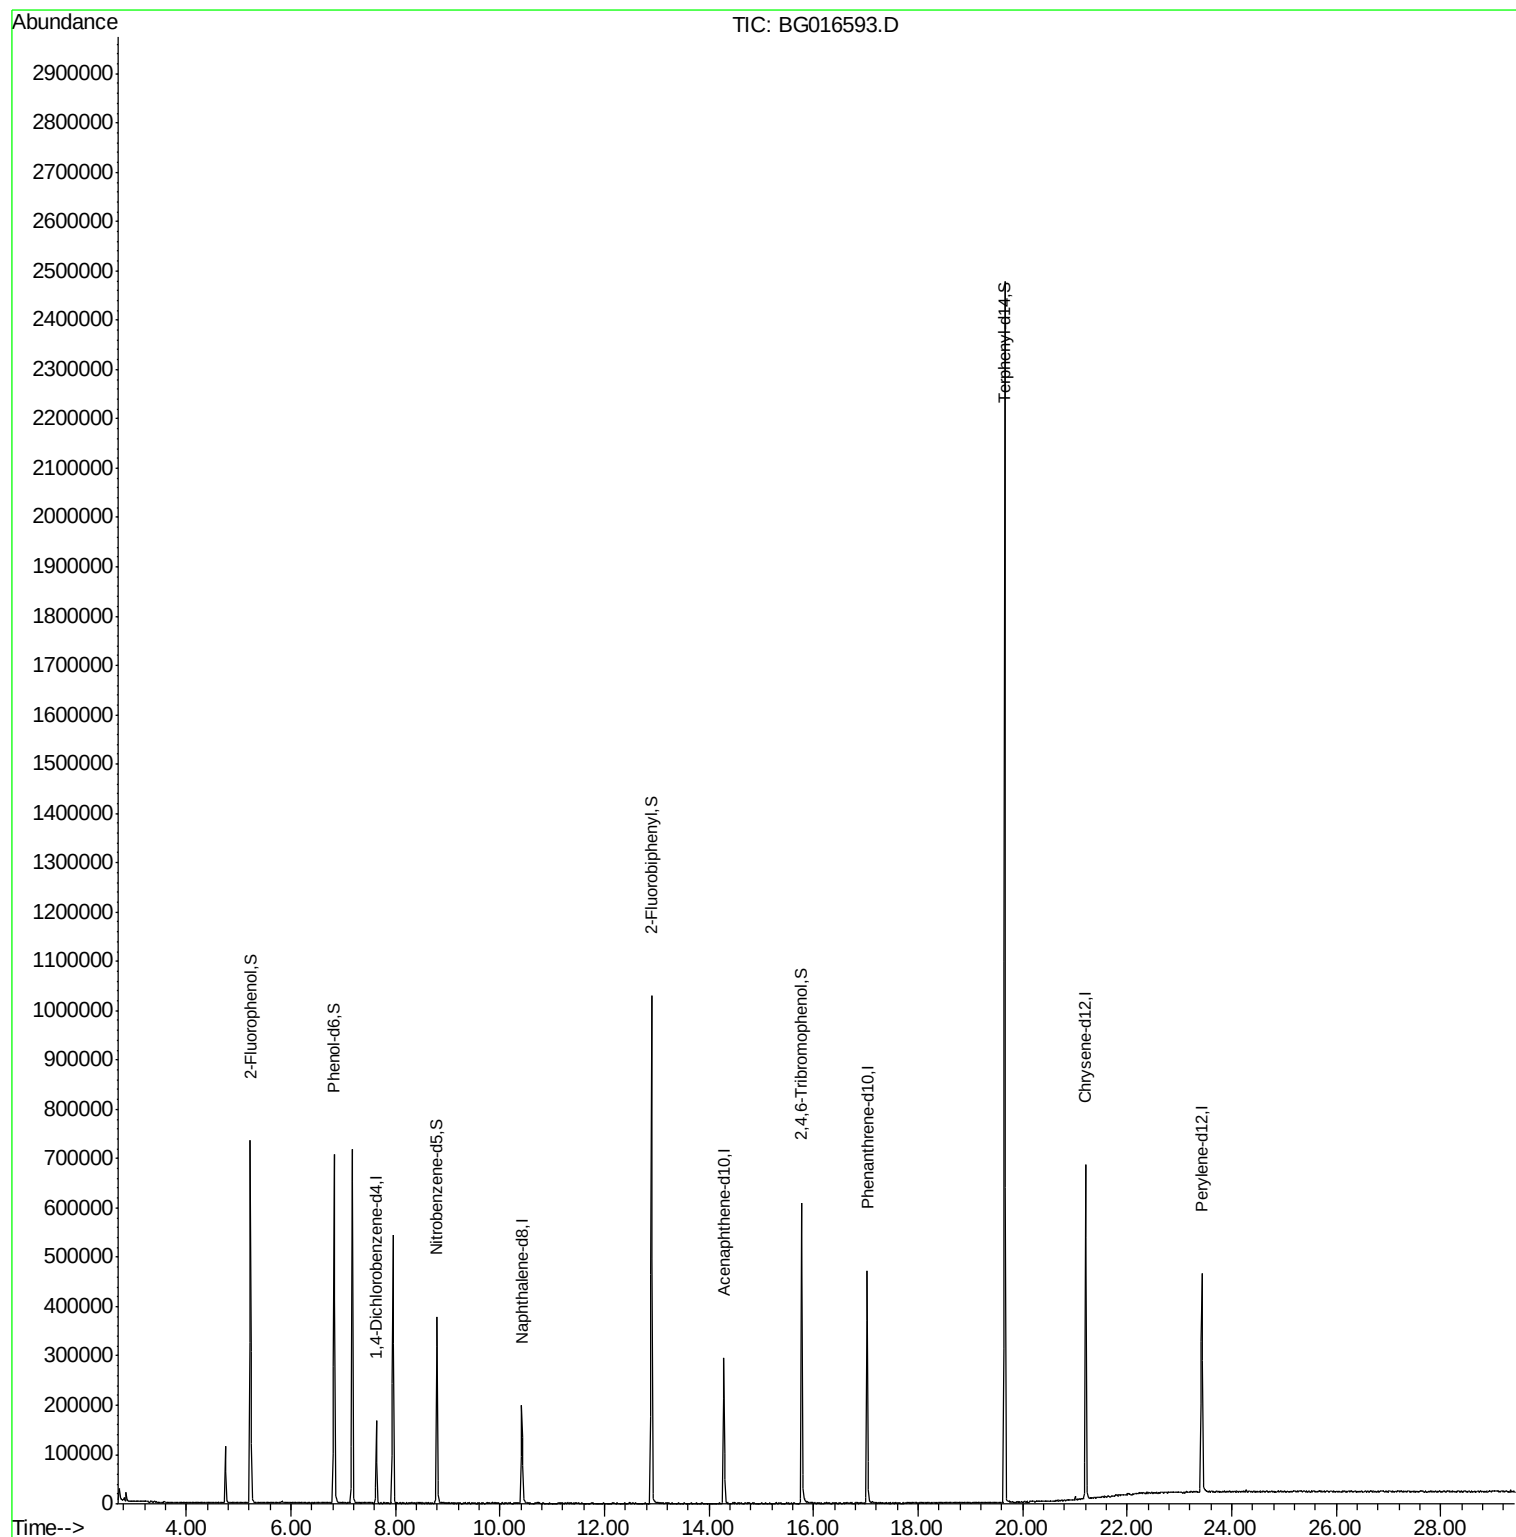

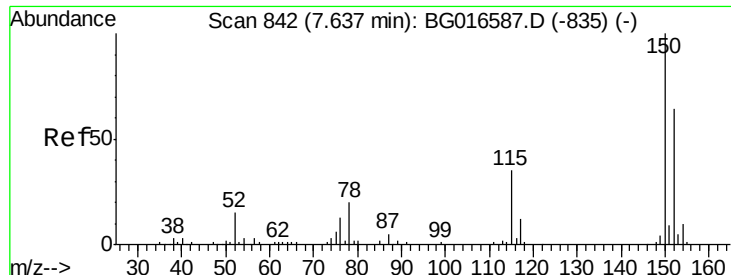


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.63 min Scan# 842
Delta R.T. -0.00 min
Lab File: BG016593.D
Acq: 21 Apr 2015 20:58

Instrument :
BNA_G
ClientSampleId :
PB82905BL

Tot Ion:152 Resp: 44775
Ion Ratio Lower Upper
152 100
150 156.6 125.5 188.3
115 57.9 44.5 66.7

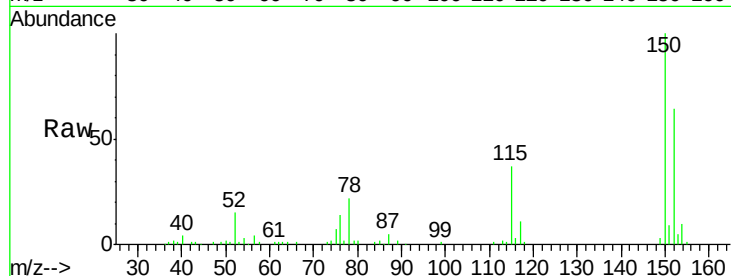


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

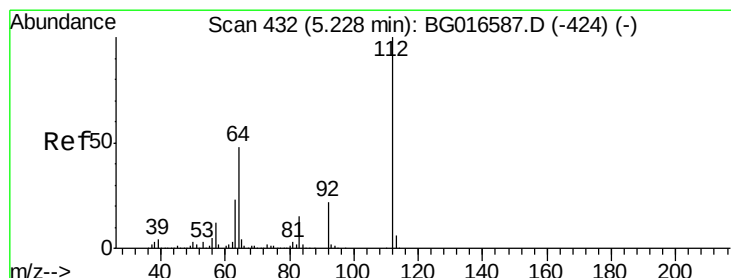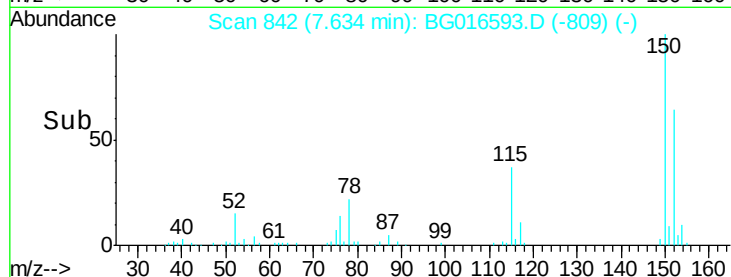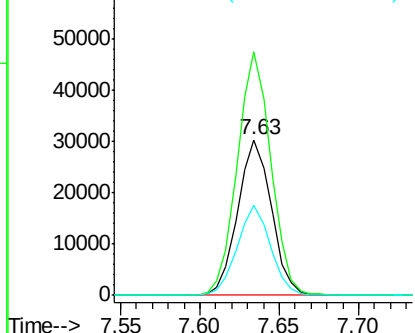



#5


2-Fluorophenol
Concen: 124.74 ng
RT: 5.23 min Scan# 432
Delta R.T. -0.00 min
Lab File: BG016593.D
Acq: 21 Apr 2015 20:58

Tgt Ion:112 Resp: 348489
Ion Ratio Lower Upper
112 100
64 48.5 38.5 57.7
63 23.3 18.2 27.4

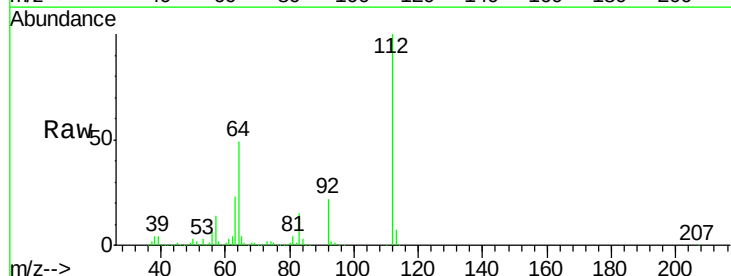

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

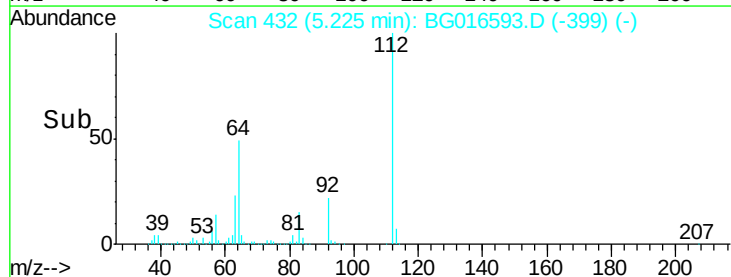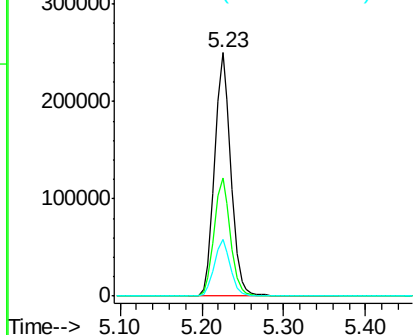

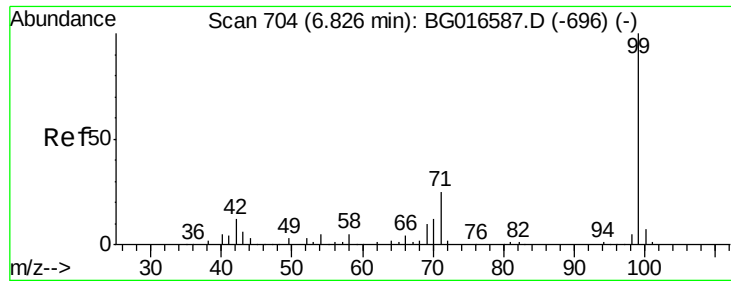

#7

Phenol-d6

Concen: 118.85 ng

RT: 6.82 min Scan# 704

Delta R.T. -0.00 min

Lab File: BG016593.D

Acq: 21 Apr 2015 20:58

Instrument :

BNA_G

ClientSampleId :

PB82905BL


Tot Ion: 99 Resp: 463871

Ion Ratio Lower Upper




99 100

42 12.3 9.5 14.3

71 26.1 20.2 30.2

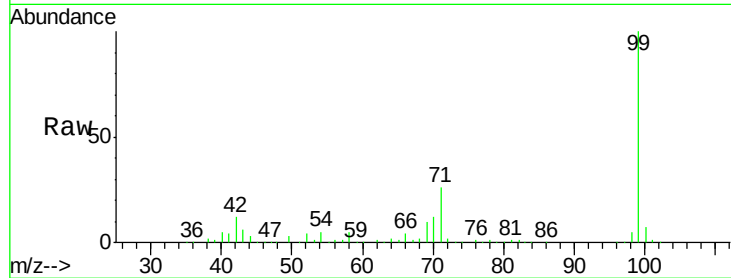

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

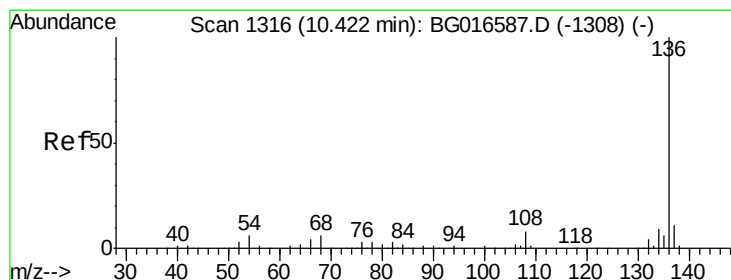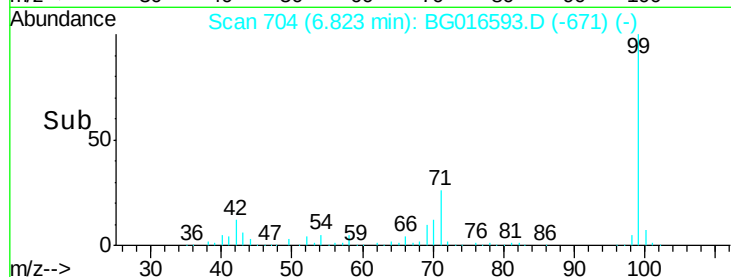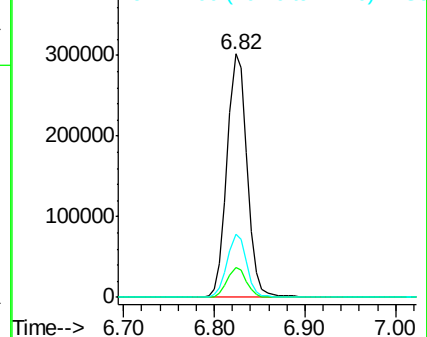

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.42 min Scan# 1316

Delta R.T. -0.00 min

Lab File: BG016593.D

Acq: 21 Apr 2015 20:58

Tgt Ion: 136 Resp: 184939


Ion Ratio Lower Upper

136 100



137 10.6 8.8 13.2


54 6.9 4.9 7.3

68 6.5 4.9 7.3

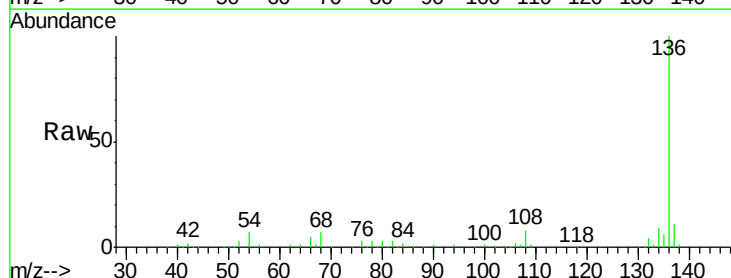

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

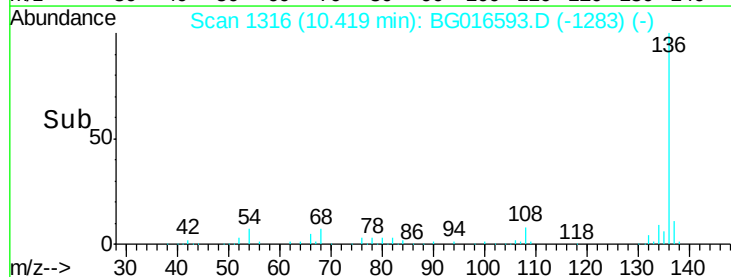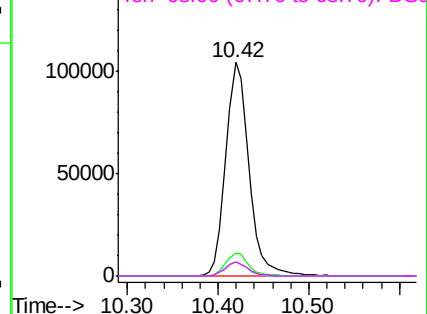


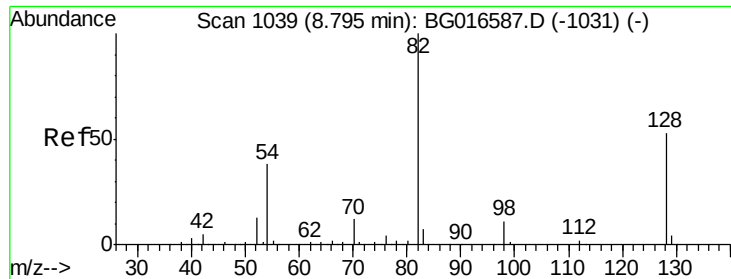




#23
Nitrobenzene-d5
Concen: 75.90 ng
RT: 8.79 min Scan# 1039
Delta R.T. -0.00 min
Lab File: BG016593.D
Acq: 21 Apr 2015 20:58

Instrument :
BNA_G
ClientSampleId :
PB82905BL

Tot Ion: 82 Resp: 227978
Ion Ratio Lower Upper
82 100
128 51.6 42.7 64.1
54 37.6 30.6 45.8

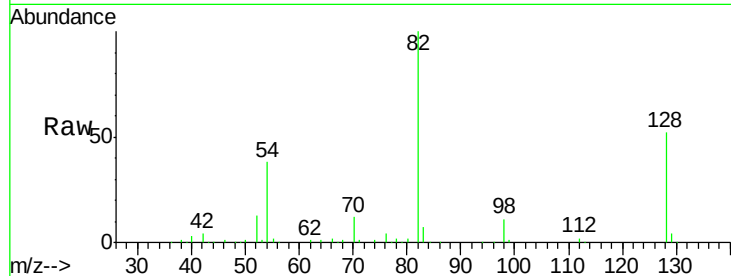


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

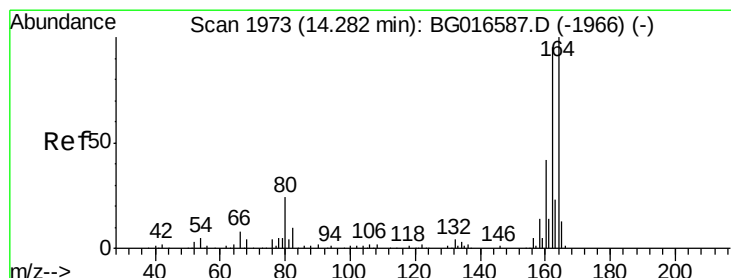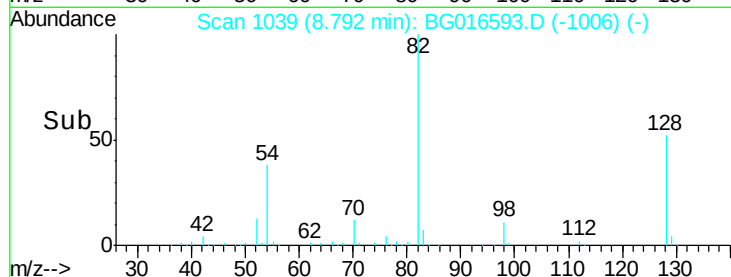
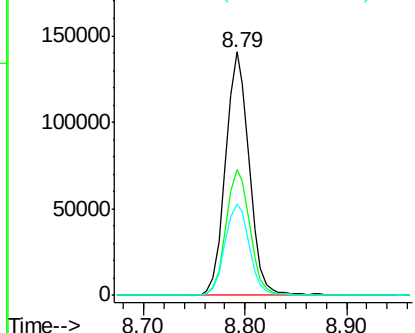



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.28 min Scan# 1973
Delta R.T. -0.00 min
Lab File: BG016593.D
Acq: 21 Apr 2015 20:58

Tgt Ion:164 Resp: 101168
Ion Ratio Lower Upper
164 100
162 96.0 75.8 113.6
160 44.5 33.8 50.6

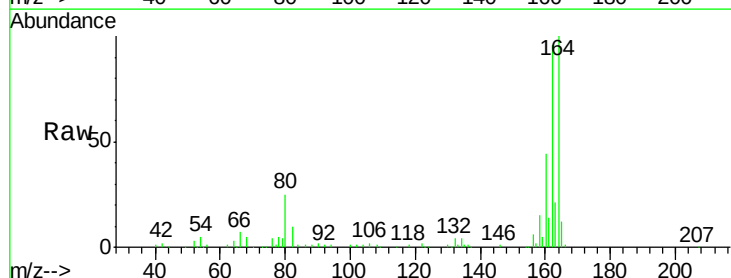

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

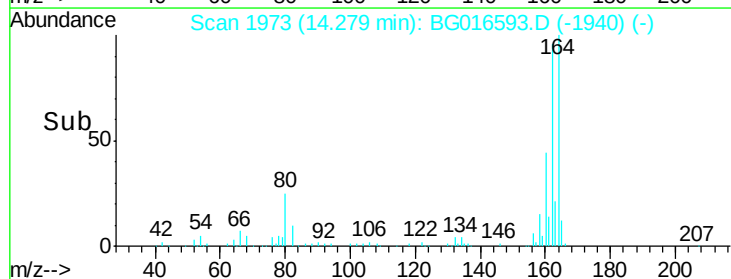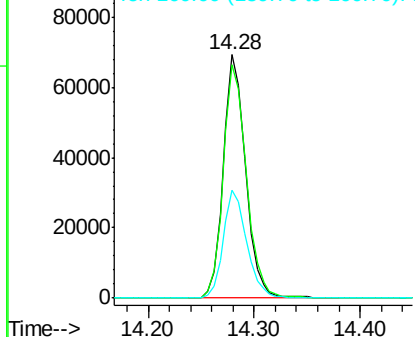


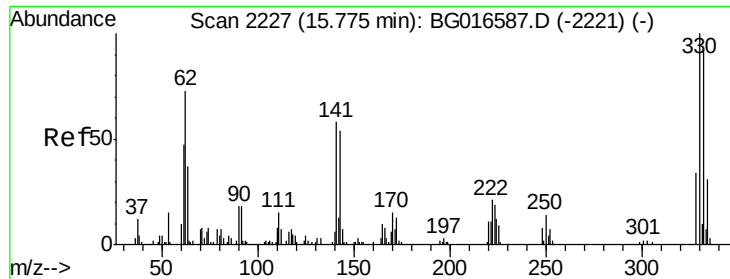




#41
 2,4,6-Tribromophenol
 Concen: 126.29 ng
 RT: 15.77 min Scan# 2227
 Delta R.T. -0.00 min
 Lab File: BG016593.D
 Acq: 21 Apr 2015 20:58

Instrument :
 BNA_G
 ClientSampleId :
 PB82905BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	76.6	114.8
141	55.2	45.9	68.9

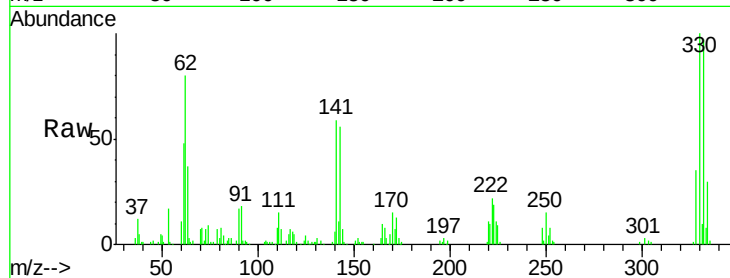


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

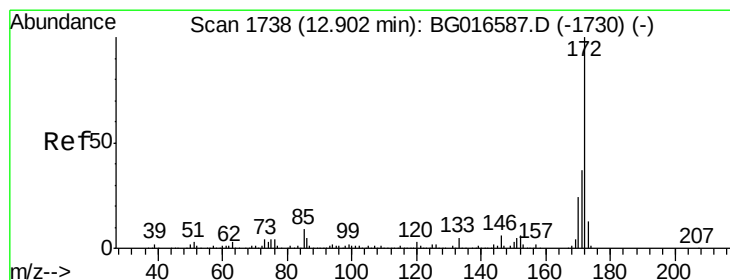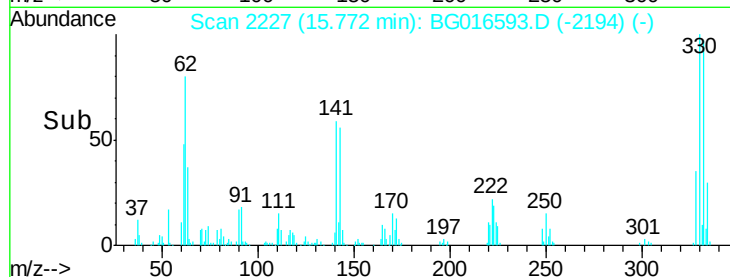
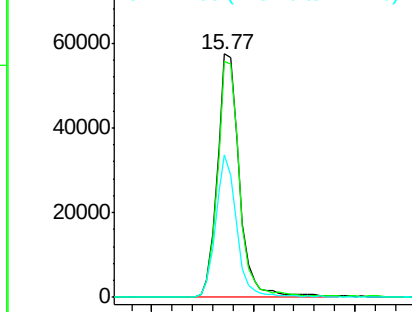



#44
 2-Fluorobiphenyl
 Concen: 84.03 ng
 RT: 12.90 min Scan# 1738
 Delta R.T. -0.00 min
 Lab File: BG016593.D
 Acq: 21 Apr 2015 20:58

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.6	44.4
170	23.9	19.4	29.0

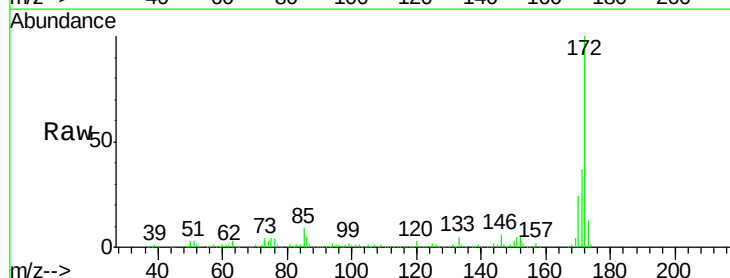

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

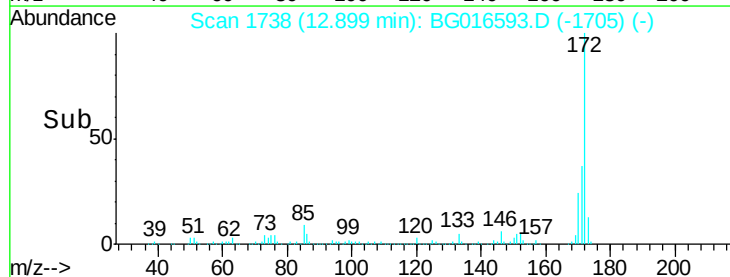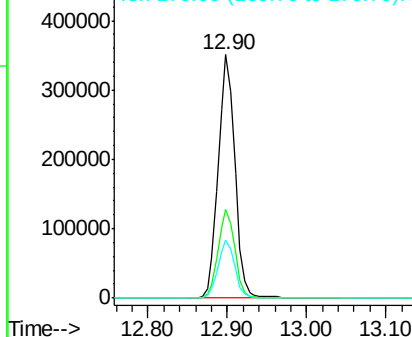


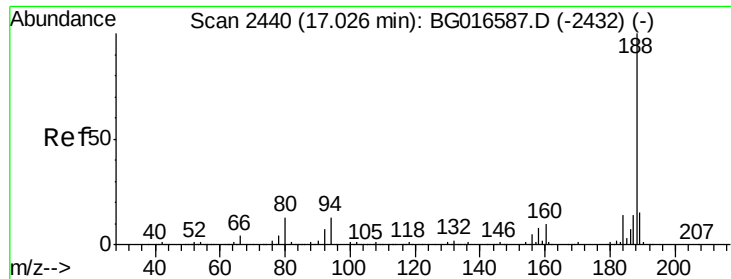




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.02 min Scan# 2440
Delta R.T. -0.00 min
Lab File: BG016593.D
Acq: 21 Apr 2015 20:58

Instrument :
BNA_G
ClientSampleId :
PB82905BL

Tot Ion:188 Resp: 250602
Ion Ratio Lower Upper
188 100
94 13.1 10.5 15.7
80 13.7 10.6 16.0

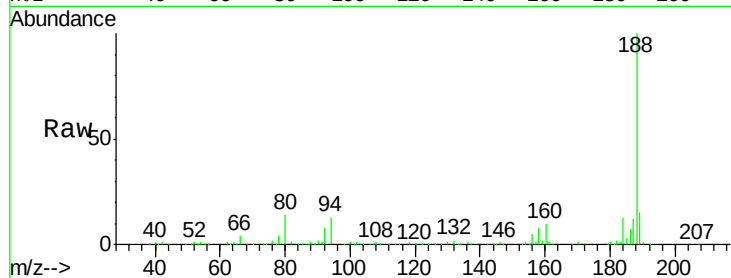


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

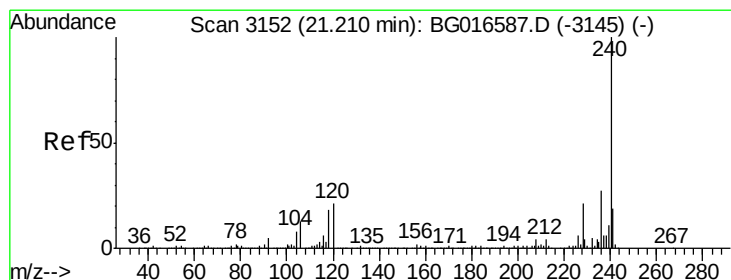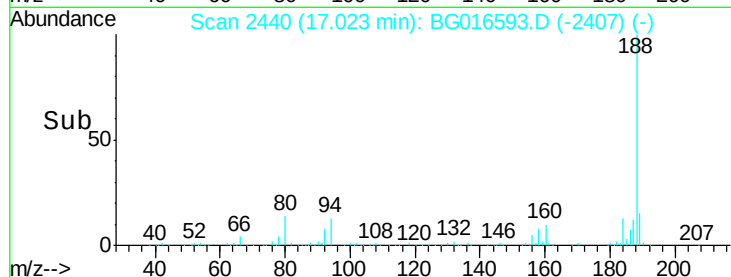
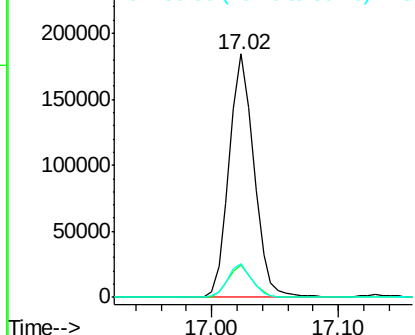



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.21 min Scan# 3152
Delta R.T. -0.00 min
Lab File: BG016593.D
Acq: 21 Apr 2015 20:58

Tgt Ion:240 Resp: 283193
Ion Ratio Lower Upper
240 100
120 19.8 16.7 25.1
236 27.3 21.7 32.5

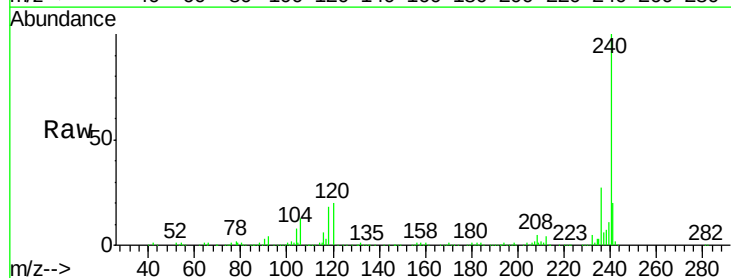

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

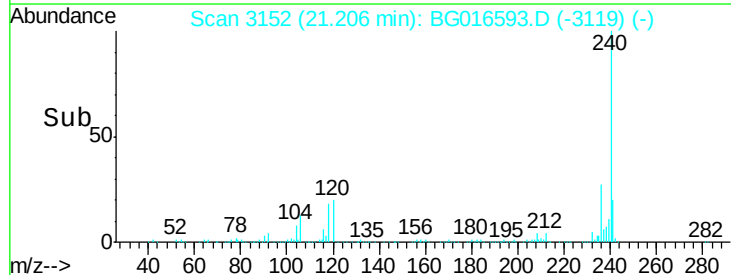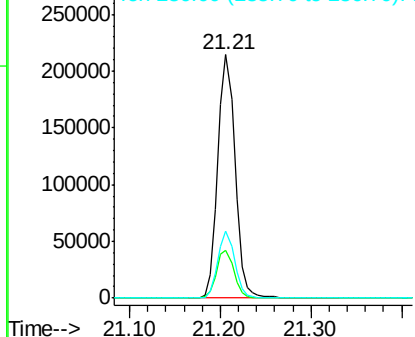

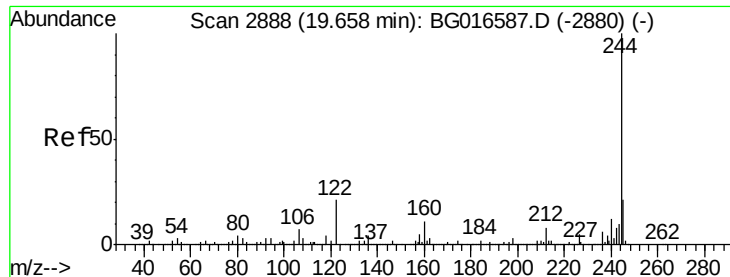

#78

Terphenyl-d14

Concen: 76.84 ng

RT: 19.66 min Scan# 2888

Delta R.T. -0.00 min

Lab File: BG016593.D

Acq: 21 Apr 2015 20:58

Instrument :

BNA_G

ClientSampleId :

PB82905BL


Tot Ion:244 Resp: 903246

Ion Ratio Lower Upper

244 100

212 8.4 6.8 10.2




122 21.4 17.0 25.6

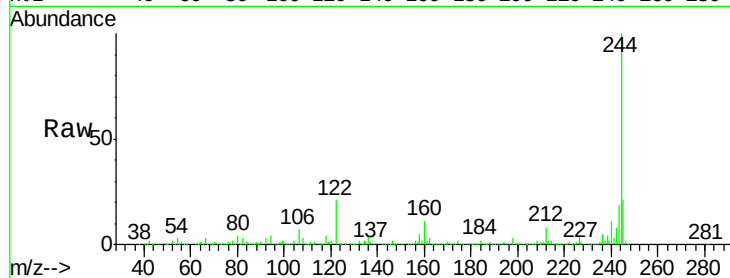

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

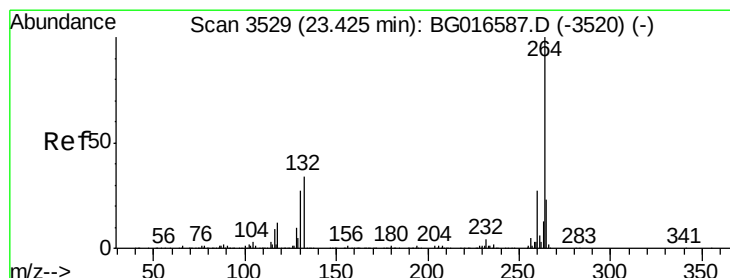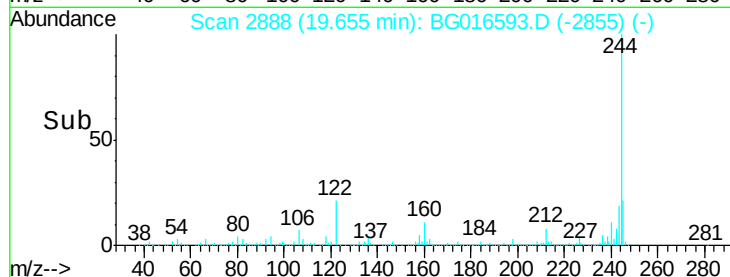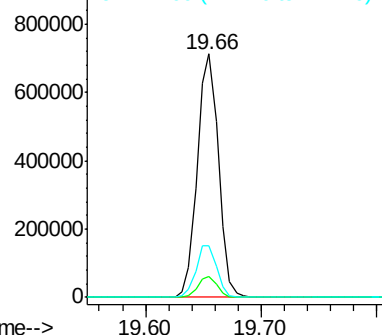

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.43 min Scan# 3530

Delta R.T. 0.00 min

Lab File: BG016593.D

Acq: 21 Apr 2015 20:58


Tgt Ion:264 Resp: 259244

Ion Ratio Lower Upper

264 100

260 25.4 21.4 32.2

265 21.3 18.7 28.1

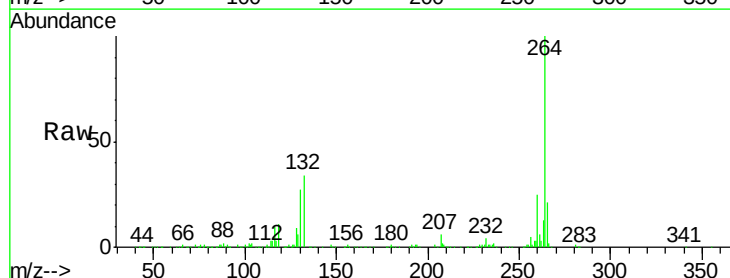

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

