
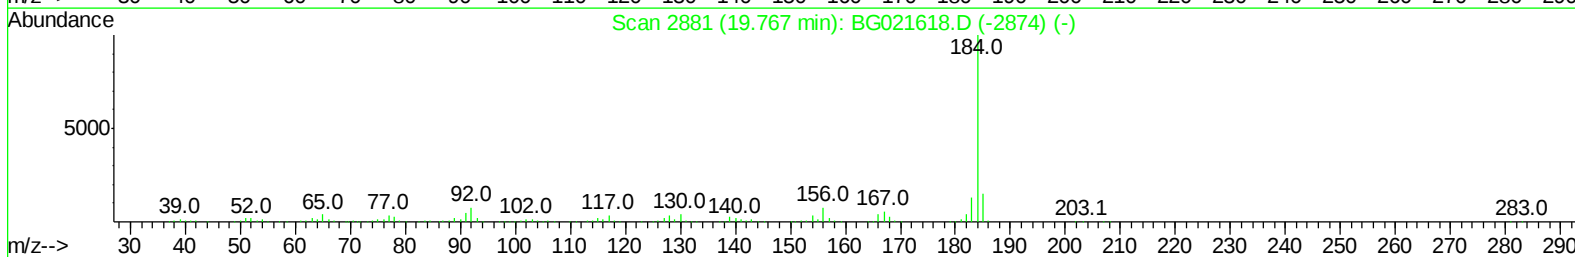
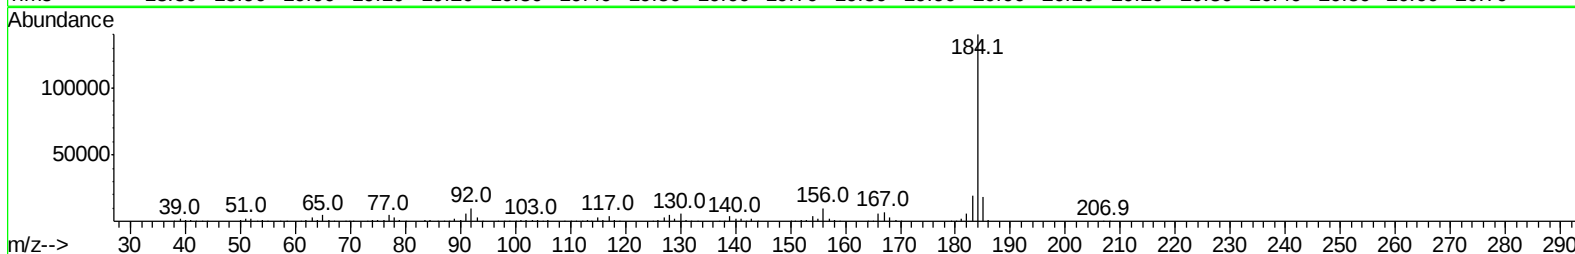


Data Path : U:\HPCHEM1\BNA G\DATA\BG042116\
Data File : BG021777.D
Acq On : 20 Apr 2016 9:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 03:26:56 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

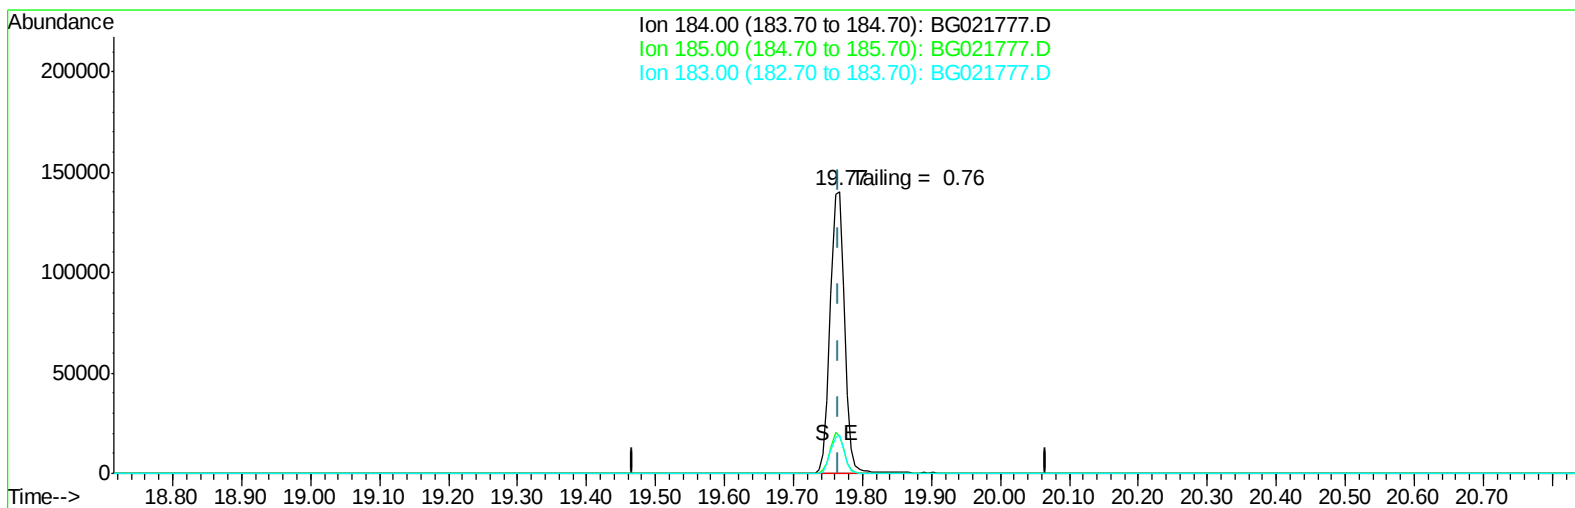

TIC: BG021777.D

(76) Benzidine




19.766min (-0.000) 39832.12ng

response 202151

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.31
183.00	12.80	13.86
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG042116\
Data File : BG021777.D
Acq On : 20 Apr 2016 9:49
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 03:26:56 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

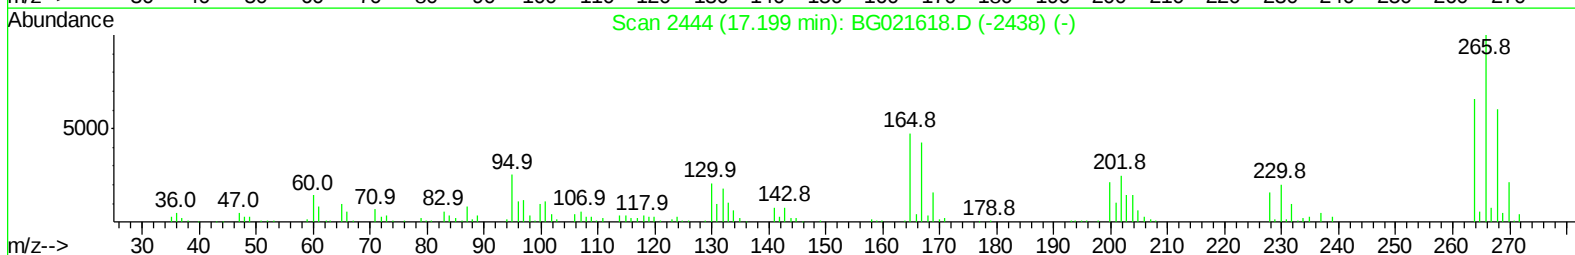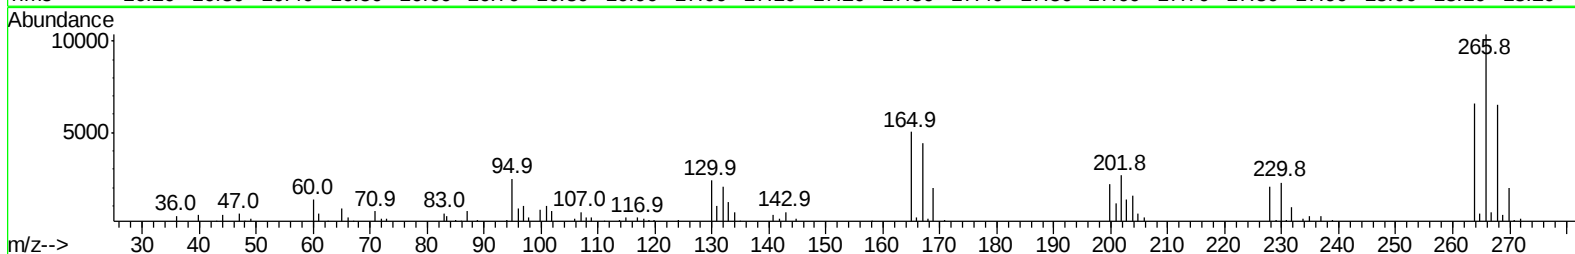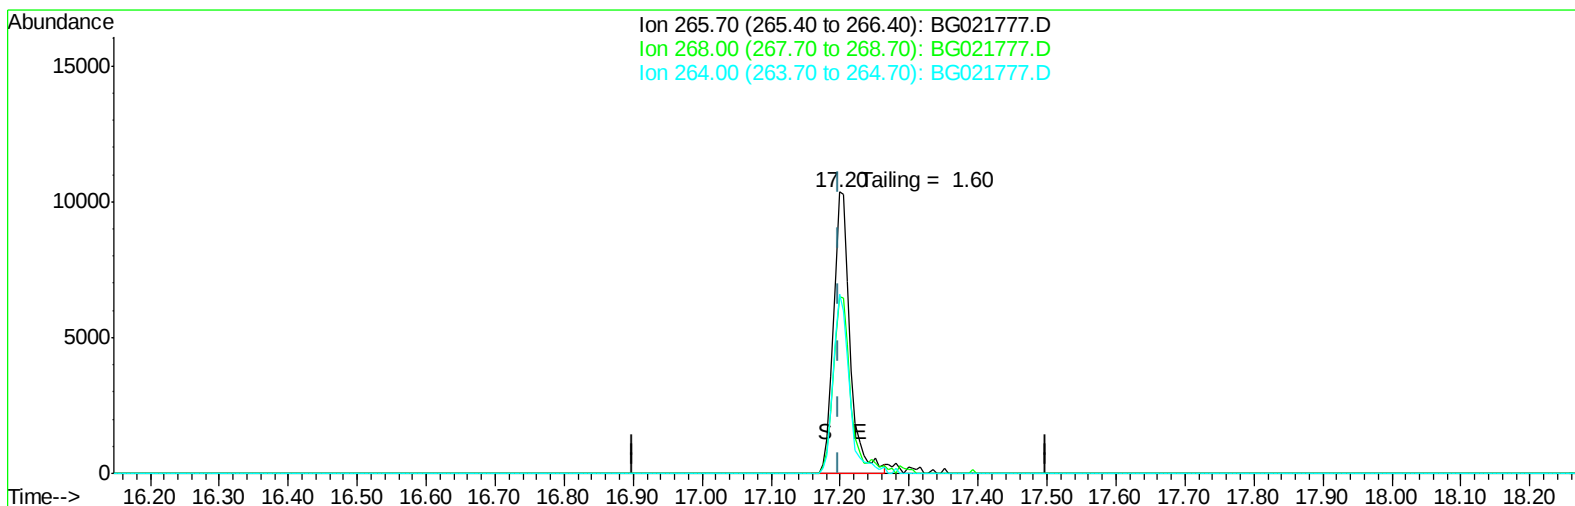

TIC: BG021777.D

(69) Pentachlorophenol (C)

17.199min (-0.000) 0.00ng

response 17590

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	62.60
264.00	67.20	63.42
0.00	0.00	0.00