
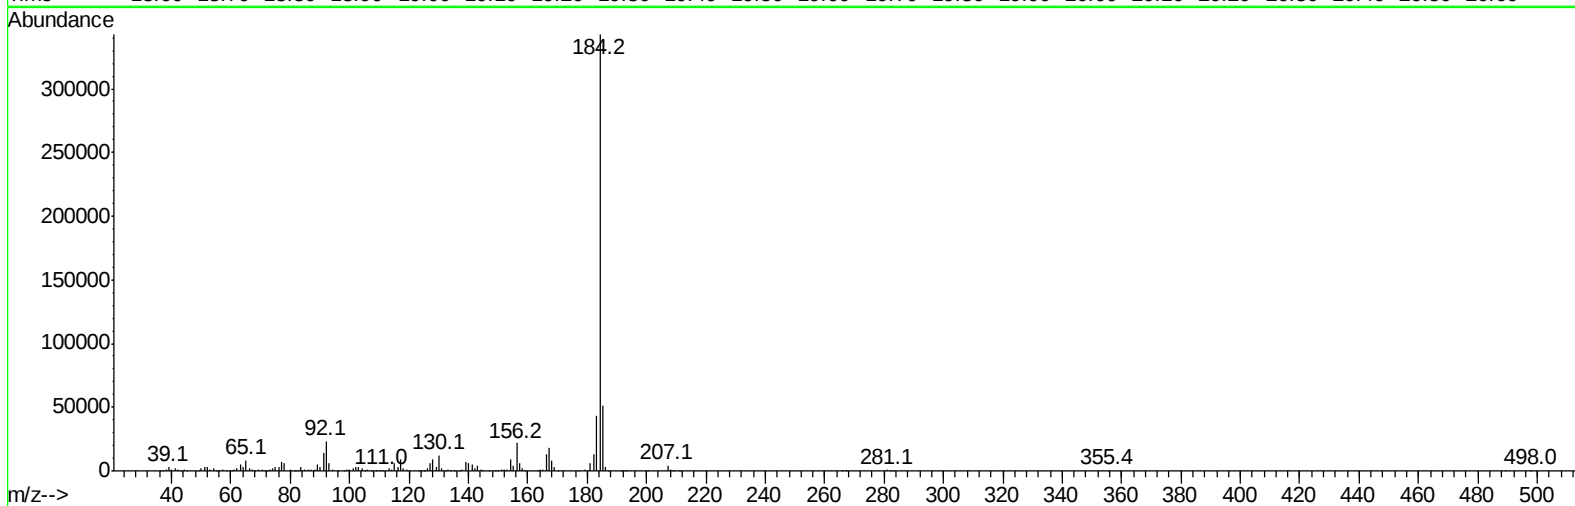


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042117\
Data File : BG026687.D
Acq On : 21 Apr 2017 15:32
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 04:49:43 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

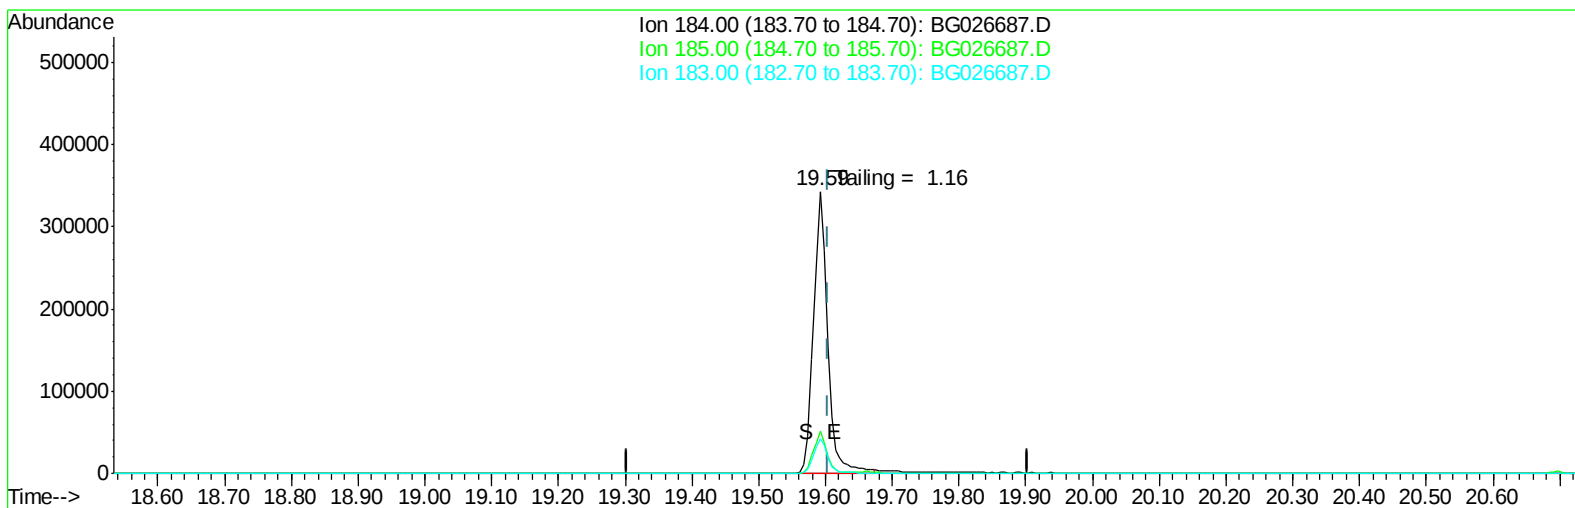

TIC: BG026687.D

(76) Benzidine



19.592min (-0.012) 53632.31ng

response 502743

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.87
183.00	13.80	12.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042117\
Data File : BG026687.D
Acq On : 21 Apr 2017 15:32
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 04:49:43 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 18:04:39 2017
Response via : Initial Calibration

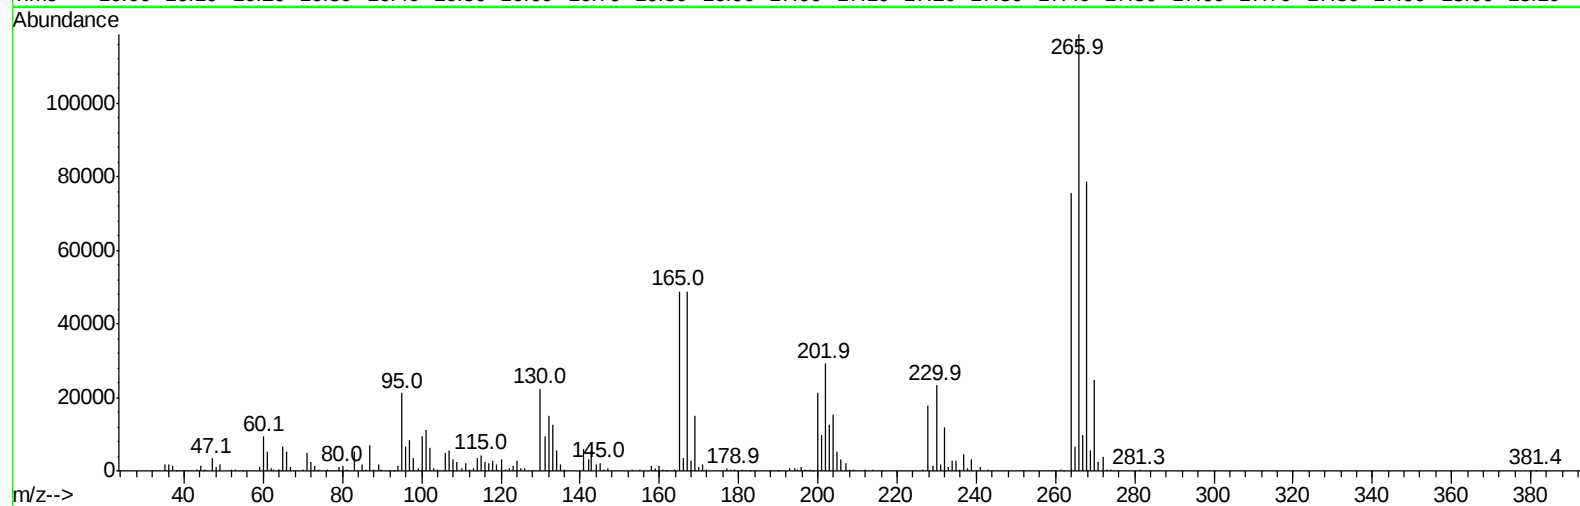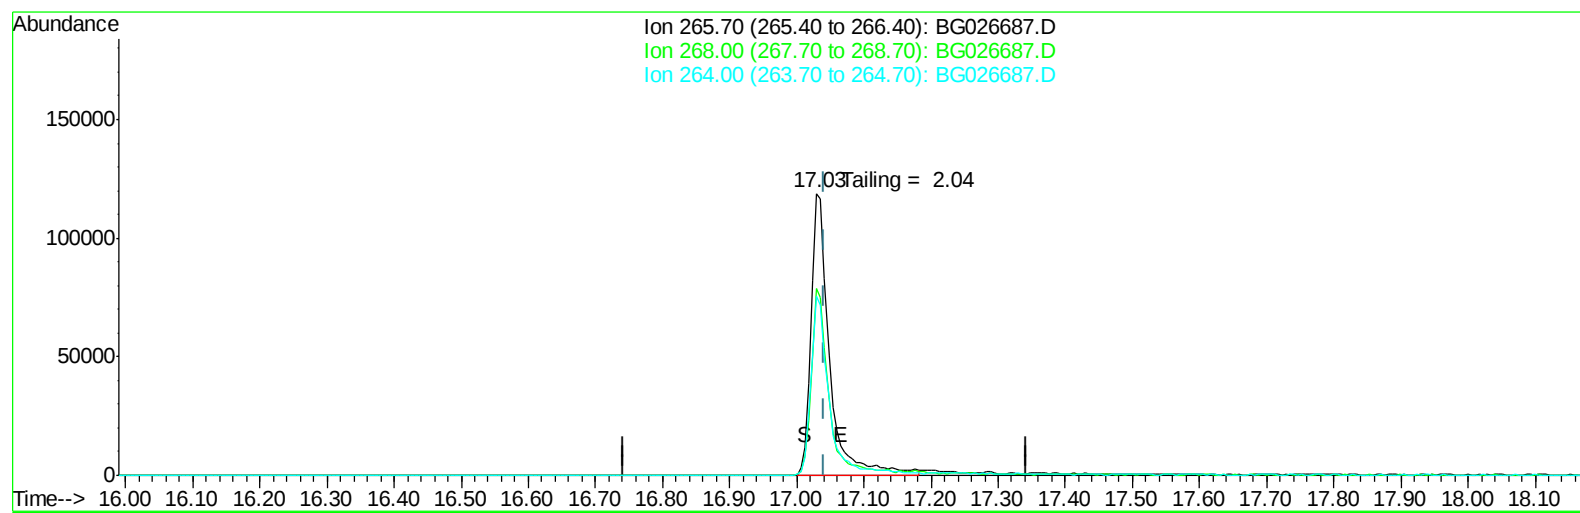

TIC: BG026687.D

(69) Pentachlorophenol (C)

17.030min (-0.013) 278607.77ng

response 226460

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	66.27
264.00	62.60	63.52
0.00	0.00	0.00