

Data Path : Z:\HPCHEM1\BNA G\Data\BG042117\
 Data File : BG026694.D
 Acq On : 21 Apr 2017 20:11
 Operator : SJ/MA
 Sample : I2782-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BLINDDUPLICATE- 42017

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.617	423	430	440	rBV	1071026	1787773	14.41%	3.317%
2	7.215	695	702	718	rBV	654158	1194133	9.63%	2.215%
3	7.568	755	762	773	rBV	2100210	3679353	29.66%	6.826%
4	8.032	834	841	852	rVB	521798	907102	7.31%	1.683%
5	8.355	886	896	904	rBV	1932028	3420691	27.57%	6.346%
6	9.189	1030	1038	1051	rBV	1463742	2673721	21.55%	4.960%
7	10.829	1309	1317	1329	rBV	764440	1406408	11.34%	2.609%
8	13.267	1724	1732	1741	rBV	5035309	7726628	62.28%	14.334%
9	14.636	1958	1965	1976	rBV2	1284516	2096671	16.90%	3.890%
10	16.122	2209	2218	2233	rBV	4173451	6621537	53.37%	12.284%
11	17.368	2423	2430	2441	rBV2	1827652	2865095	23.09%	5.315%
12	18.249	2576	2580	2588	rBV2	76248	145806	1.18%	0.270%
13	19.518	2791	2796	2801	rBV2	86206	149267	1.20%	0.277%
14	19.971	2866	2873	2882	rBV	8871261	12405870	100.00%	23.015%
15	21.616	3146	3153	3162	rBV	2078804	3375875	27.21%	6.263%
16	24.789	3682	3693	3706	rBV2	1168822	3447103	27.79%	6.395%


Sum of corrected areas: 53903033

Data Path : Z:\HPCHEM1\BNA G\Data\BG042117\
Data File : BG026694.D
Acq On : 21 Apr 2017 20:11
Operator : SJ/MA
Sample : I2782-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BLINDDUPLICATE- 42017

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

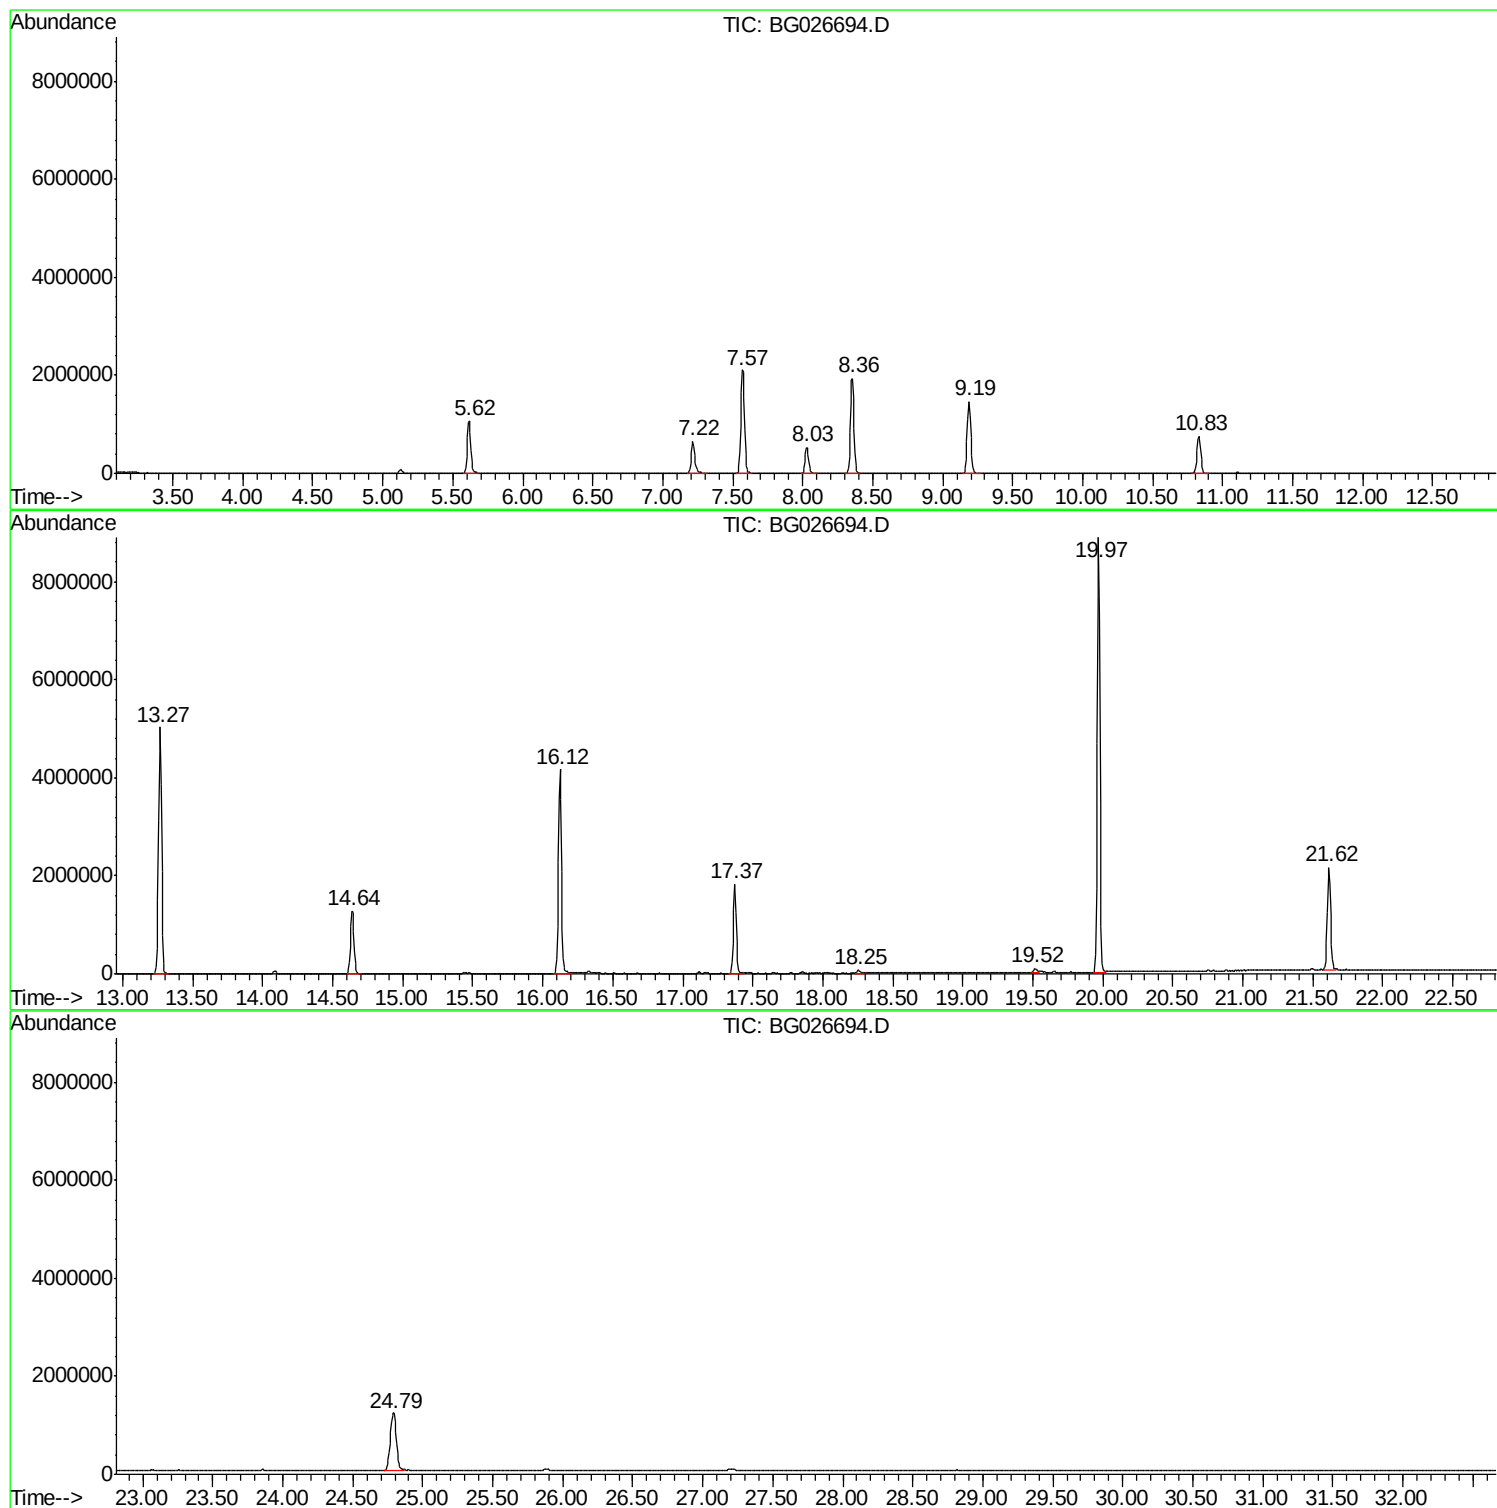

Data Path : Z:\HPCHEM1\BNA G\Data\BG042117\
Data File : BG026694.D
Acq On : 21 Apr 2017 20:11
Operator : SJ/MA
Sample : I2782-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BLINDDUPLICATE- 42017










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.57	81.12 ng	3679350	1,4-Dichlorobenzene-d4	8.03

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

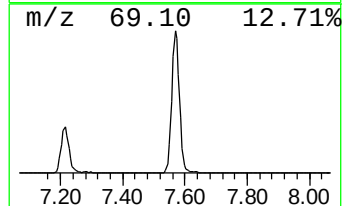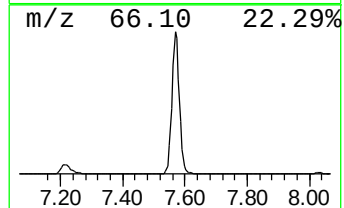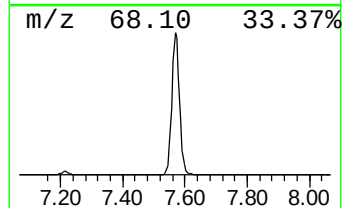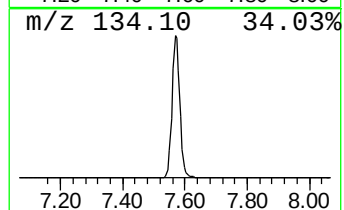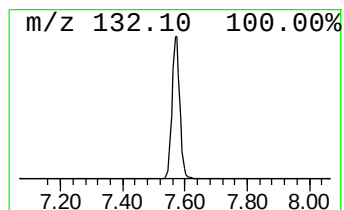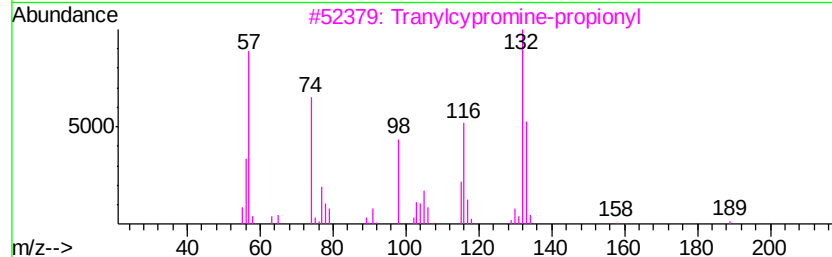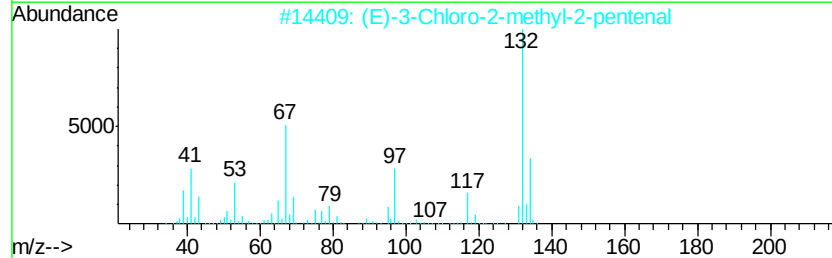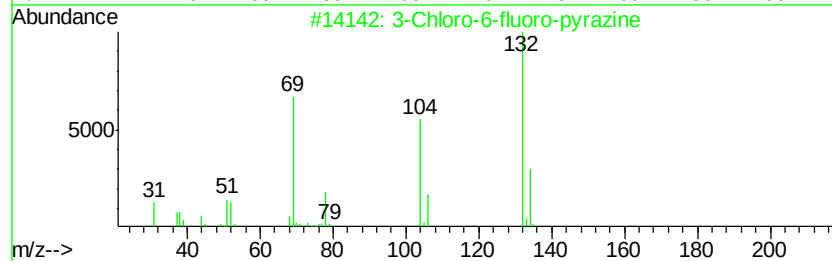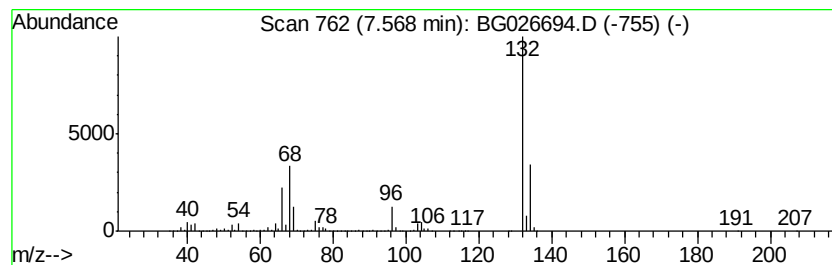

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042117\
Data File : BG026694.D
Acq On : 21 Apr 2017 20:11
Operator : SJ/MA
Sample : I2782-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BLINDDUPLICATE- 42017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.57	7.57	81.1	ng	3679350	1	8.03	907102	20.0