


Data Path : Z:\HPCHEM1\BNA G\Data\BG042117\
 Data File : BG026687.D
 Acq On : 21 Apr 2017 15:32
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 18 18:04:39 2017

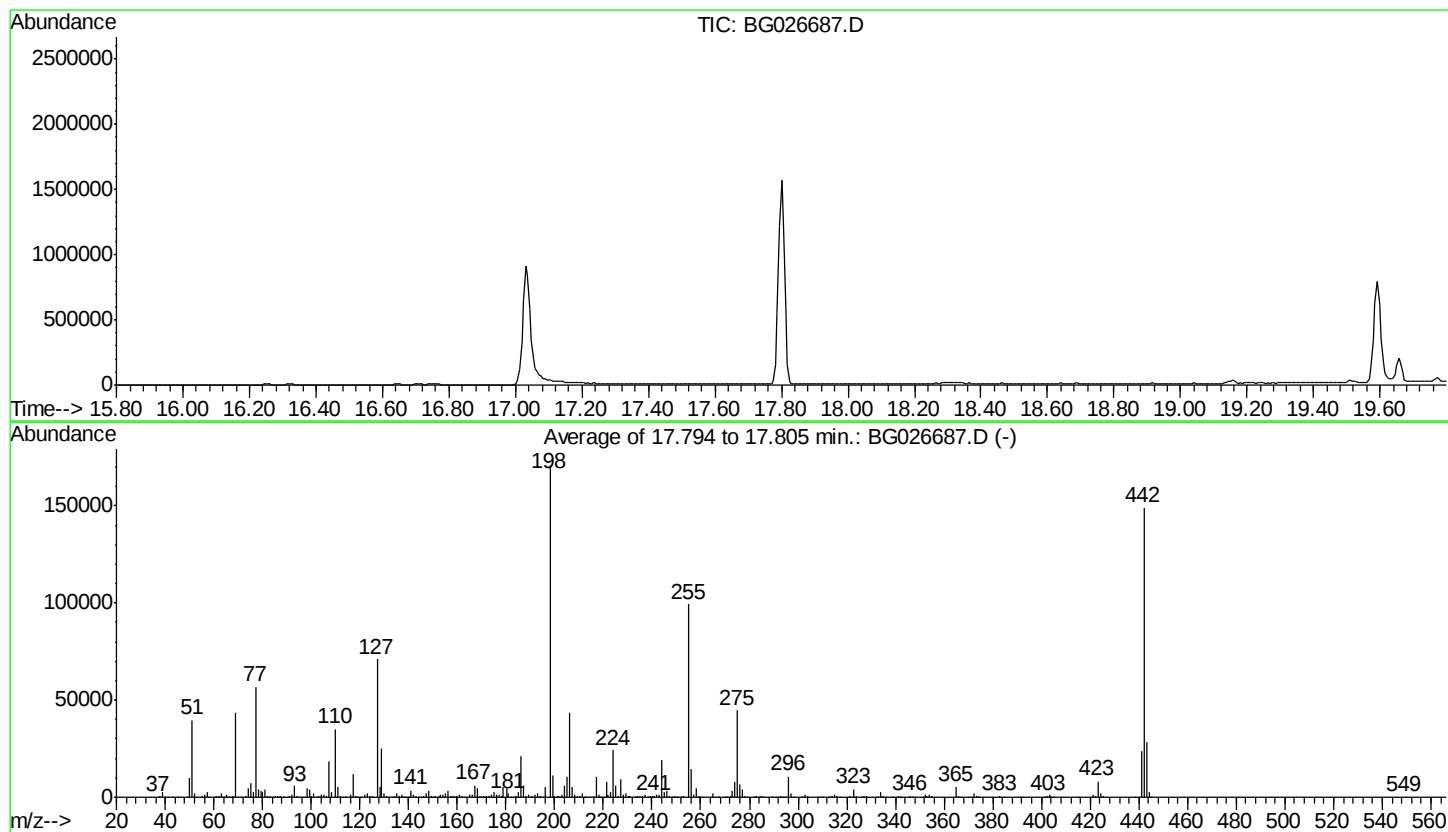

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	39857	PASS
68	69	0.00	2	1.5	630	PASS
69	198	0.00	100	25.4	43290	PASS
70	69	0.00	2	0.7	305	PASS
127	198	10	80	41.6	70994	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	170688	PASS
199	198	5	9	6.6	11264	PASS
275	198	10	60	26.1	44520	PASS
365	198	1	100	3.1	5353	PASS
441	442	0.01	24	15.8	23482	PASS
442	198	50	100	87.3	149018	PASS
443	442	15	24	19.2	28672	PASS