

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
 Data File : BG048814.D
 Acq On : 21 Apr 2021 10:22
 Operator : CG/JU
 Sample : PB135874TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB135874TB

Quant Time: Apr 21 11:22:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	17437	20.00	ng	0.00
21) Naphthalene-d8	10.89	136	68677	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	48709	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	126925	20.00	ng	0.00
76) Chrysene-d12	21.77	240	140893	20.00	ng	0.00
86) Perylene-d12	25.10	264	134345	20.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.61	112	146963	140.96	ng	0.00
7) Phenol-d6	7.23	99	183506	124.44	ng	0.00
23) Nitrobenzene-d5	9.23	82	140546	91.62	ng	0.00
42) 2,4,6-Tribromophenol	16.22	330	86103	131.84	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	313750	93.02	ng	0.00
79) Terphenyl-d14	20.09	244	674183	82.36	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	9.24	70	22270	22.384	ng	# 66
41) Hexachlorocyclopentadiene	12.76	237	63	5.927	ng	# 31
51) 2,6-Dinitrotoluene	14.72	165	6485	7.693	ng	# 10
57) 2,4-Dinitrotoluene	14.72	165	6485	5.298	ng	# 15
67) 4-Bromophenyl-phenylether	16.22	248	6719	4.599	ng	# 1
77) Benzidine	20.09	184	12650	3.306	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
Data File : BG048814.D
Acq On : 21 Apr 2021 10:22
Operator : CG/JU
Sample : PB135874TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135874TB

Quant Time: Apr 21 11:22:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

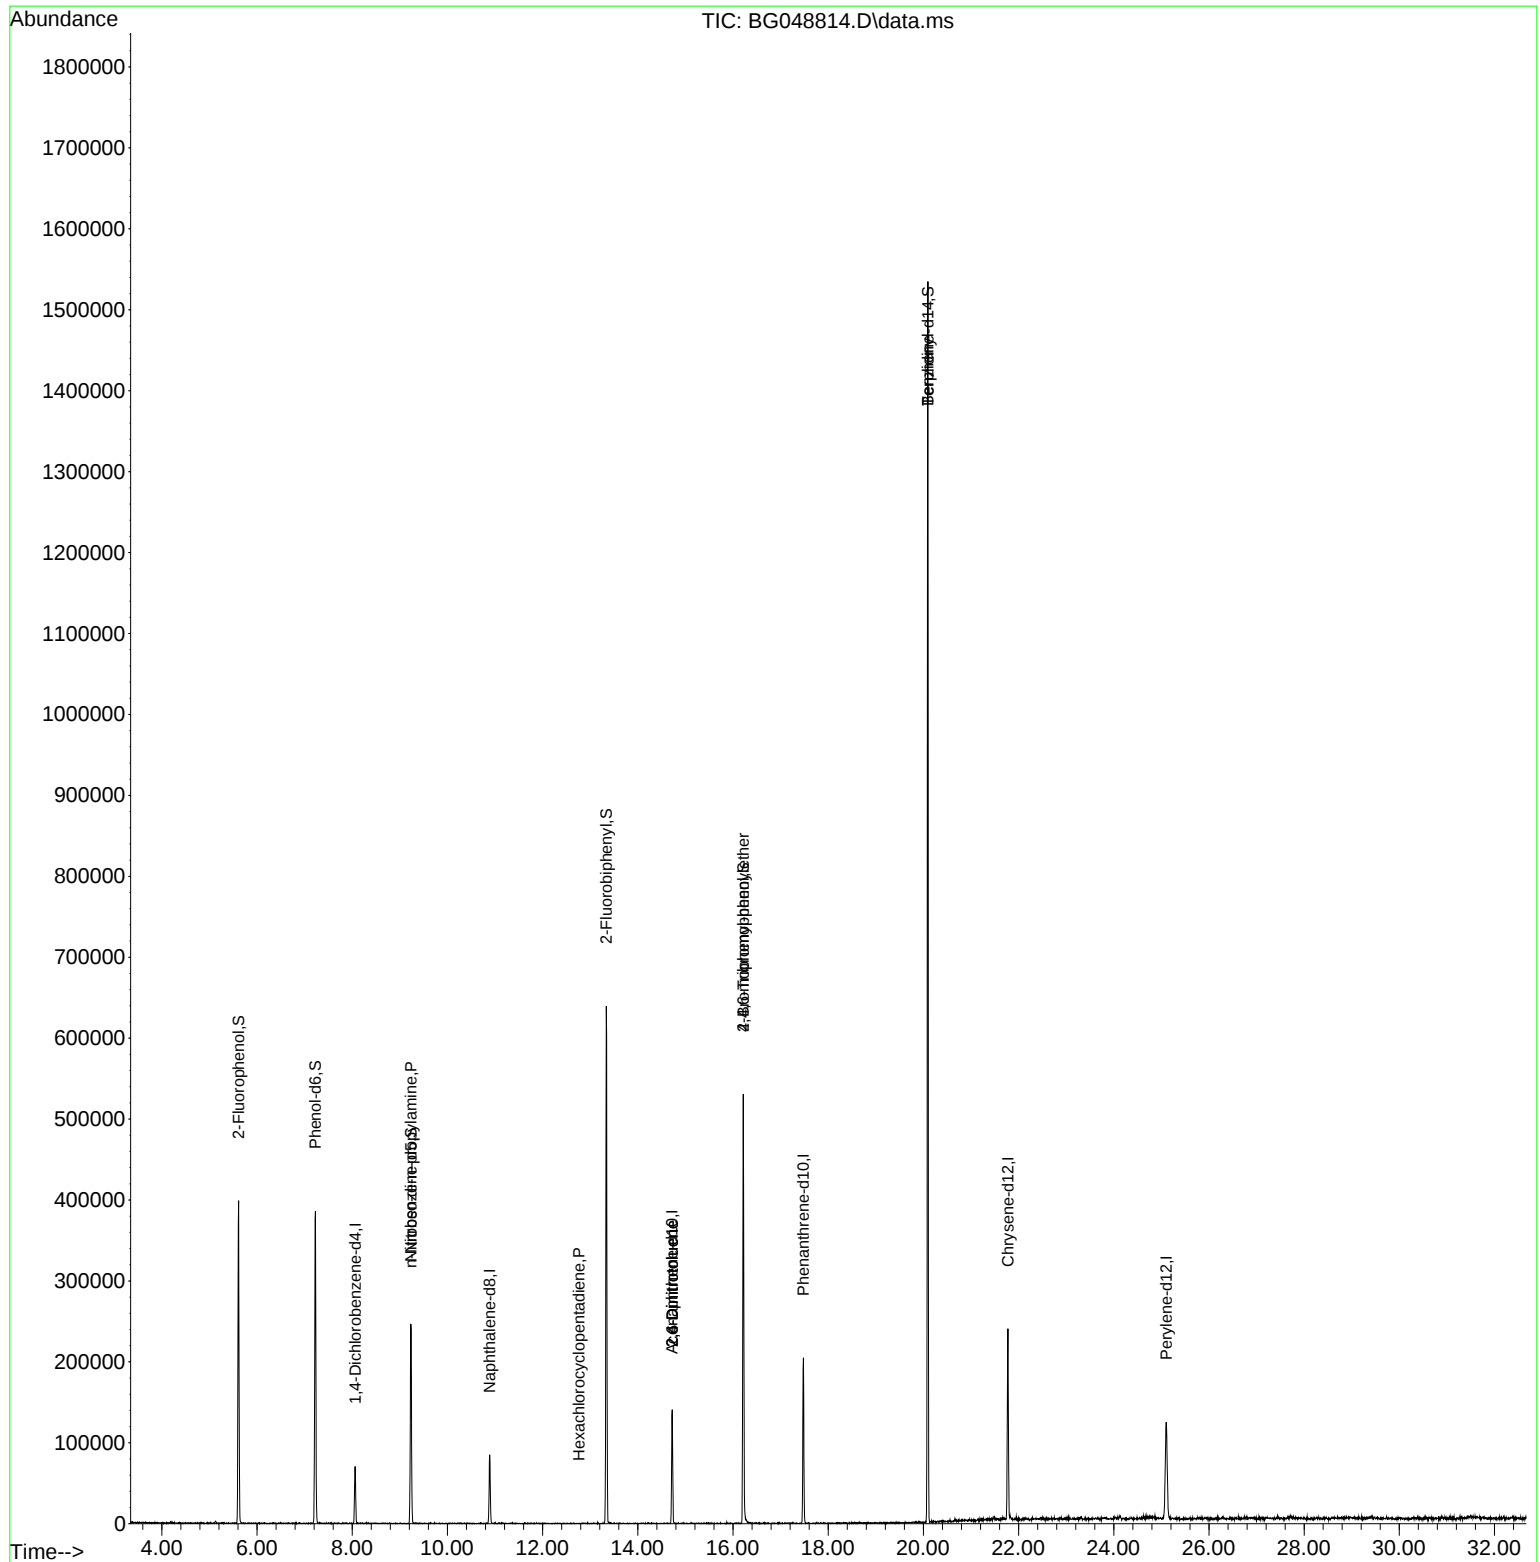

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng

Instrument :
BNA_G
ClientSampleId :
PB135874TB