
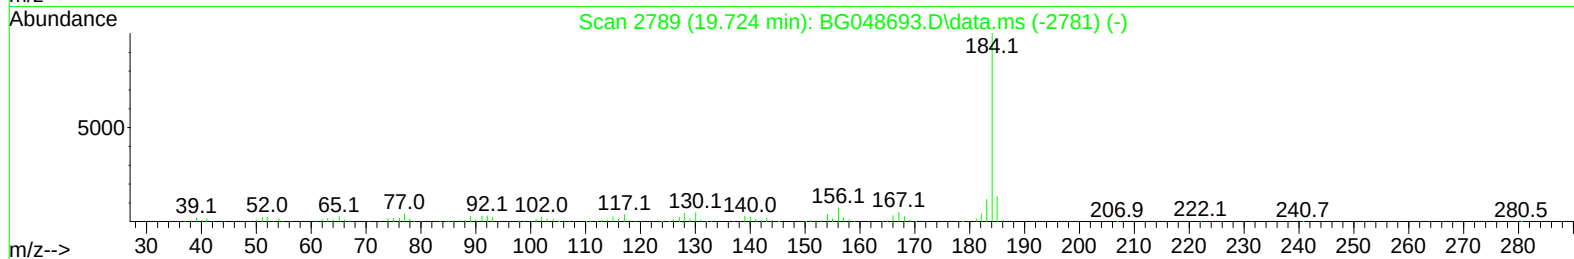
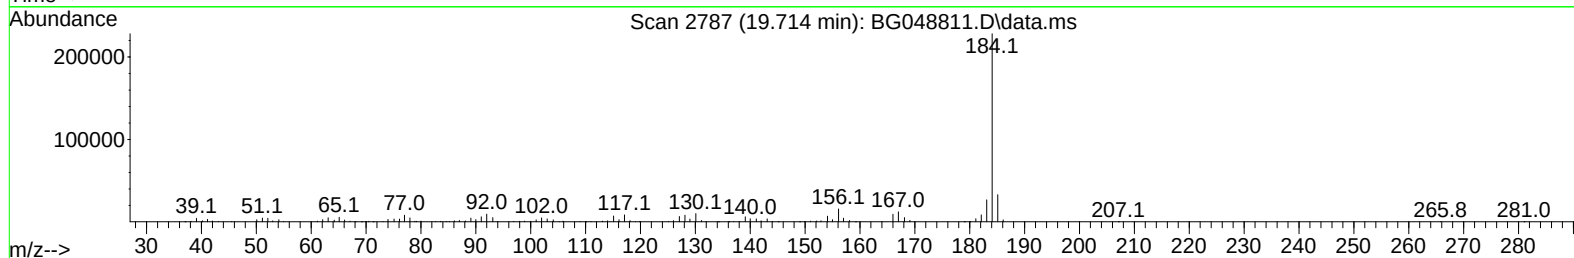


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
Data File : BG048811.D
Acq On : 21 Apr 2021 8:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 11:13:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

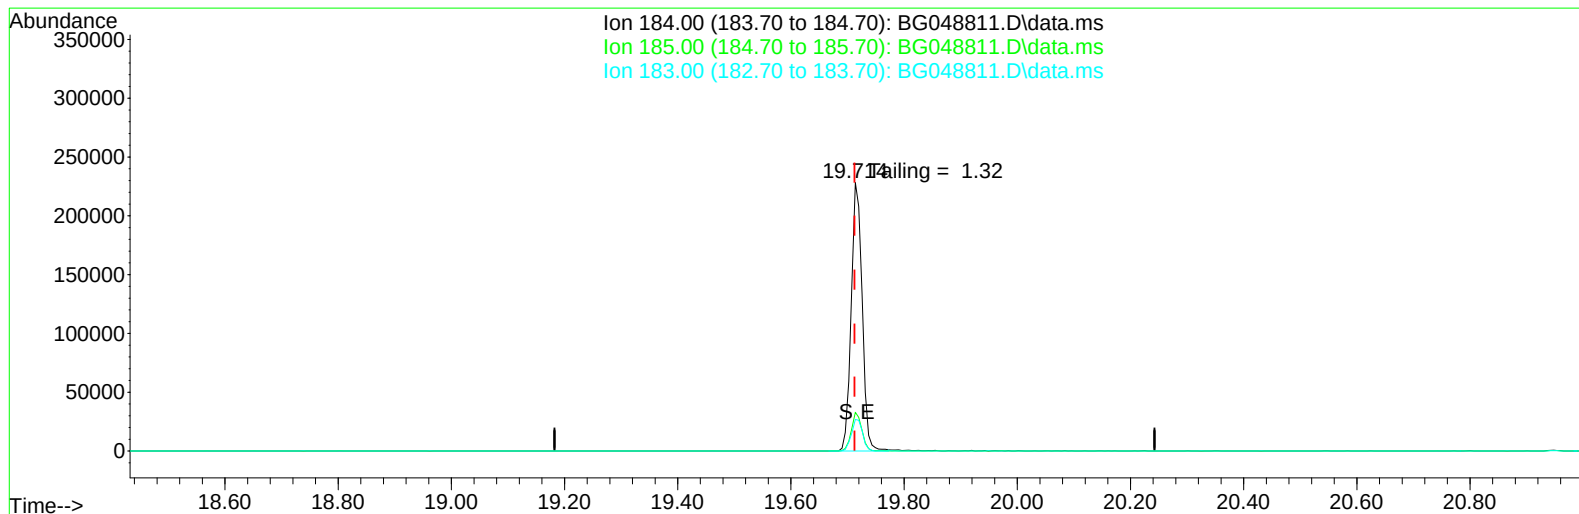




TIC: BG048811.D\data.ms

(77) Benzidine**19.714min (+ 0.002) 192389.13 ng****response 308250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.43
183.00	11.70	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
Data File : BG048811.D
Acq On : 21 Apr 2021 8:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 11:13:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

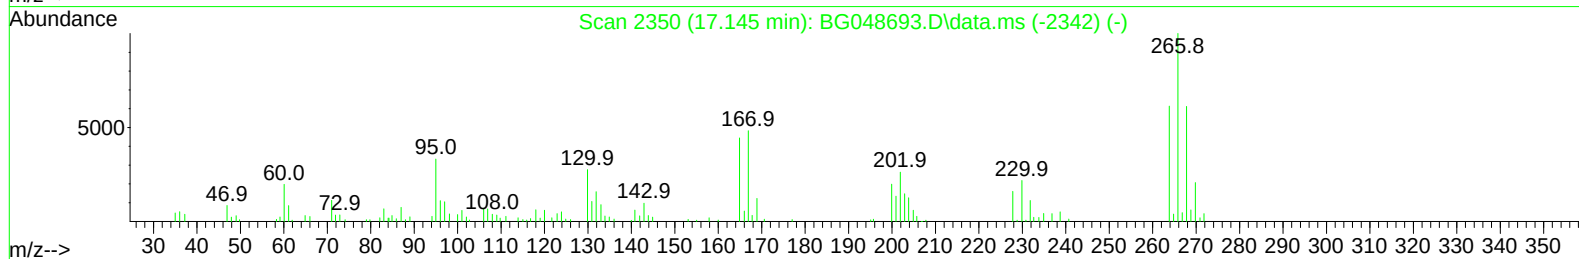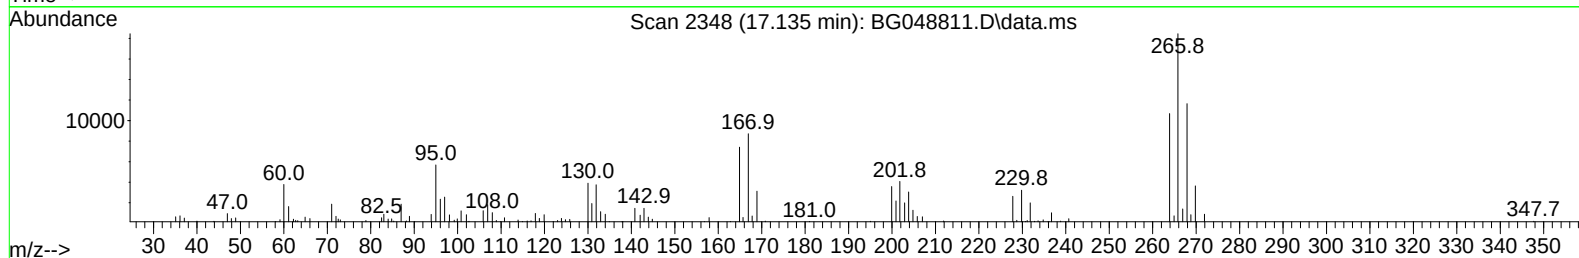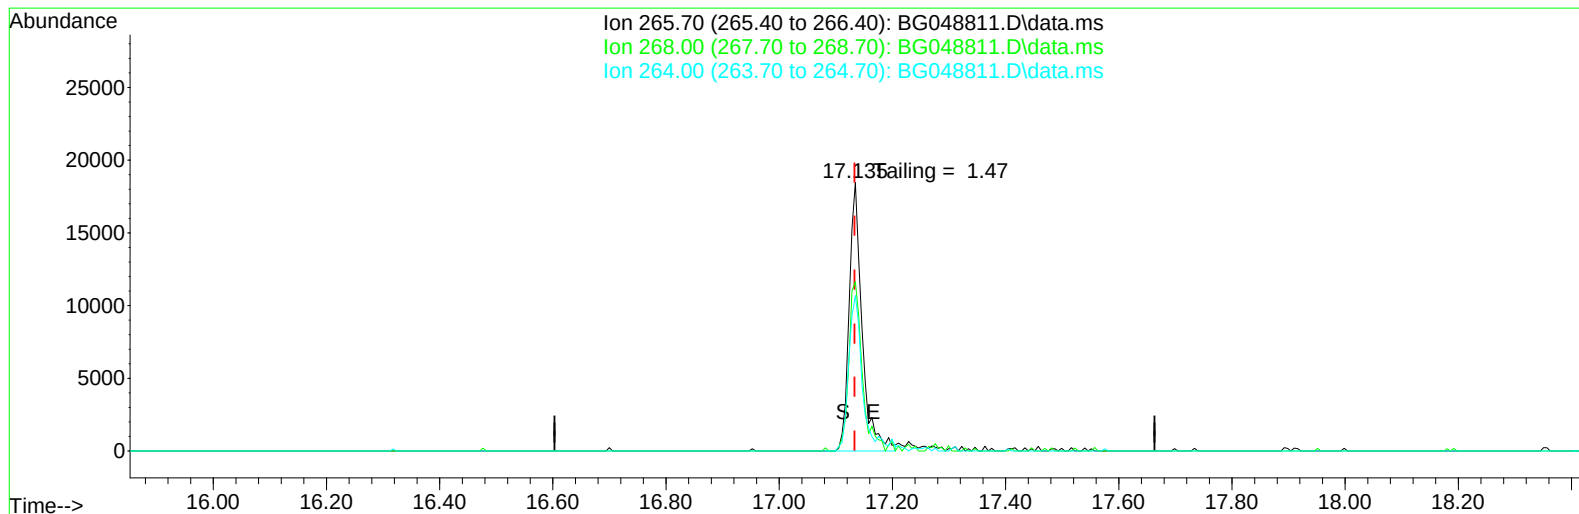

TIC: BG048811.D\data.ms

(70) Pentachlorophenol (C)

17.135min (+ 0.002) 31379.82 ng

response 28851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.09
264.00	61.30	57.89
0.00	0.00	0.00