

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
 Data File : BG048819.D
 Acq On : 21 Apr 2021 14:31
 Operator : CG/JU
 Sample : M2090-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SEDGWICK-COMP-4

Quant Time: Apr 21 15:20:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.062	152	18490	20.00	ng	# 0.00
21) Naphthalene-d8	10.888	136	71011	20.00	ng	# 0.00
39) Acenaphthene-d10	14.725	164	48150	20.00	ng	0.00
64) Phenanthrene-d10	17.474	188	127057	20.00	ng	# 0.00
76) Chrysene-d12	21.775	240	133707	20.00	ng	0.00
86) Perylene-d12	25.101	264	129413	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.612	112	155479	140.64	ng	0.00
7) Phenol-d6	7.228	99	171707	109.81	ng	0.00
23) Nitrobenzene-d5	9.237	82	165825	104.55	ng	0.00
42) 2,4,6-Tribromophenol	16.217	330	107892	167.12	ng	0.00
45) 2-Fluorobiphenyl	13.338	172	357920	107.35	ng	0.00
79) Terphenyl-d14	20.095	244	758443	97.63	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.166	163	10023	2.78	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
Data File : BG048819.D
Acq On : 21 Apr 2021 14:31
Operator : CG/JU
Sample : M2090-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4

Quant Time: Apr 21 15:20:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration




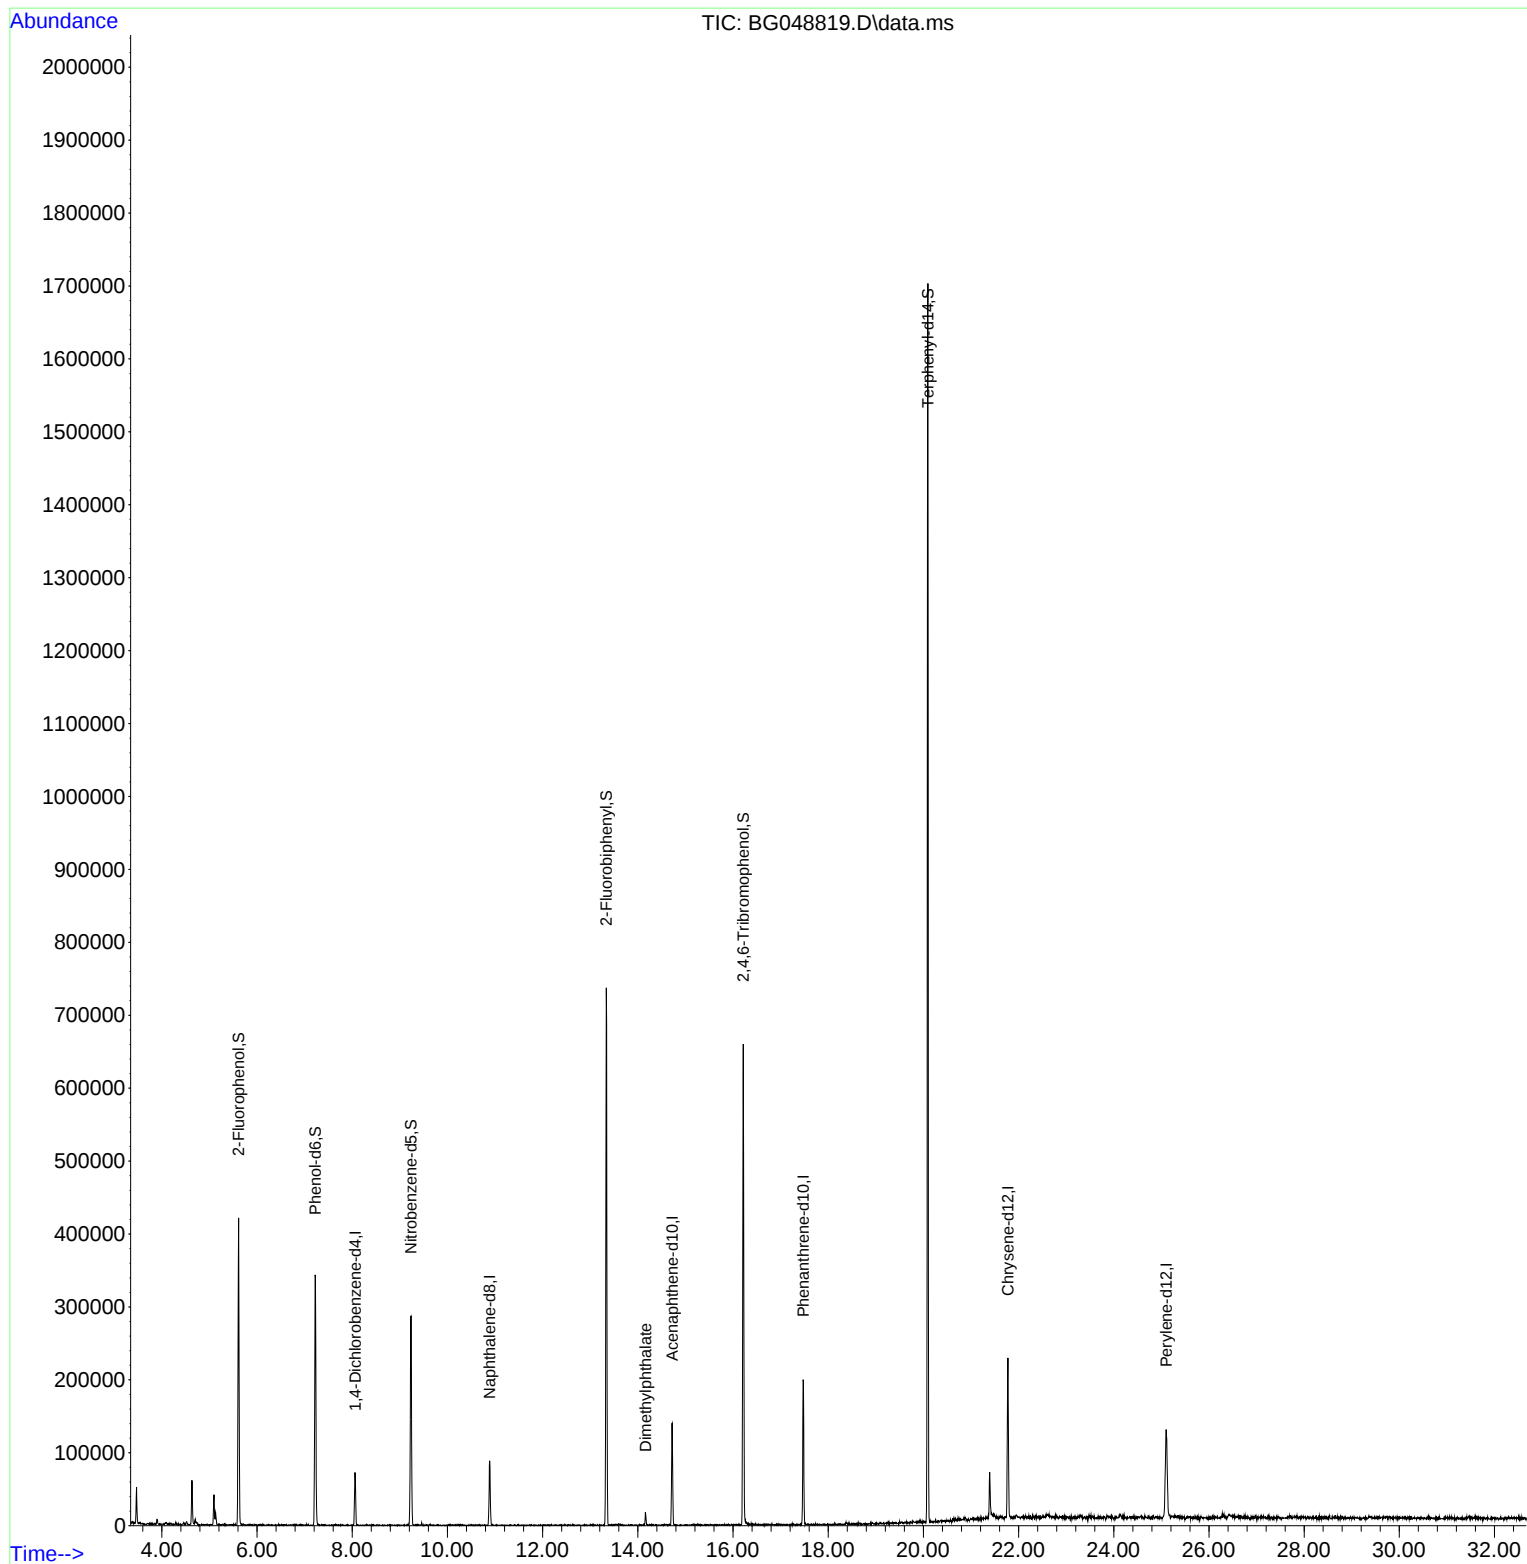




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.062 min Scan# 804
Delta R.T. 0.001 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31




Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4


Tgt Ion:152 Resp: 18490
Ion Ratio Lower Upper
152 100
150 153.6 119.4 179.0
115 50.8 60.2 90.4#

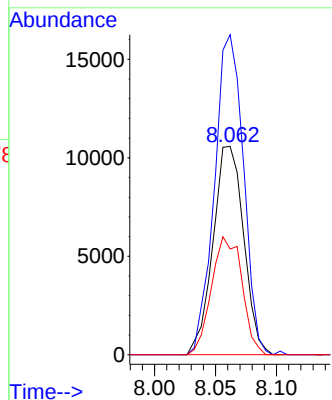

#5
2-Fluorophenol
Concen: 140.64 ng
RT: 5.612 min Scan# 387
Delta R.T. 0.007 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Tgt Ion:112 Resp: 155479
Ion Ratio Lower Upper
112 100
64 61.5 46.7 70.1
63 40.1 35.3 52.9


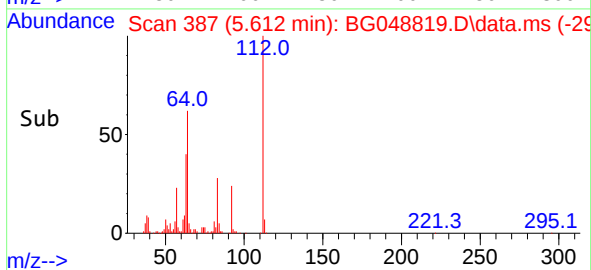
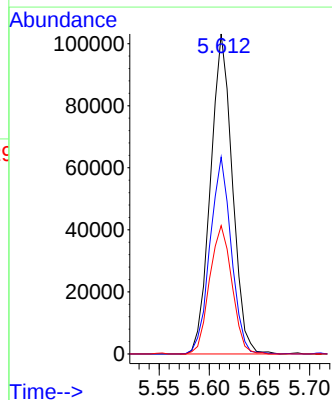





#7
Phenol-d6
Concen: 109.81 ng
RT: 7.228 min Scan# 662
Delta R.T. 0.007 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31




Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4


Tgt Ion: 99 Resp: 171707
Ion Ratio Lower Upper
99 100
42 24.7 20.5 30.7
71 48.7 41.5 62.3

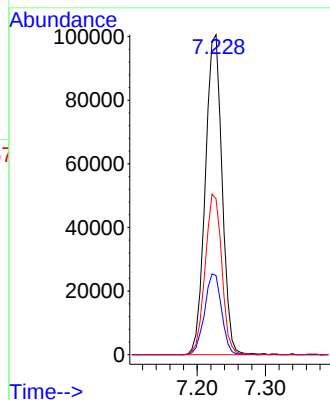

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.888 min Scan# 1285
Delta R.T. -0.005 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Tgt Ion: 136 Resp: 71011
Ion Ratio Lower Upper
136 100
137 11.2 8.2 12.2
54 7.5 5.5 8.3
68 4.3 2.3 3.5#


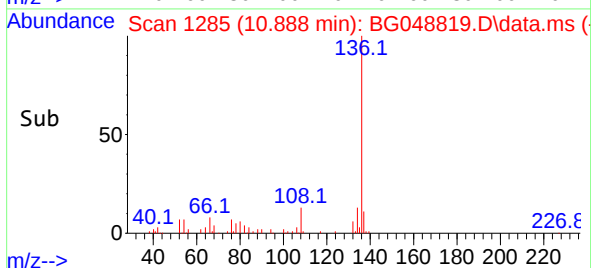
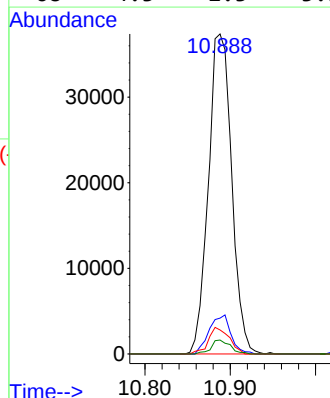



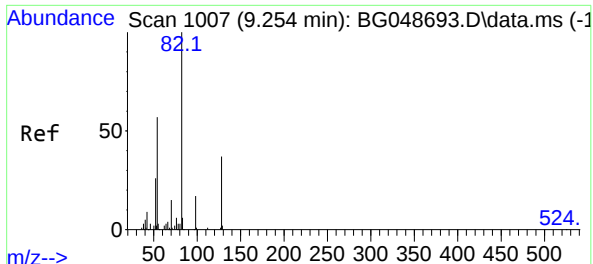

#23
Nitrobenzene-d5
Concen: 104.55 ng
RT: 9.237 min Scan# 1004
Delta R.T. 0.001 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31




Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4


Tgt Ion: 82 Resp: 165825
Ion Ratio Lower Upper
82 100
128 35.2 29.8 44.6
54 57.6 45.8 68.8

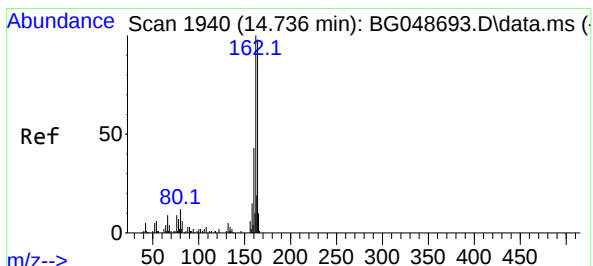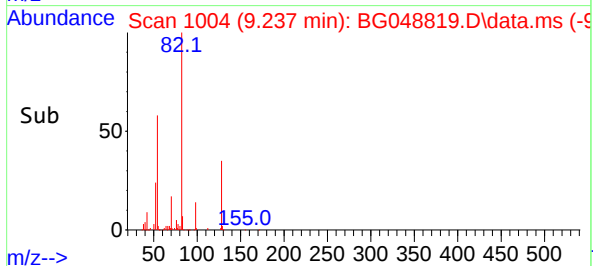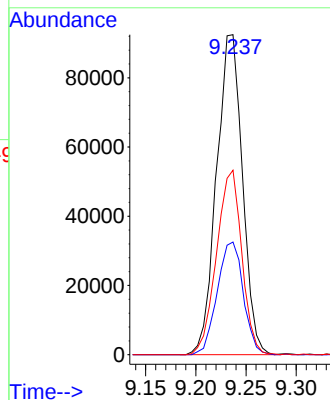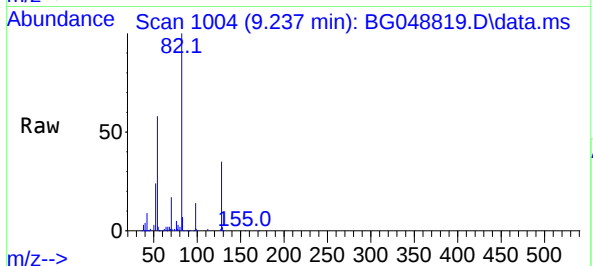

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.725 min Scan# 1938
Delta R.T. 0.001 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Tgt Ion:164 Resp: 48150
Ion Ratio Lower Upper
164 100
162 92.3 81.4 122.0
160 39.7 34.9 52.3


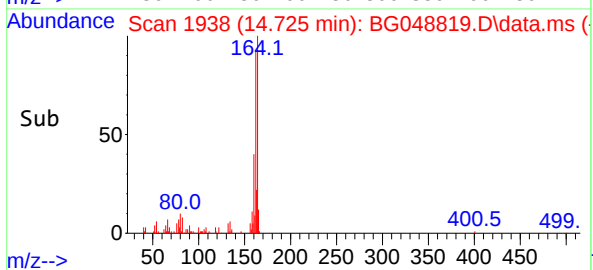
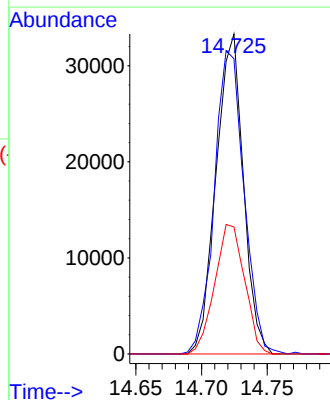
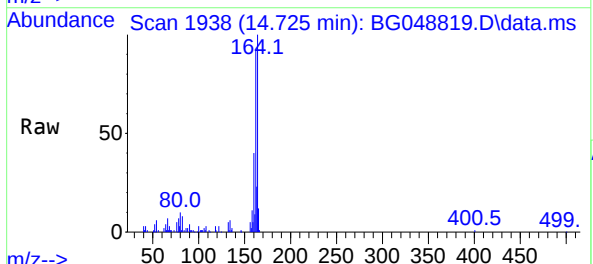




#42
2,4,6-Tribromophenol
Concen: 167.12 ng
RT: 16.217 min Scan# 2192
Delta R.T. 0.001 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31




Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4


Tgt Ion:330 Resp: 107892
Ion Ratio Lower Upper
330 100
332 96.6 77.3 115.9
141 45.6 35.6 53.4

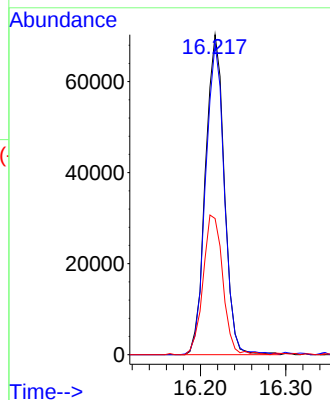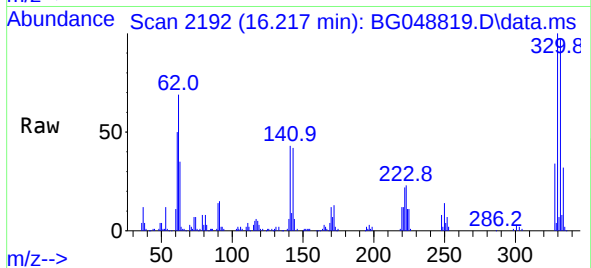

#45
2-Fluorobiphenyl
Concen: 107.35 ng
RT: 13.338 min Scan# 1702
Delta R.T. -0.005 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Tgt Ion:172 Resp: 357920
Ion Ratio Lower Upper
172 100
171 35.0 28.6 43.0
170 21.7 18.6 27.8


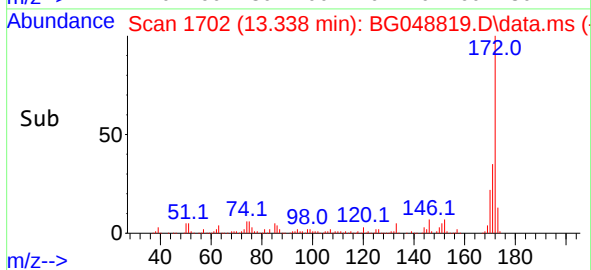
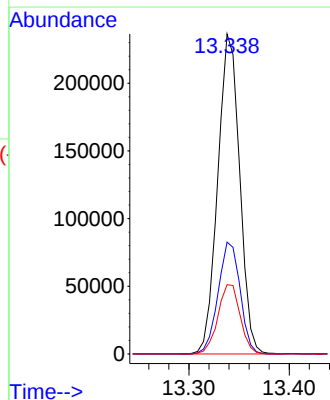





#50
Dimethylphthalate
Concen: 2.78 ng
RT: 14.166 min Scan# 1843
Delta R.T. -0.005 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31




Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4


Tgt Ion:163	Resp:	10023
Ion Ratio	Lower	Upper
163	100	
194	3.9	3.0 4.6
164	8.9	8.6 12.8

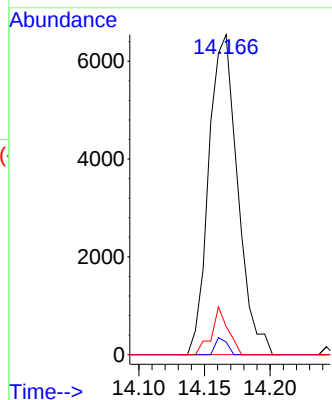

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.474 min Scan# 2406
Delta R.T. -0.005 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Tgt Ion:188	Resp:	127057
Ion Ratio	Lower	Upper
188	100	
94	5.1	5.4 8.0#
80	4.7	3.7 5.5

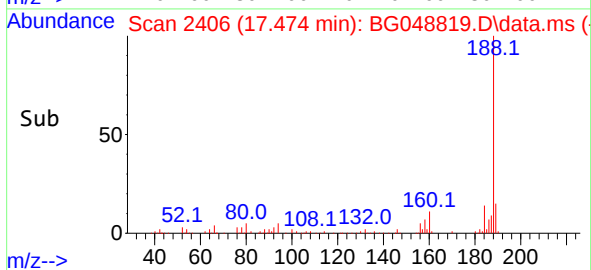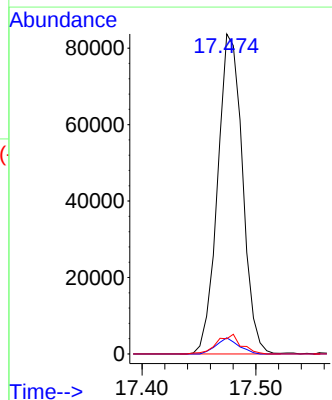







#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.775 min Scan# 3138
Delta R.T. -0.005 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Instrument :
BNA_G
ClientSampleId :
SEDGWICK-COMP-4

Tgt Ion:240 Resp: 133707




Ion	Ratio	Lower	Upper
240	100		
120	5.2	4.2	6.2
236	25.3	21.8	32.6

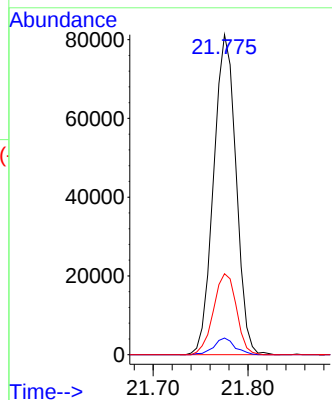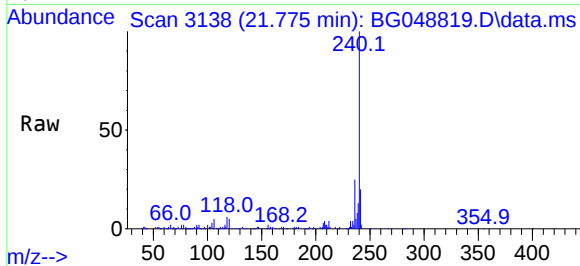


#79
Terphenyl-d14
Concen: 97.63 ng
RT: 20.095 min Scan# 2852
Delta R.T. 0.001 min
Lab File: BG048819.D
Acq: 21 Apr 2021 14:31

Tgt Ion:244 Resp: 758443


Ion	Ratio	Lower	Upper
244	100		
212	8.1	6.9	10.3
122	5.7	5.0	7.6

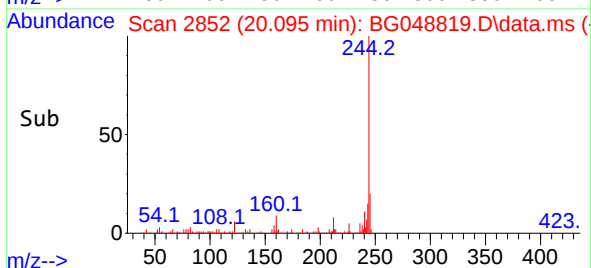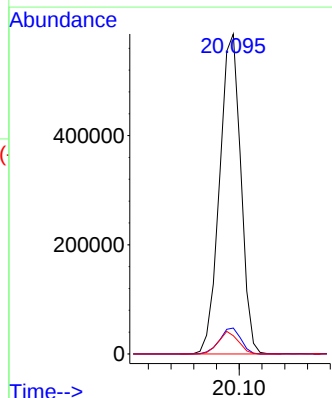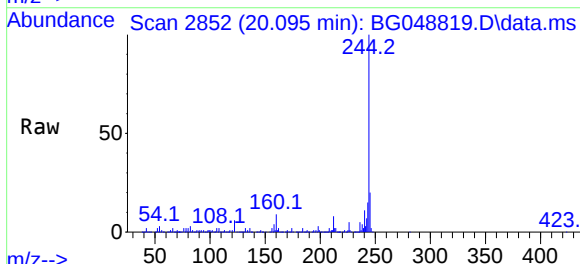

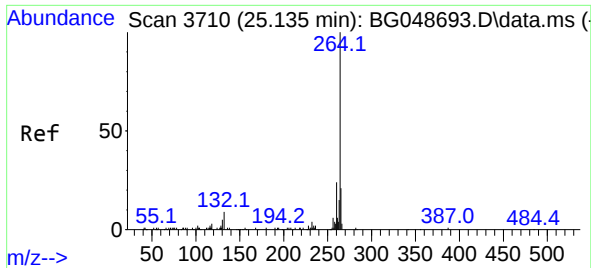

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.101 min Scan# 3704
 Delta R.T. -0.011 min
 Lab File: BG048819.D
 Acq: 21 Apr 2021 14:31

Instrument :
 BNA_G
 ClientSampleId :
 SEDGWICK-COMP-4

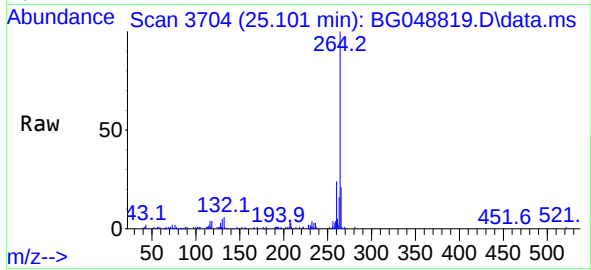

Tgt Ion:264 Resp: 129413

Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.4	29.2
265	21.0	16.9	25.3

