


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
 Data File : BG048811.D
 Acq On : 21 Apr 2021 8:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 17:33:30 2021

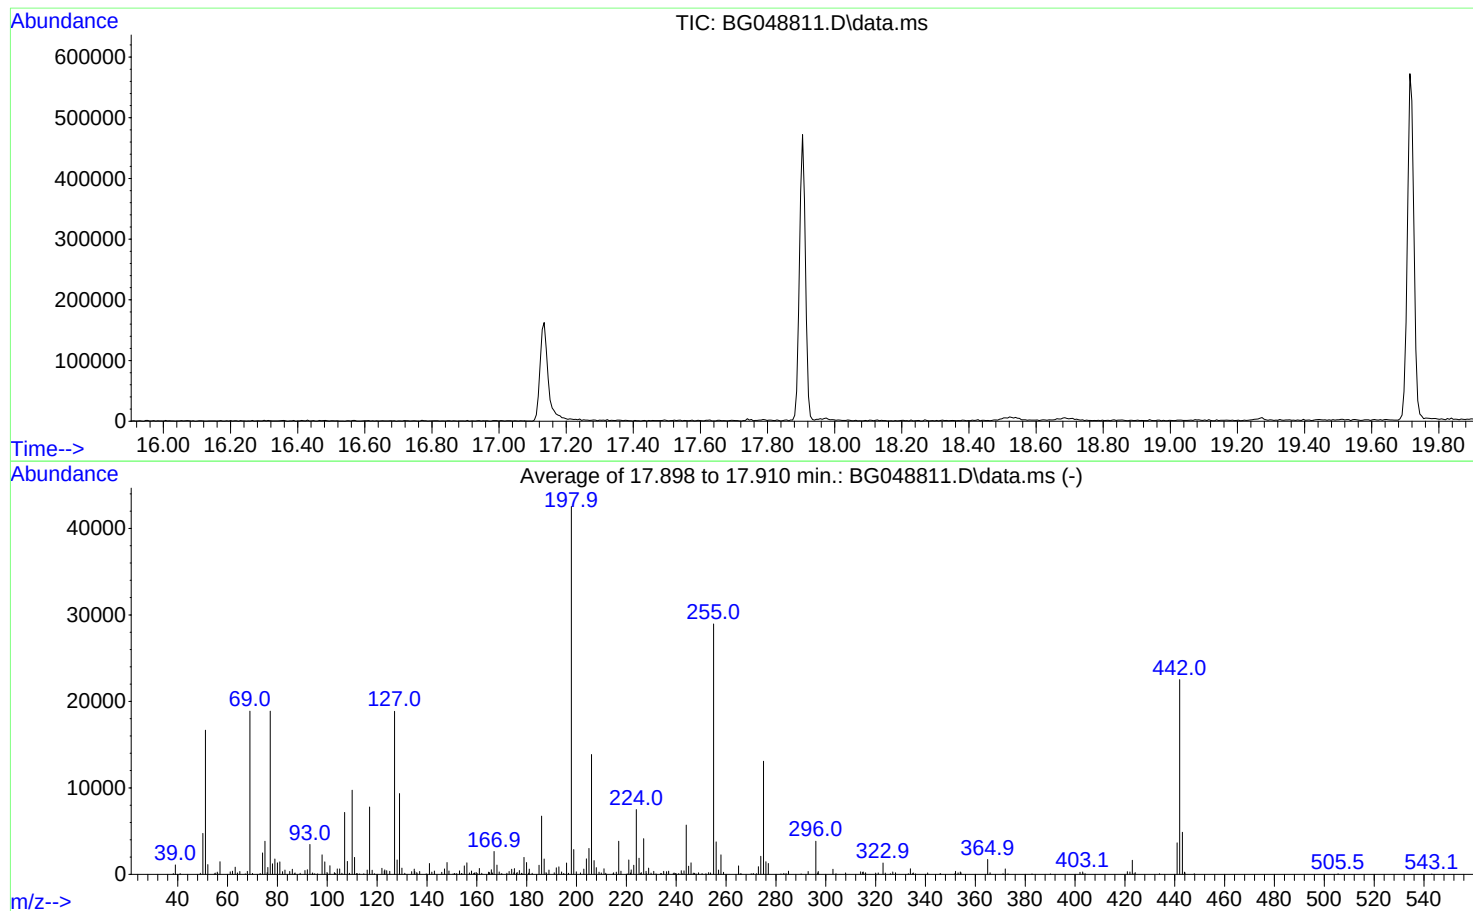




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	16662	PASS
68	69	0.00	2	1.9	356	PASS
69	198	0.00	100	44.4	18875	PASS
70	69	0.00	2	0.6	115	PASS
127	198	10	80	44.3	18857	PASS
197	198	0.00	2	0.3	138	PASS
198	198	100	100	100.0	42536	PASS
199	198	5	9	6.7	2860	PASS
275	198	10	60	30.8	13087	PASS
365	198	1	100	4.0	1719	PASS
441	198	0.01	100	8.6	3638	PASS
442	198	50	100	53.0	22525	PASS
443	442	15	24	21.6	4868	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
Data File : BG048811.D
Acq On : 21 Apr 2021 8:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 21 11:13:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

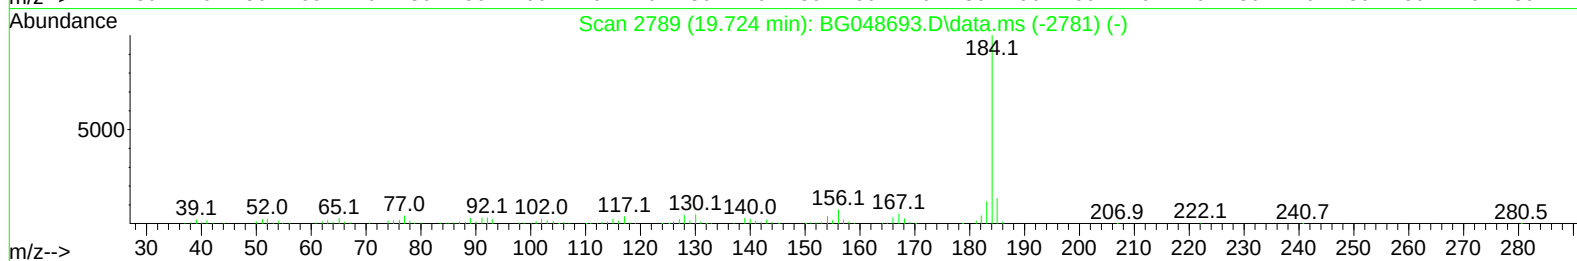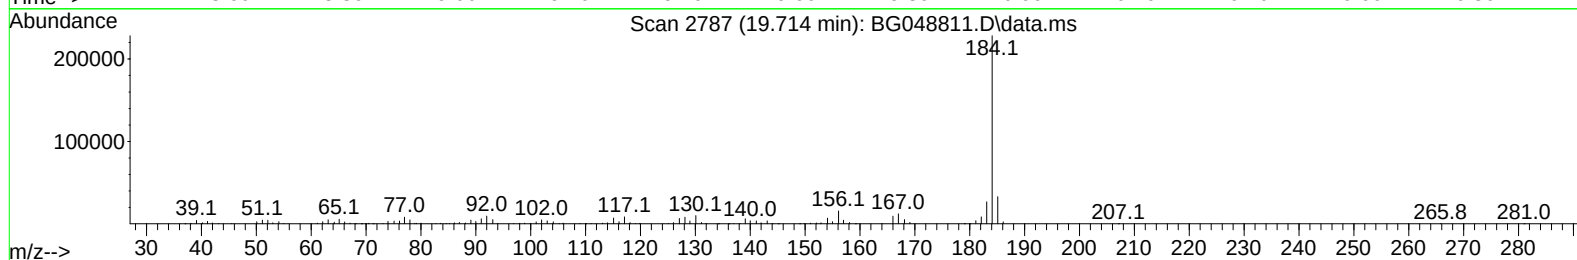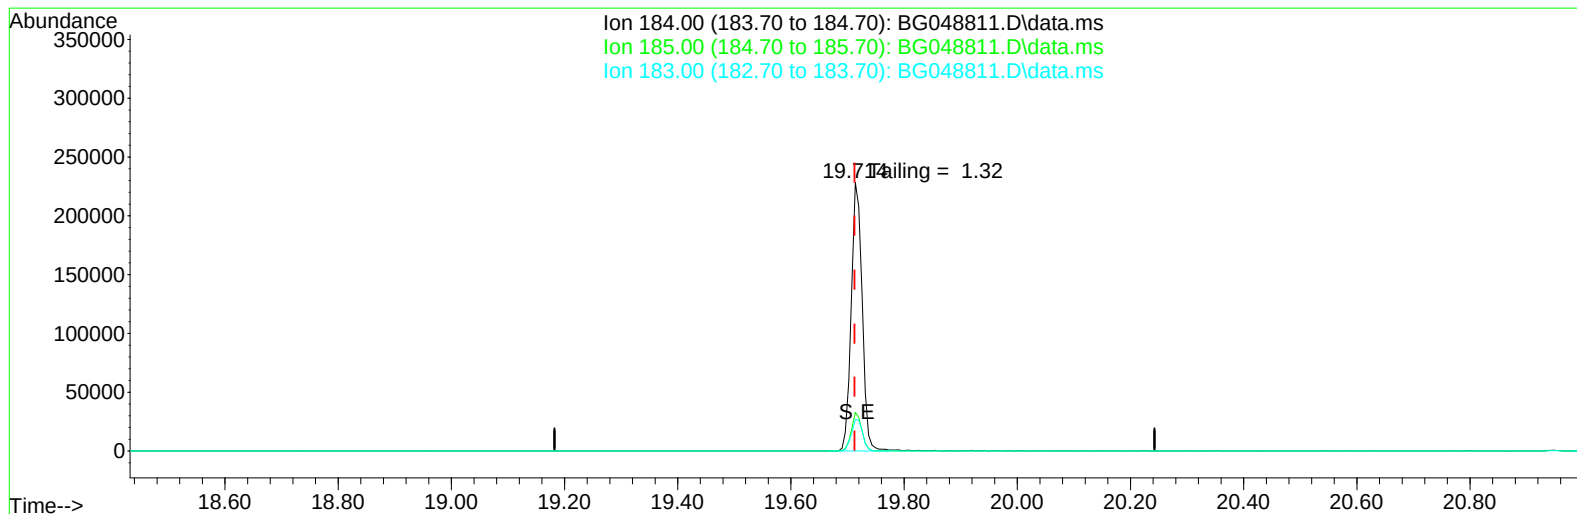

TIC: BG048811.D\data.ms

(77) Benzidine

19.714min (+ 0.002) 192389.13 ng




response 308250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.43
183.00	11.70	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042121\
 Data File : BG048811.D
 Acq On : 21 Apr 2021 8:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 11:13:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

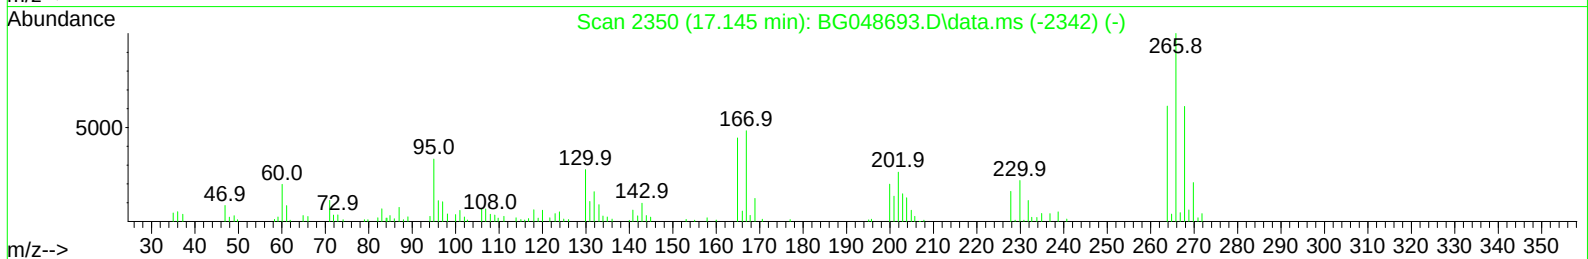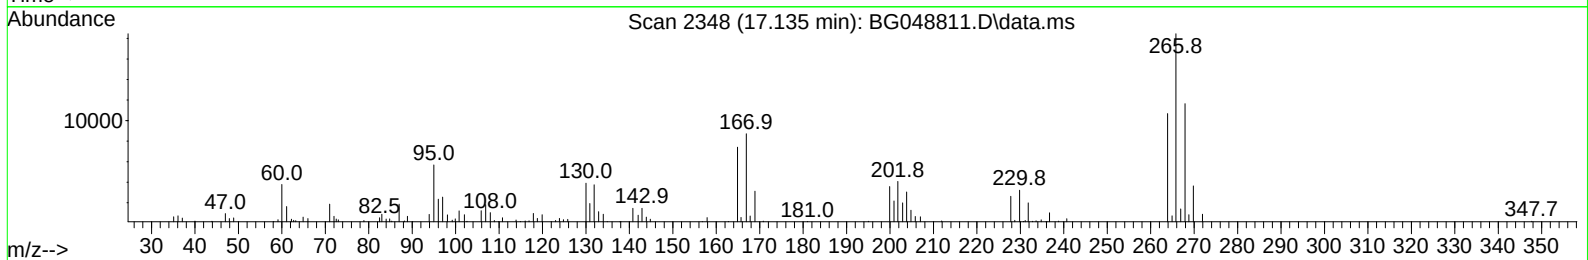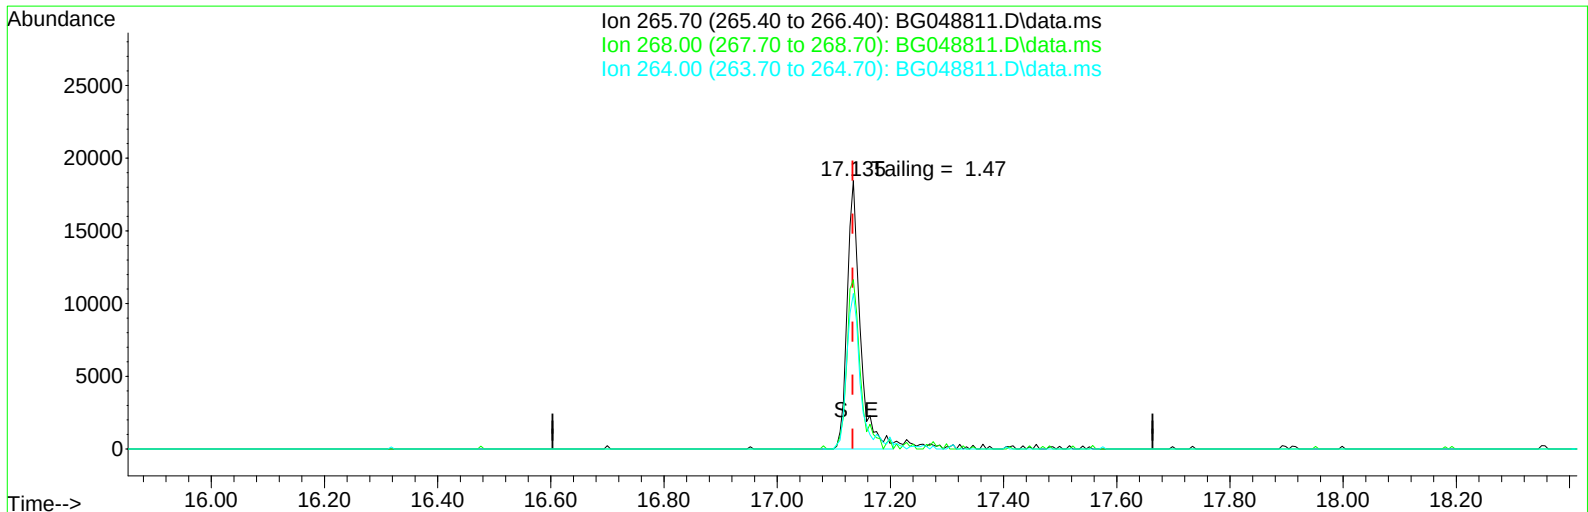

TIC: BG048811.D\data.ms

(70) Pentachlorophenol (C)

17.135min (+ 0.002) 31379.82 ng

response 28851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.09
264.00	61.30	57.89
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/21/2021	BNA_G	BG048811.D
Compound Name	Response	Retention Time
DDT	155490	20.95
DDD	5314	20.5
DDE	362	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5676	161166	3.52