

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042215\
 Data File : BG016647.D
 Acq On : 23 Apr 2015 9:34
 Operator : TP/IZ
 Sample : G1976-01DL 2X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 23 15:42:53 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 22 02:10:07 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	50411	20.00	ng	0.00
21) Naphthalene-d8	10.42	136	253668	20.00	ng	0.00
38) Acenaphthene-d10	14.28	164	163390	20.00	ng	0.00
63) Phenanthrene-d10	17.02	188	346986	20.00	ng	0.00
75) Chrysene-d12	21.21	240	306508	20.00	ng	0.00
86) Perylene-d12	23.43	264	294875	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.23	112	76955	24.47	ng	0.00
7) Phenol-d6	6.84	99	70127	15.96	ng	0.00
23) Nitrobenzene-d5	8.79	82	156815	38.06	ng	0.00
41) 2,4,6-Tribromophenol	15.78	330	65712	59.21	ng	0.00
44) 2-Fluorobiphenyl	12.90	172	370230	37.53	ng	0.00
78) Terphenyl-d14	19.66	244	384709	30.24	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.78	77	36475	18.24	ng	# 1
18) Hexachloroethane	8.73	117	25628	17.88	ng	# 1
22) Acetophenone	8.43	105	63207	11.19	ng	# 52
27) 2,4-Dimethylphenol	9.62	122	10319	2.56	ng	98
31) Naphthalene	10.47	128	686013	51.81	ng	99
32) Benzoic acid	9.79	122	1232	7.98	ng	# 1
33) 4-Chloroaniline	10.47	127	95637	15.79	ng	# 38
37) 2-Methylnaphthalene	12.09	142	218371	23.03	ng	99
53) 2,4-Dinitrophenol	14.42	184	329	8.60	ng	# 1
64) 4,6-Dinitro-2-methylphenol	15.43	198	390	4.27	ng	# 1
69) Pentachlorophenol	16.69	266	2551	7.83	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042215\
Data File : BG016647.D
Acq On : 23 Apr 2015 9:34
Operator : TP/IZ
Sample : G1976-01DL 2X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 23 15:42:53 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 02:10:07 2015
Response via : Initial Calibration

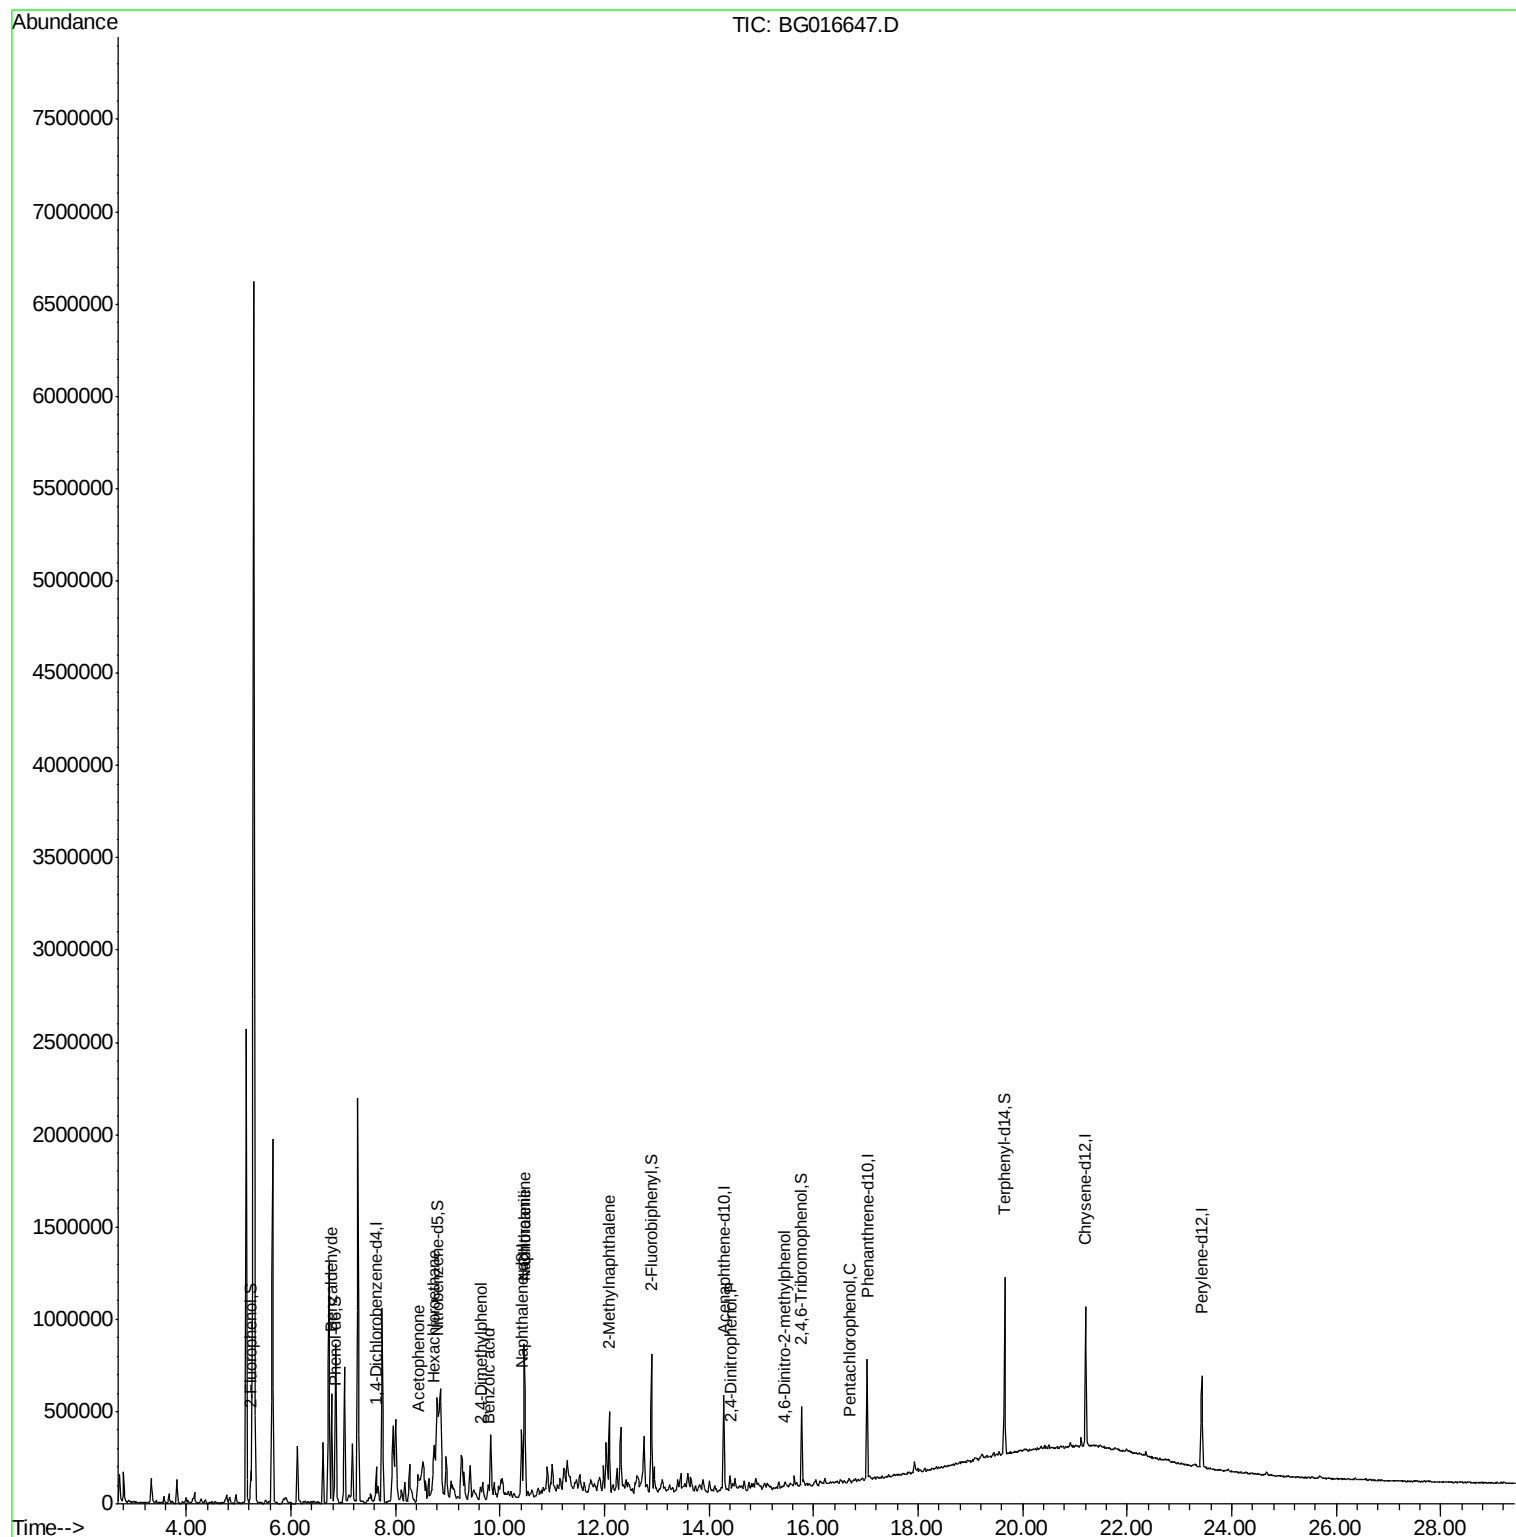




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.63 min Scan# 842
Delta R.T. -0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	162.0	125.5	188.3
115	55.6	44.5	66.7

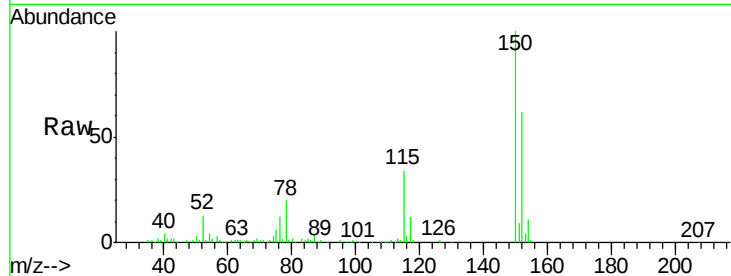


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

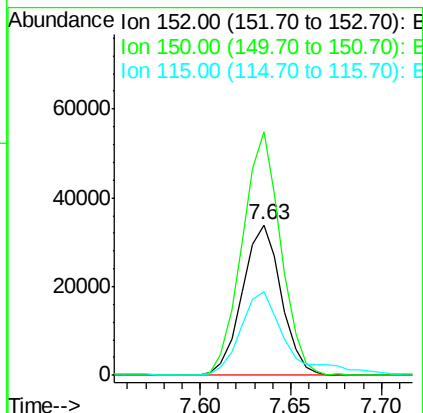



#5


2-Fluorophenol
Concen: 24.47 ng
RT: 5.23 min Scan# 433
Delta R.T. 0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Tgt Ion	Ratio	Lower	Upper
112	100		
64	44.3	38.5	57.7
63	23.7	18.2	27.4



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

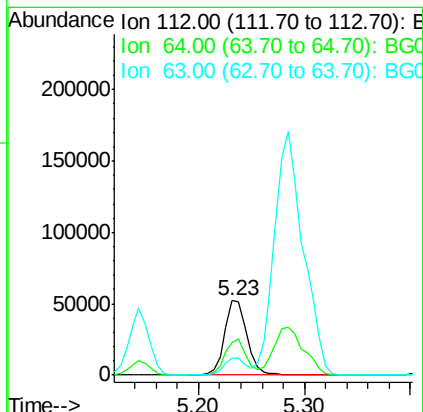



#7

Phenol-d6

Concen: 15.96 ng

RT: 6.84 min Scan# 706

Delta R.T. 0.01 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 70127

Ion Ratio Lower Upper




99 100

42 11.0 9.5 14.3

71 26.2 20.2 30.2



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

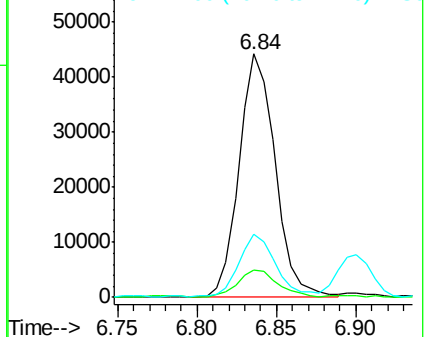

#9

Benzaldehyde

Concen: 18.24 ng

RT: 6.78 min Scan# 696

Delta R.T. -0.00 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34


Tgt Ion: 77 Resp: 36475

Ion Ratio Lower Upper



77 100


105 985.0 81.6 121.6#

106 92.0 87.4 127.4



Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 105.00 (104.70 to 105.70): BGC
Ion 106.00 (105.70 to 106.70): BGC




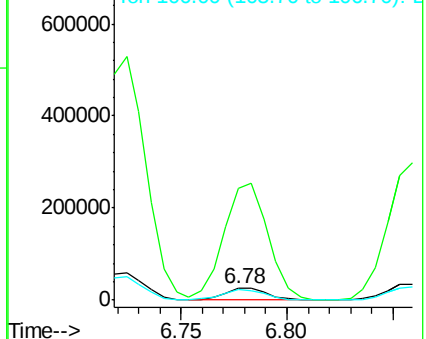




#18
Hexachloroethane
Concen: 17.88 ng
RT: 8.73 min Scan# 1029
Delta R.T. 0.03 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34




Instrument :
BNA_G
ClientSampleId :


Tot Ion:117 Resp: 25628
Ion Ratio Lower Upper
117 100
119 304.2 73.8 110.8#
201 0.0 62.2 93.2#

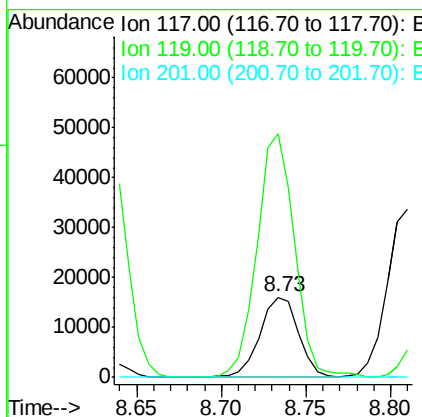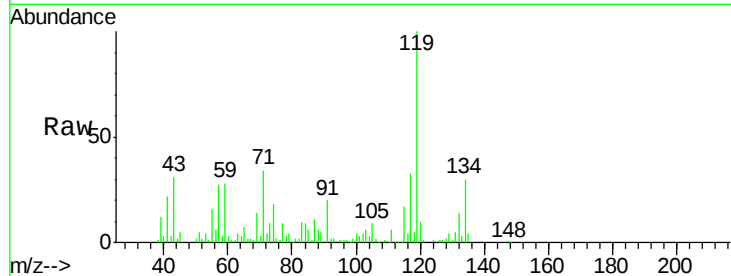

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.42 min Scan# 1316
Delta R.T. -0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Tgt Ion:136 Resp: 253668
Ion Ratio Lower Upper
136 100
137 10.1 8.8 13.2
54 7.4 4.9 7.3#
68 7.8 4.9 7.3#



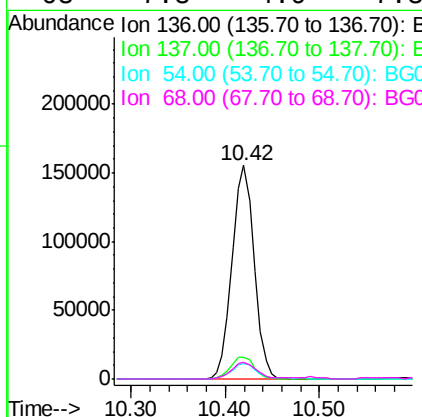





#22
 Acetophenone
 Concen: 11.19 ng
 RT: 8.43 min Scan# 978
 Delta R.T. -0.03 min
 Lab File: BG016647.D
 Acq: 23 Apr 2015 9:34




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:	105	Resp:	63207
Ion	Ratio	Lower	Upper
105	100		
71	1.5	1.8	2.6#
51	3.6	16.5	24.7#
120	0.6	26.8	40.2#

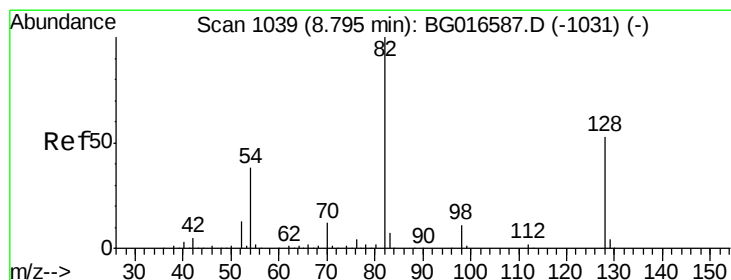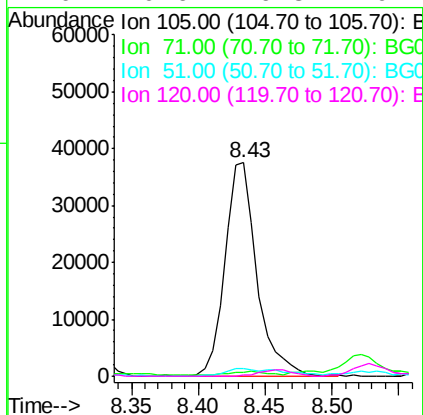

#23
 Nitrobenzene-d5
 Concen: 38.06 ng
 RT: 8.79 min Scan# 1039
 Delta R.T. -0.00 min
 Lab File: BG016647.D
 Acq: 23 Apr 2015 9:34

Tgt Ion:	82	Resp:	156815
Ion	Ratio	Lower	Upper
82	100		
128	53.0	42.7	64.1
54	36.7	30.6	45.8



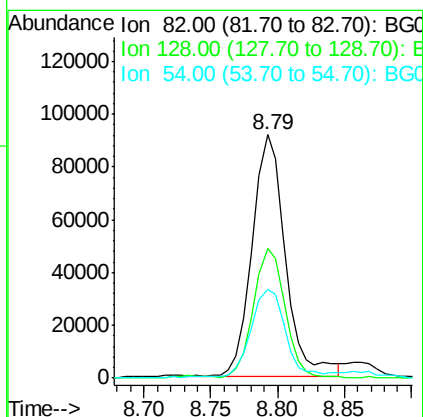
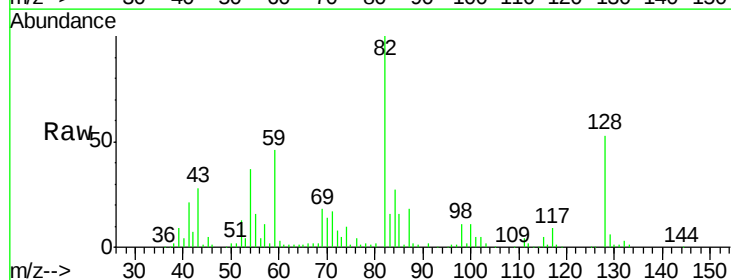




#27
2,4-Dimethylphenol
Concen: 2.56 ng
RT: 9.62 min Scan# 1180
Delta R.T. 0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34




Instrument :
BNA_G
ClientSampled :


Tot Ion:122 Resp: 10319
Ion Ratio Lower Upper
122 100
107 106.3 82.9 124.3
121 58.2 47.0 70.4

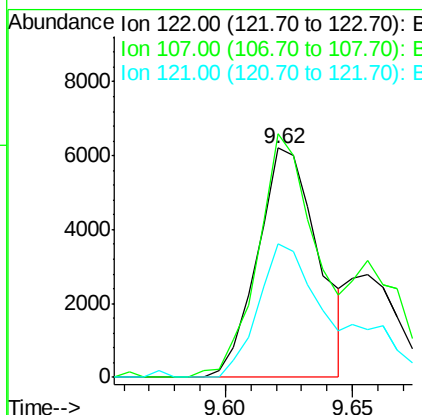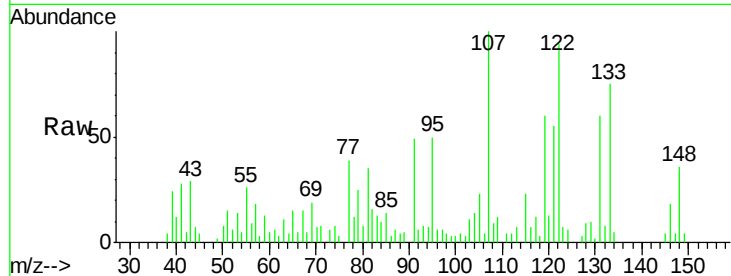

#31
Naphthalene
Concen: 51.81 ng
RT: 10.47 min Scan# 1324
Delta R.T. -0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Tgt Ion:128 Resp: 686013
Ion Ratio Lower Upper
128 100
129 11.9 9.2 13.8
127 13.7 10.6 16.0

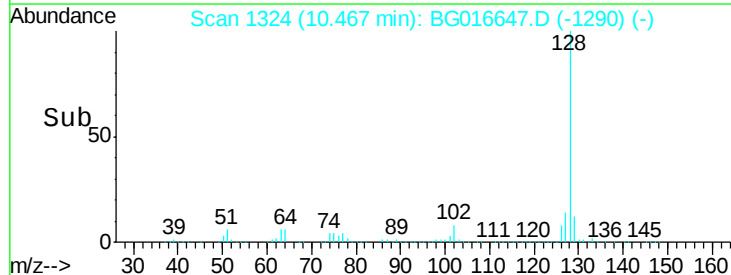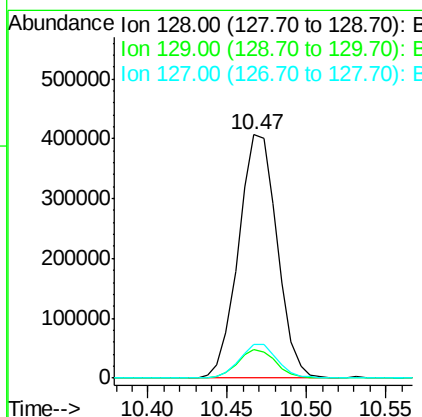



#32

Benzoic acid

Concen: 7.98 ng

RT: 9.79 min Scan# 1208

Delta R.T. 0.02 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34

Instrument :

BNA_G

ClientSampled :


Tot Ion:122 Resp: 1232

Ion Ratio Lower Upper

122 100

105 346.9 95.5 135.5#




77 172.5 60.2 100.2#



Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BGC

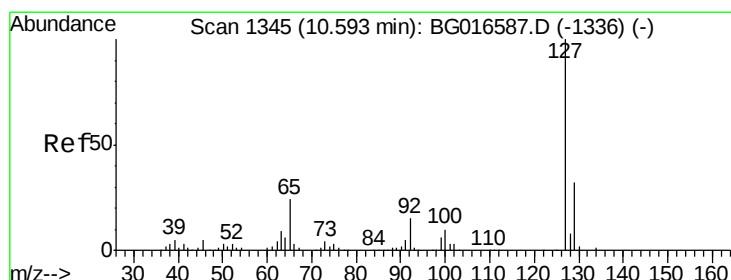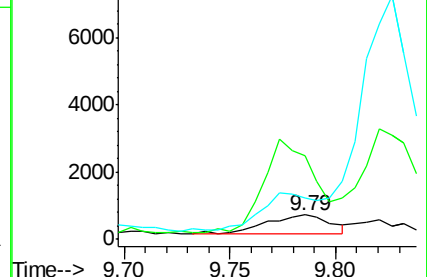

#33

4-Chloroaniline

Concen: 15.79 ng

RT: 10.47 min Scan# 1325

Delta R.T. -0.12 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34

Tgt Ion:127 Resp: 95637


Ion Ratio Lower Upper

127 100

129 78.7 25.4 38.0#

65 0.0 19.0 28.4#

92 0.3 12.3 18.5#


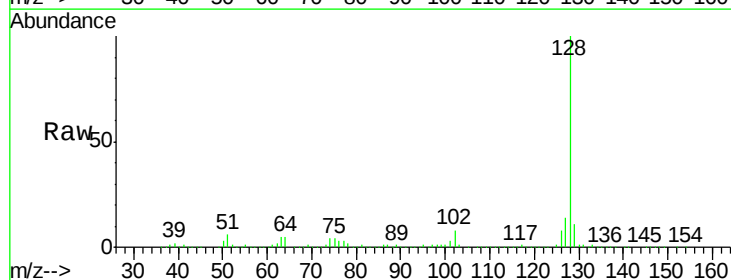



Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 65.00 (64.70 to 65.70): BGC

Ion 92.00 (91.70 to 92.70): BGC



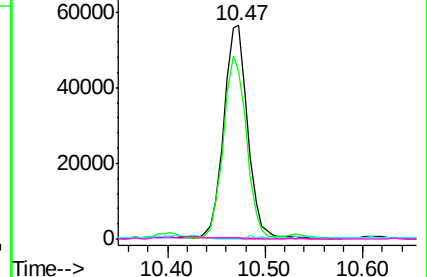



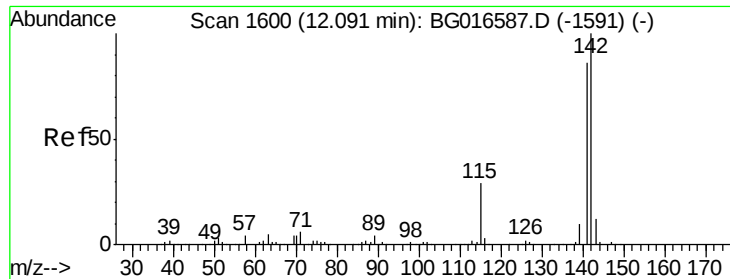

#37
2-Methylnaphthalene
Concen: 23.03 ng
RT: 12.09 min Scan# 1600
Delta R.T. -0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
142	100		
141	86.5	68.6	102.8
115	30.5	23.3	34.9

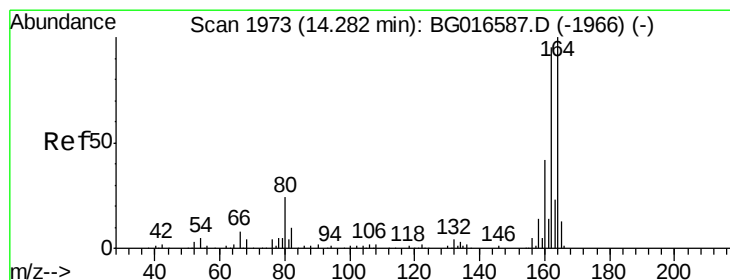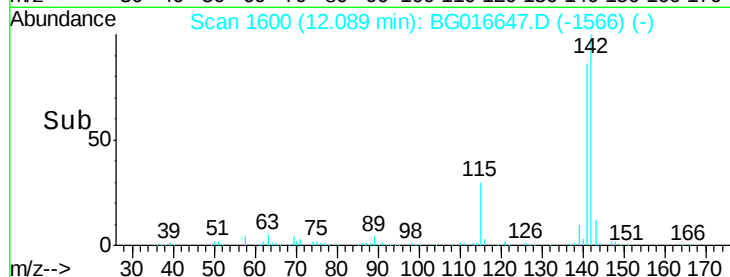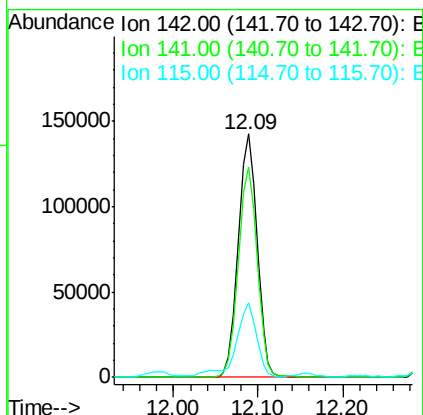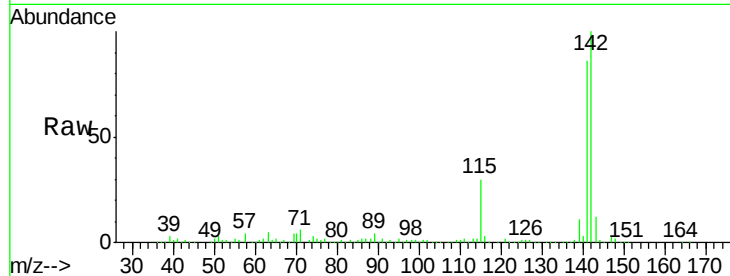

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.28 min Scan# 1973
Delta R.T. -0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Tgt Ion	Ratio	Lower	Upper
164	100		
162	98.4	75.8	113.6
160	45.1	33.8	50.6

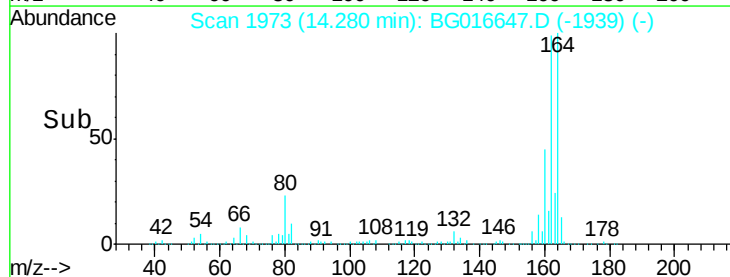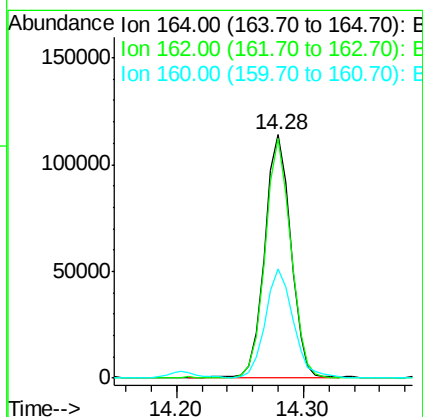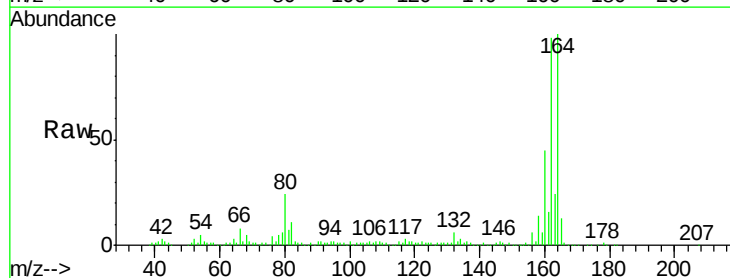

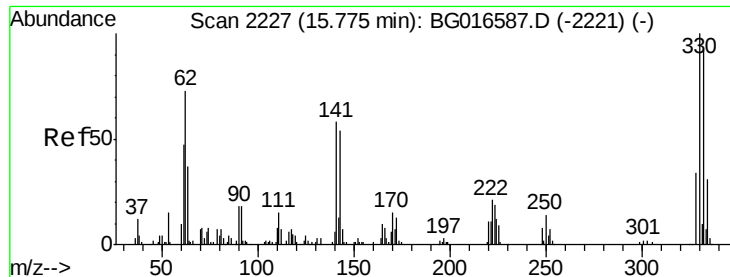

#41

2,4,6-Tribromophenol

Concen: 59.21 ng

RT: 15.78 min Scan# 2228

Delta R.T. 0.00 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34

Instrument :

BNA_G

ClientSampleId :


Tot Ion:330 Resp: 65712

Ion Ratio Lower Upper




330 100

332 94.5 76.6 114.8

141 51.3 45.9 68.9

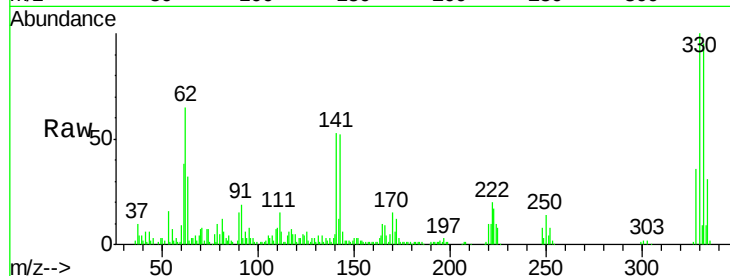

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

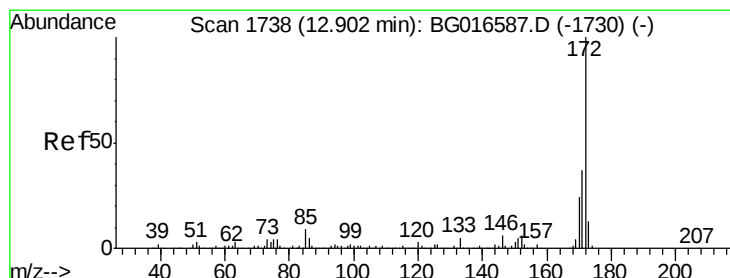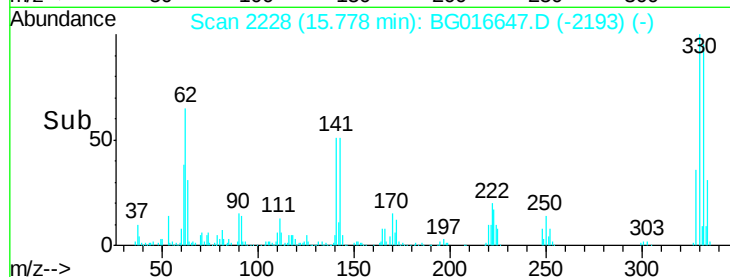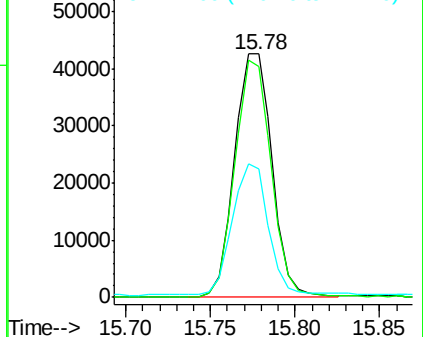

#44

2-Fluorobiphenyl

Concen: 37.53 ng

RT: 12.90 min Scan# 1738

Delta R.T. -0.00 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34


Tgt Ion:172 Resp: 370230

Ion Ratio Lower Upper



172 100


171 36.2 29.6 44.4

170 23.3 19.4 29.0

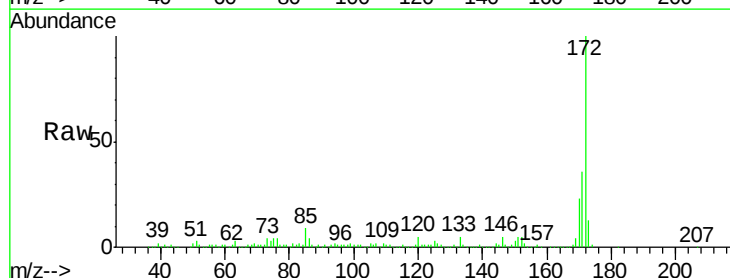

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

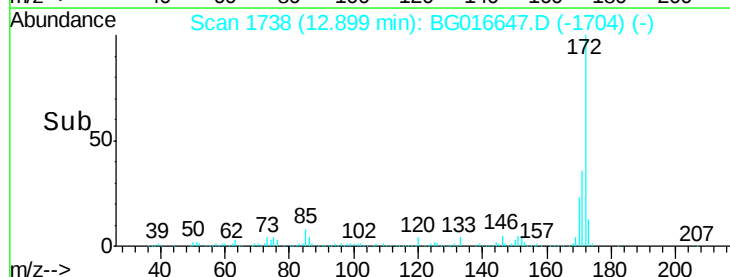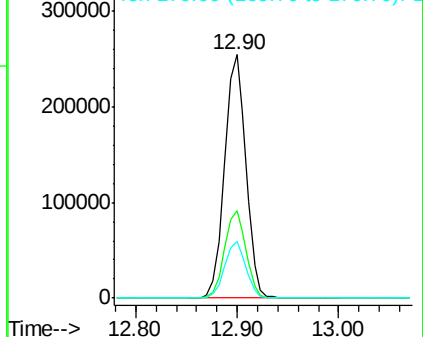


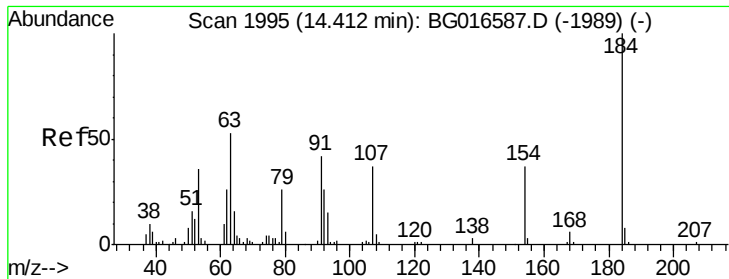




#53
 2,4-Dinitrophenol
 Concen: 8.60 ng
 RT: 14.42 min Scan# 1997
 Delta R.T. 0.01 min
 Lab File: BG016647.D
 Acq: 23 Apr 2015 9:34

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:184 Resp: 329
 Ion Ratio Lower Upper
 184 100
 63 204.5 42.6 64.0#
 154 141.7 33.4 50.0#

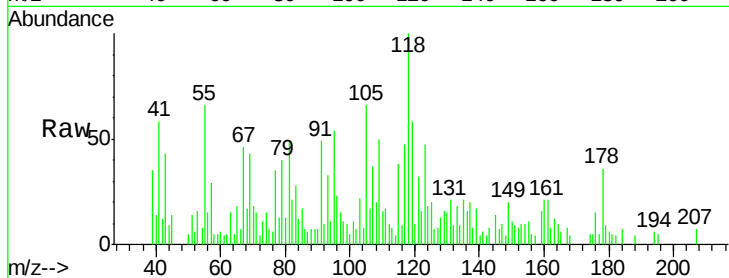


Abundance Ion 184.00 (183.70 to 184.70): E
 Ion 63.00 (62.70 to 63.70): BG
 Ion 154.00 (153.70 to 154.70): E

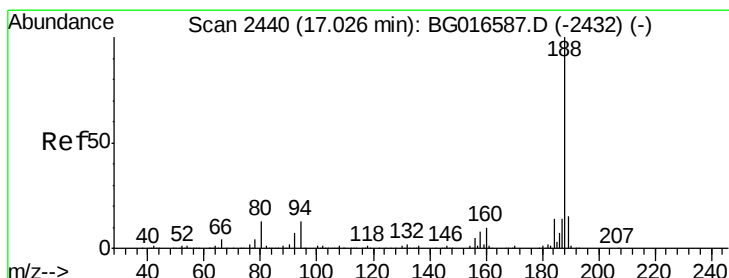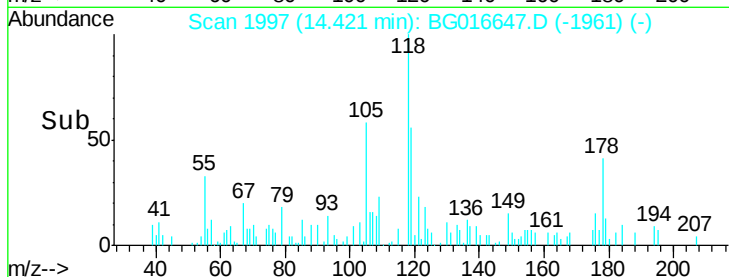
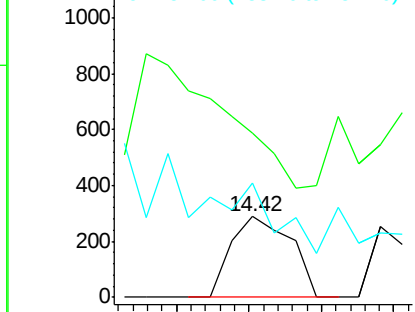



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.02 min Scan# 2440
 Delta R.T. -0.00 min
 Lab File: BG016647.D
 Acq: 23 Apr 2015 9:34

Tgt Ion:188 Resp: 346986
 Ion Ratio Lower Upper
 188 100
 94 13.0 10.5 15.7
 80 12.7 10.6 16.0

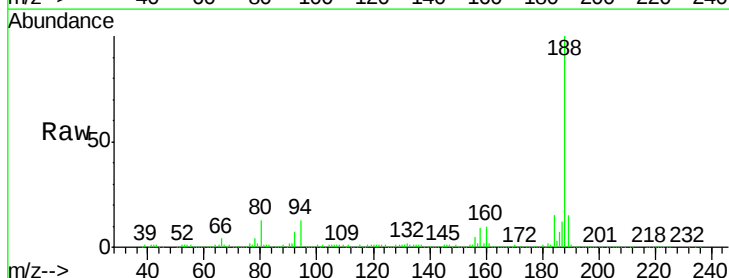

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BG
 Ion 80.00 (79.70 to 80.70): BG



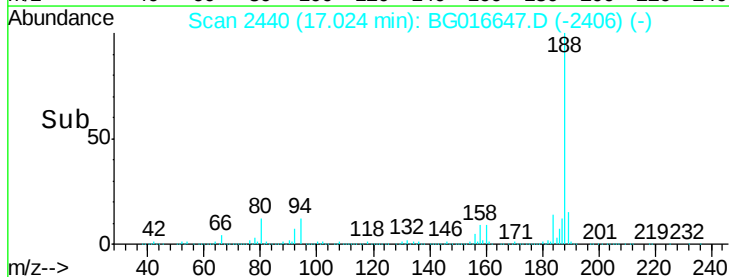
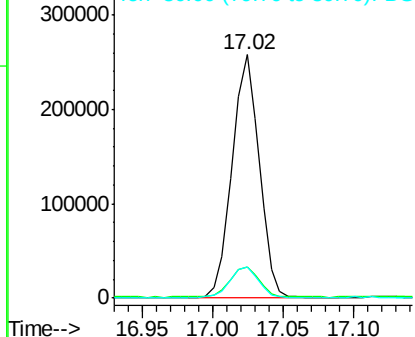




#64
4,6-Dinitro-2-methylphenol
Concen: 4.27 ng
RT: 15.43 min Scan# 2169
Delta R.T. 0.01 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34




Instrument :
BNA_G
ClientSampleId :


Tot Ion:198 Resp: 390
Ion Ratio Lower Upper
198 100
51 103.5 18.6 58.6#
105 339.1 27.7 67.7#

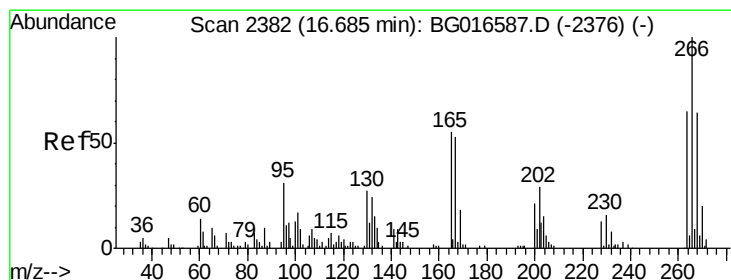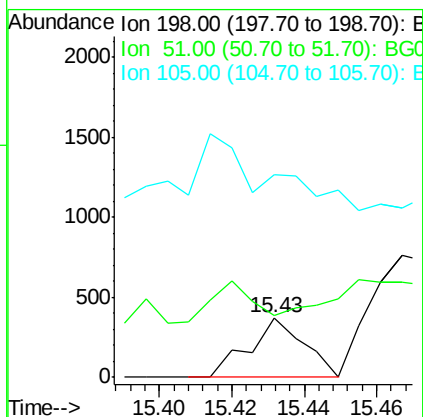

#69
Pentachlorophenol
Concen: 7.83 ng
RT: 16.69 min Scan# 2383
Delta R.T. 0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Tgt Ion:266 Resp: 2551
Ion Ratio Lower Upper
266 100
268 57.4 51.3 76.9
264 64.5 52.2 78.4

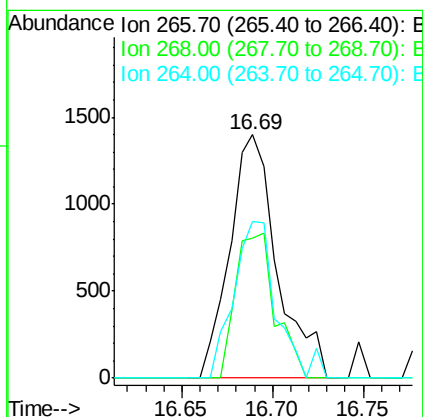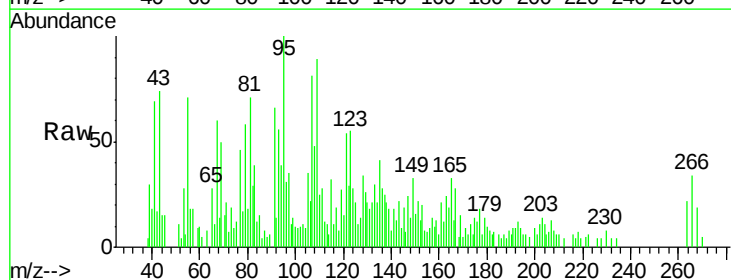



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.21 min Scan# 3152

Delta R.T. -0.00 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 306508

Ion Ratio Lower Upper

240 100

120 20.6 16.7 25.1




236 26.6 21.7 32.5

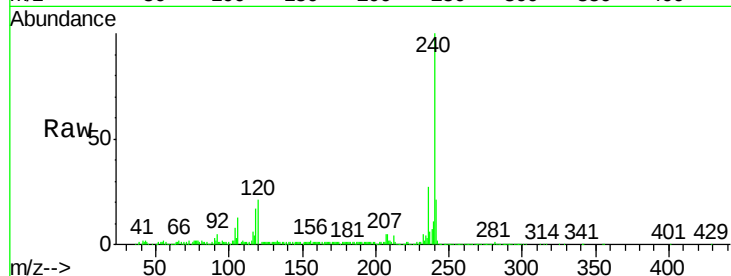

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

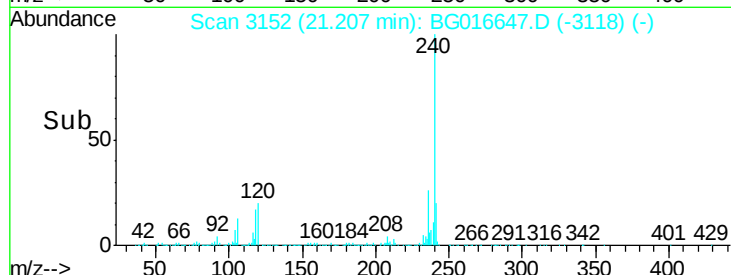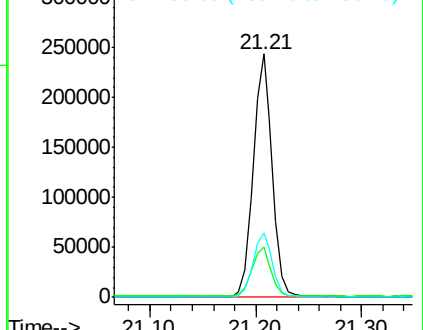

#78

Terphenyl-d14

Concen: 30.24 ng

RT: 19.66 min Scan# 2888

Delta R.T. -0.00 min

Lab File: BG016647.D

Acq: 23 Apr 2015 9:34


Tgt Ion:244 Resp: 384709

Ion Ratio Lower Upper

244 100

212 7.5 6.8 10.2



122 18.2 17.0 25.6




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

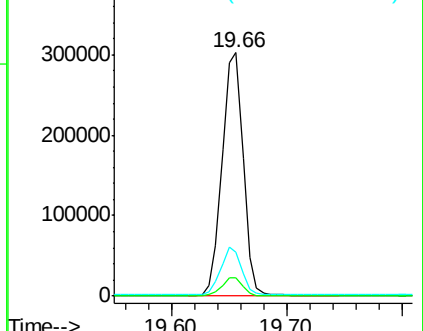



#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.43 min Scan# 3530
Delta R.T. 0.00 min
Lab File: BG016647.D
Acq: 23 Apr 2015 9:34

Instrument :
BNA_G
ClientSampleId :

Tot Ion: 264 Resp: 294875
Ion Ratio Lower Upper
264 100
260 24.7 21.4 32.2
265 21.9 18.7 28.1

