


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042215\
 Data File : BG016633.D
 Acq On : 23 Apr 2015 00:53
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 01:45:23 2015

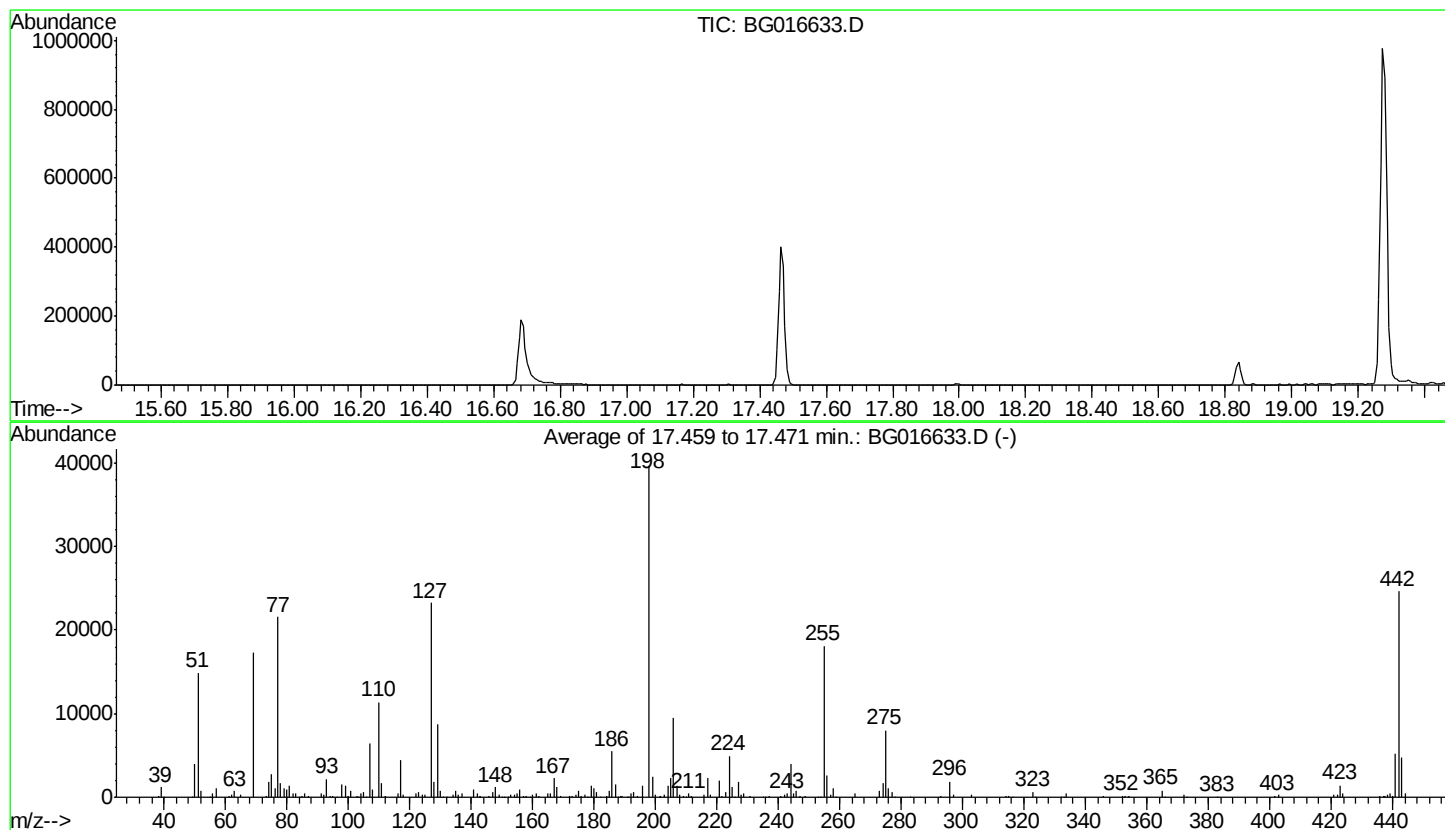

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	14889	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.7	17353	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.6	23234	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39677	PASS
199	198	5	9	6.3	2502	PASS
275	198	10	60	20.2	8017	PASS
365	198	1	100	2.1	837	PASS
441	442	0.01	24	21.0	5183	PASS
442	198	50	100	62.1	24625	PASS
443	442	15	24	19.4	4773	PASS