
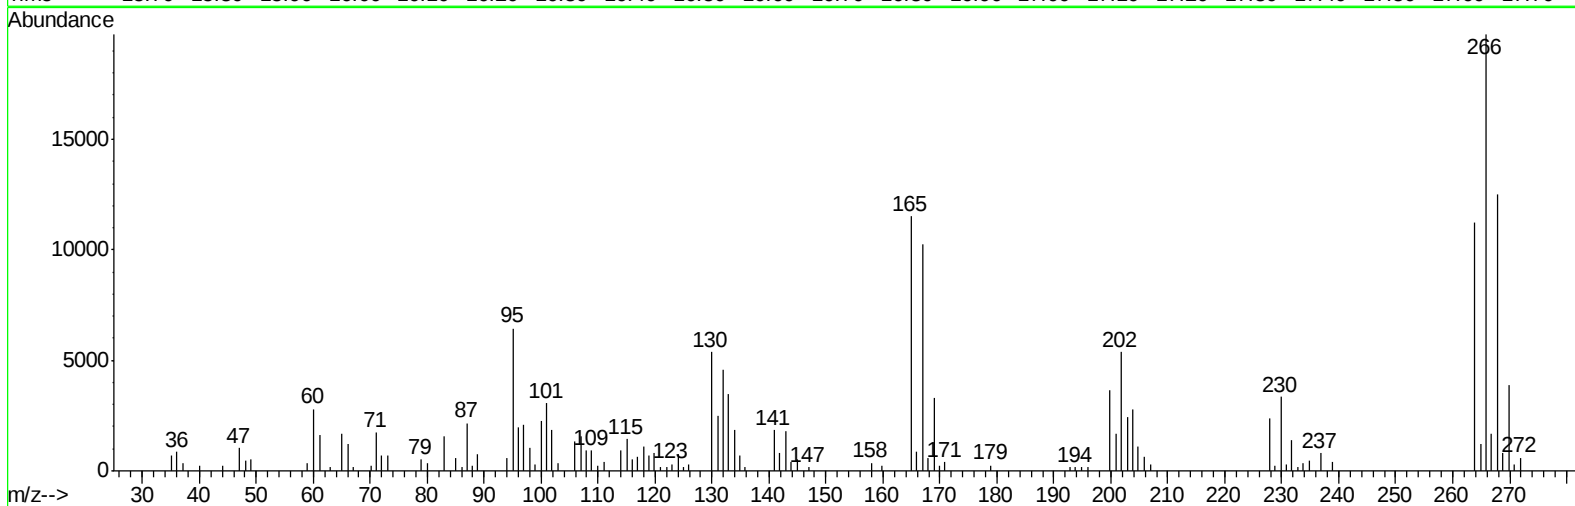


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042215\
Data File : BG016633.D
Acq On : 23 Apr 2015 00:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 07:16:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 03:17:21 2015
Response via : Initial Calibration

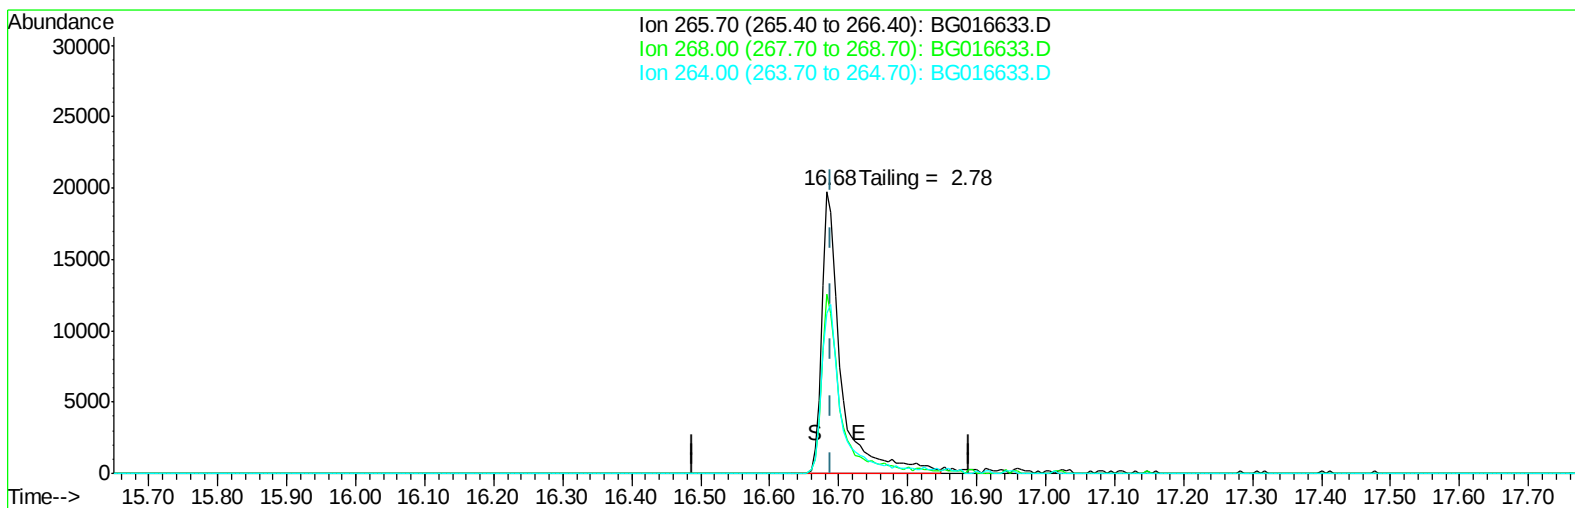

TIC: BG016633.D

(69) Pentachlorophenol (C)



16.683min (-0.006) 44757.64ng

response 35546

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.47
264.00	65.30	56.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042215\
Data File : BG016633.D
Acq On : 23 Apr 2015 00:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 07:16:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 03:17:21 2015
Response via : Initial Calibration

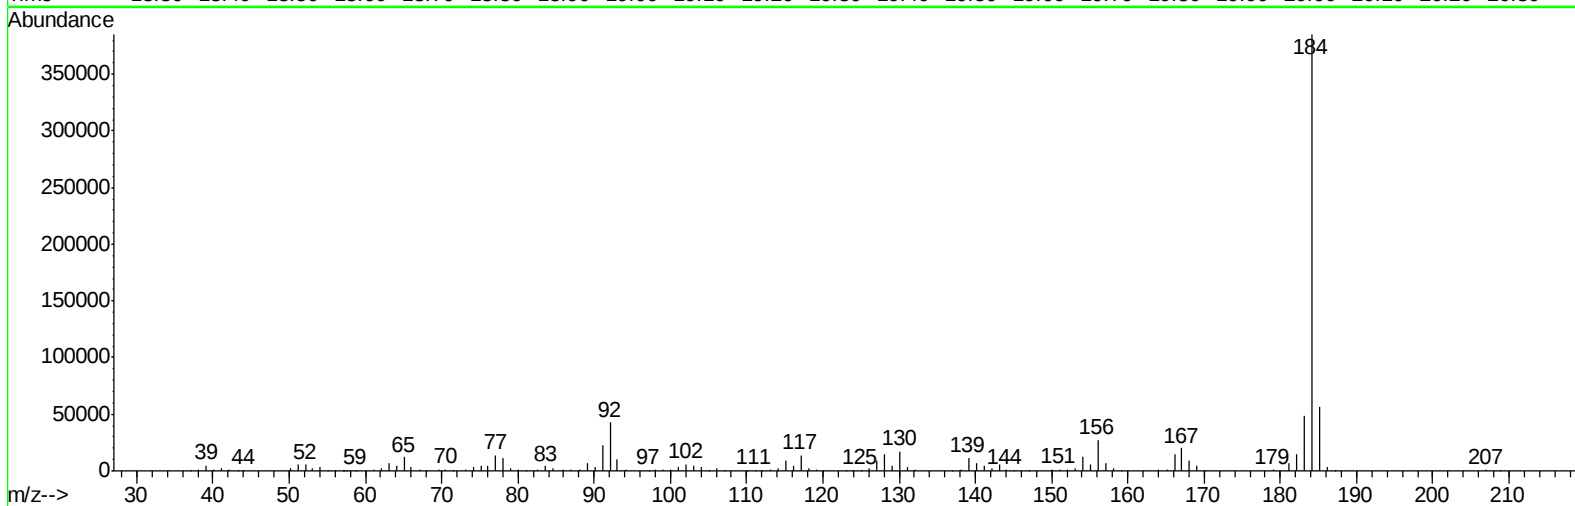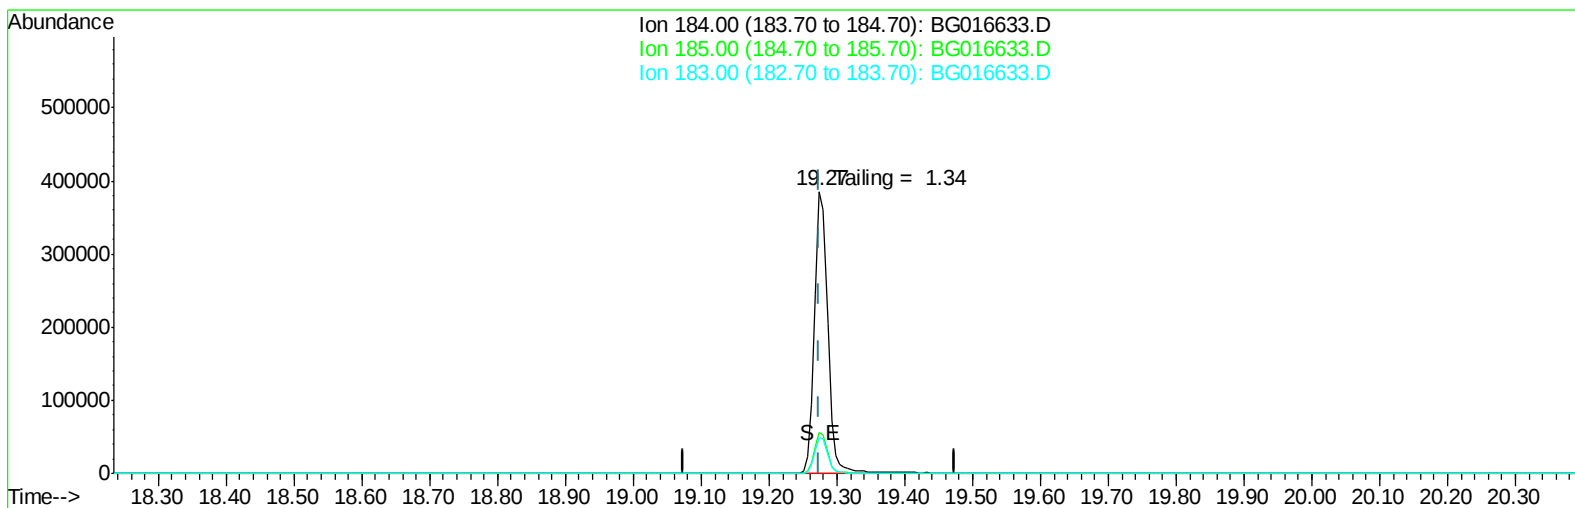

TIC: BG016633.D

(76) Benzidine

19.274min (+0.000) 21922.98ng

response 519598

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.55
183.00	12.90	12.64
0.00	0.00	0.00