


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042215\
 Data File : BG016616.D
 Acq On : 22 Apr 2015 12:46
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 22 02:10:07 2015

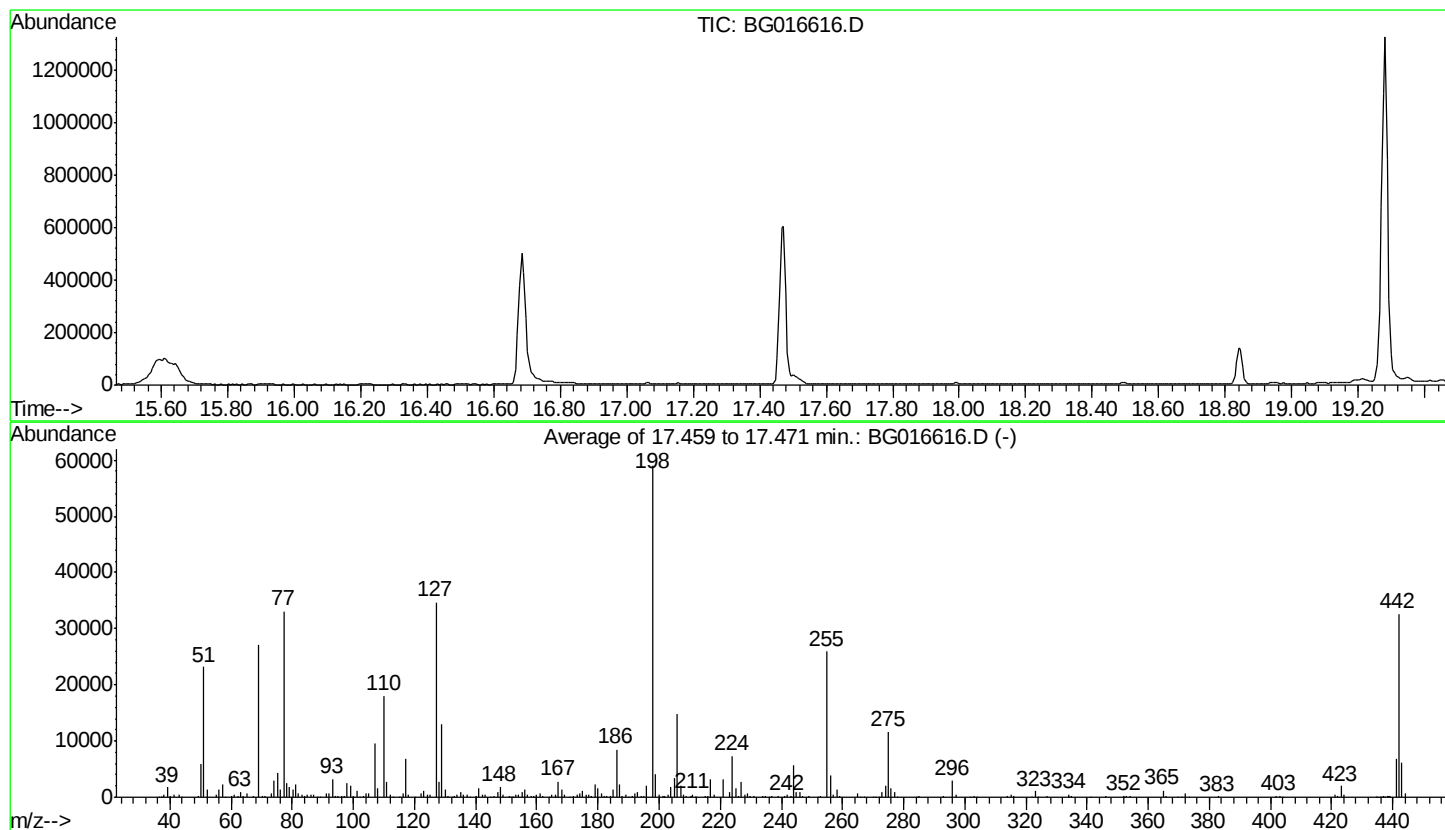

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	23224	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.0	27136	PASS
70	69	0.00	2	0.6	162	PASS
127	198	10	80	58.8	34717	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59008	PASS
199	198	5	9	7.0	4115	PASS
275	198	10	60	19.7	11649	PASS
365	198	1	100	2.0	1173	PASS
441	442	0.01	24	20.8	6809	PASS
442	198	50	100	55.4	32663	PASS
443	442	15	24	19.2	6262	PASS