
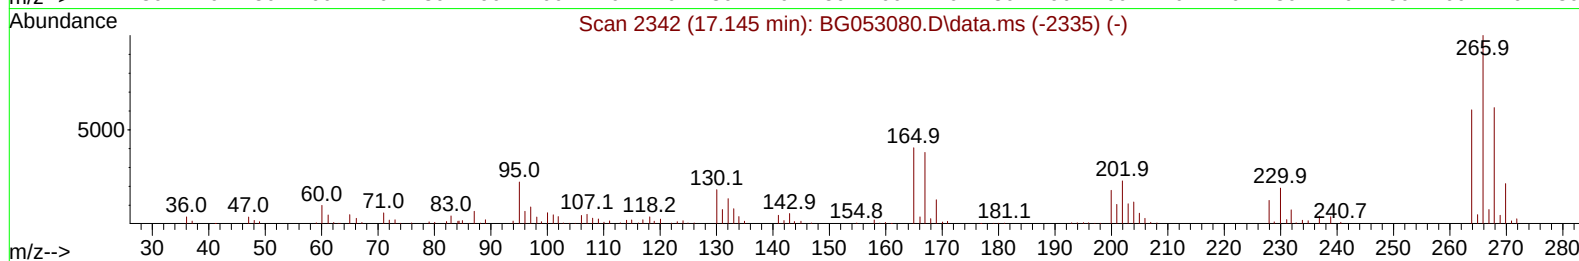
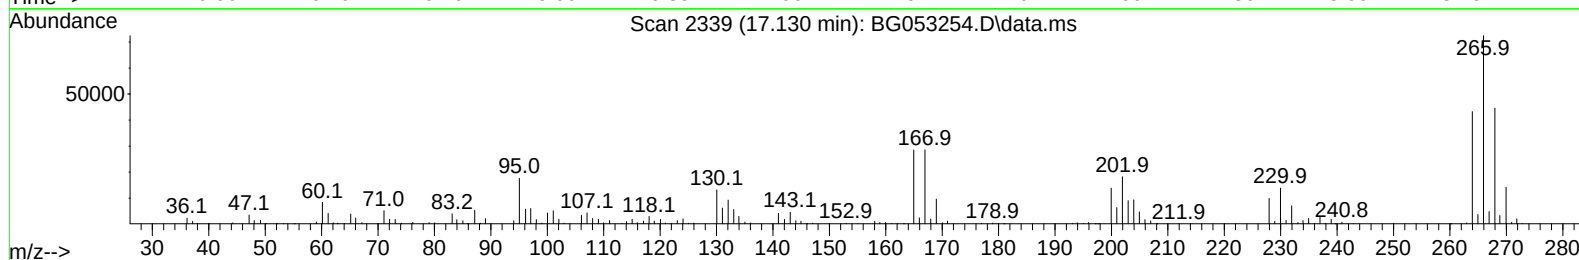


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053254.D
Acq On : 22 Apr 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 04:30:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

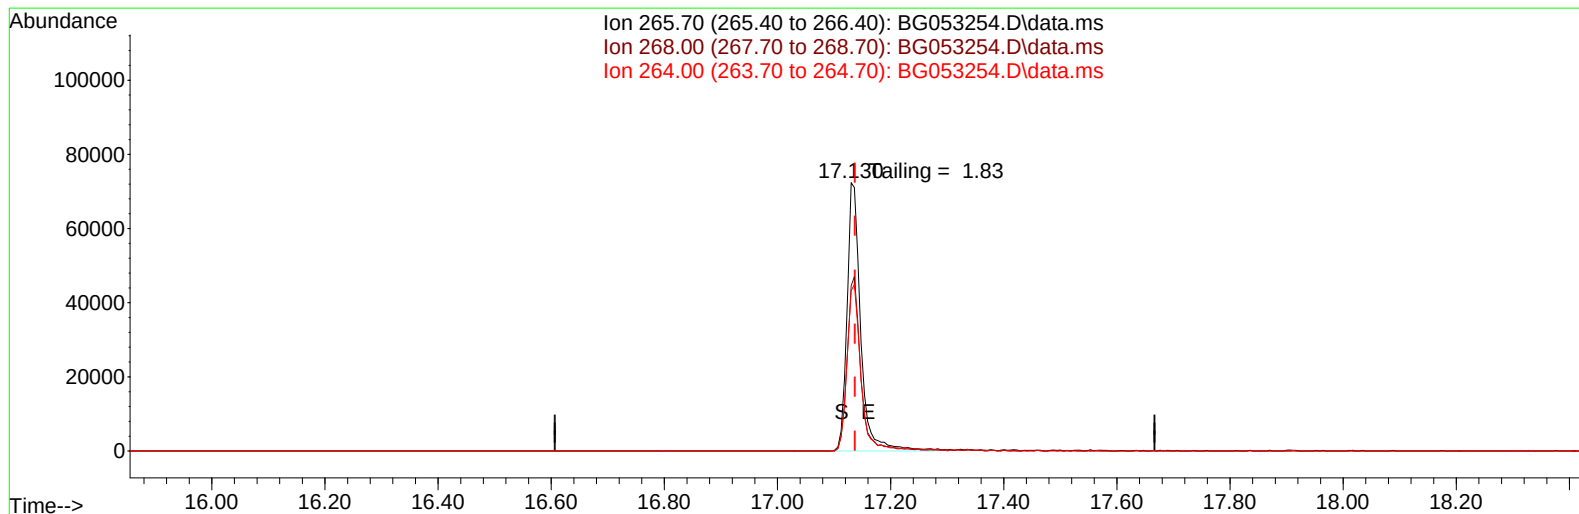

TIC: BG053254.D\data.ms

(70) Pentachlorophenol (C)




17.130min (-0.006) 40187.77 ng

response 121606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.63
264.00	56.60	59.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053254.D
Acq On : 22 Apr 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 04:30:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

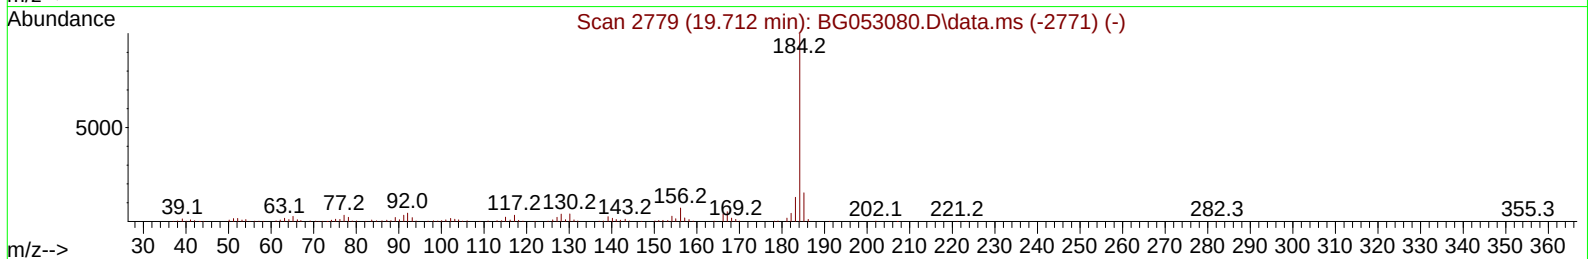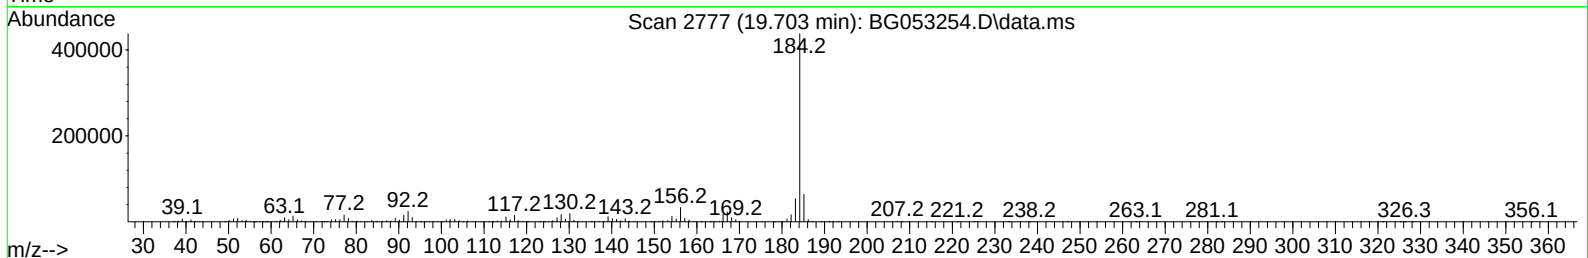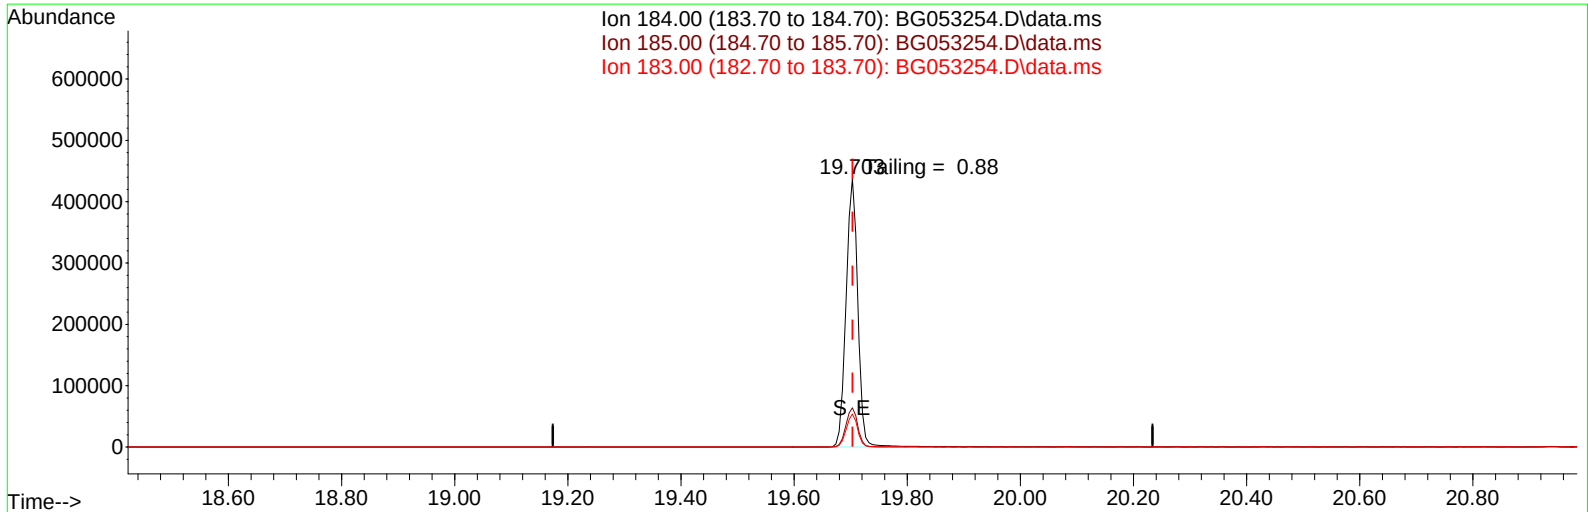

TIC: BG053254.D\data.ms

(77) Benzidine**19.703min (-0.001) 329371.94 ng****response 629633**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.62
183.00	11.80	12.32
0.00	0.00	0.00