
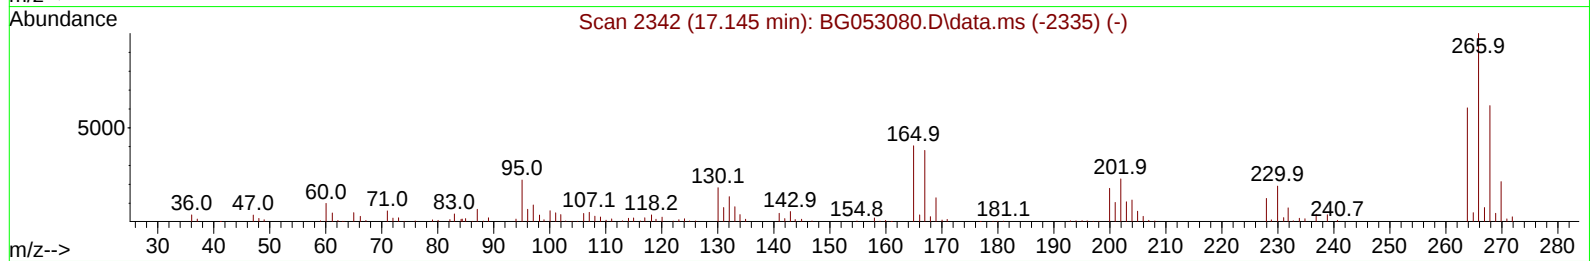
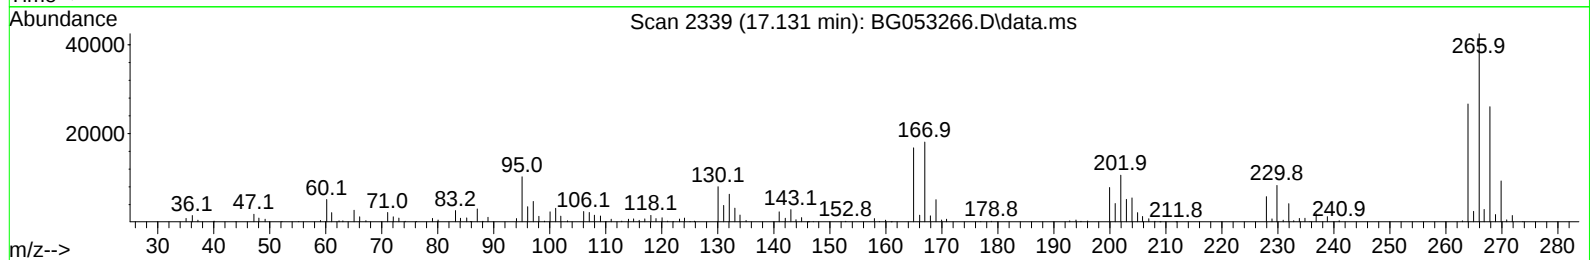


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053266.D
Acq On : 22 Apr 2022 18:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 04:37:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

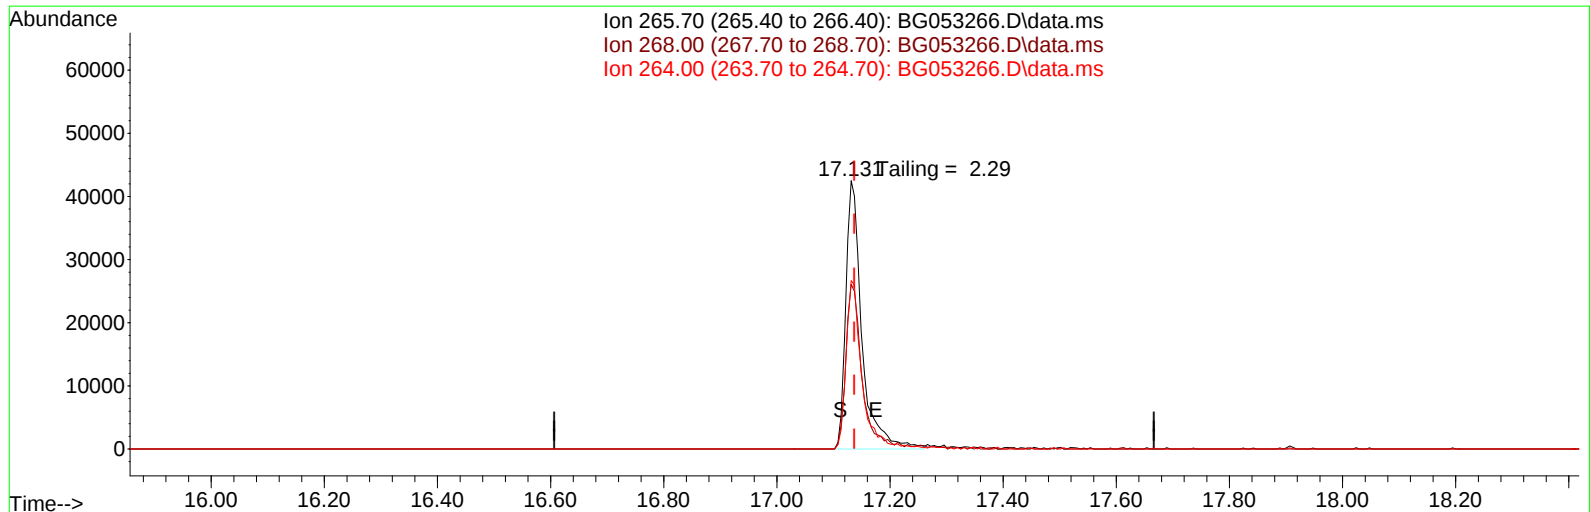

TIC: BG053266.D\data.ms

(70) Pentachlorophenol (C)




17.131min (-0.005) 23834.97 ng

response 84415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.34
264.00	56.60	62.75
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\  
Data File : BG053266.D  
Acq On    : 22 Apr 2022  18:19  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 24 04:37:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

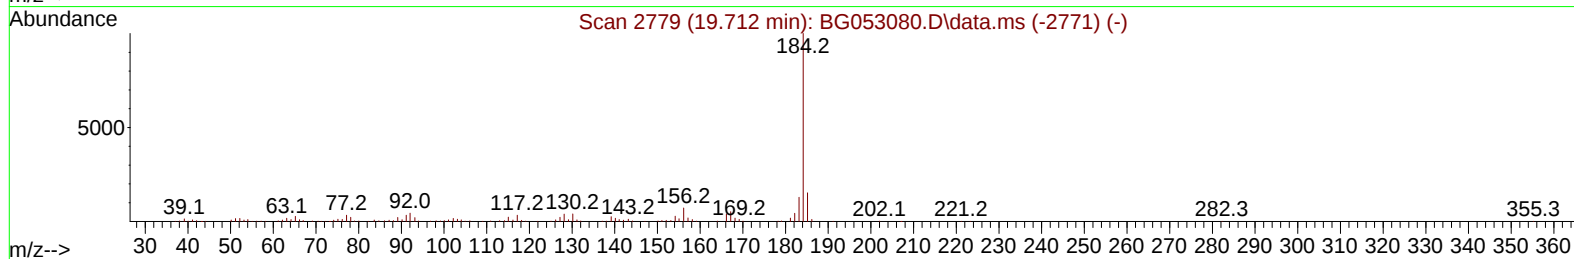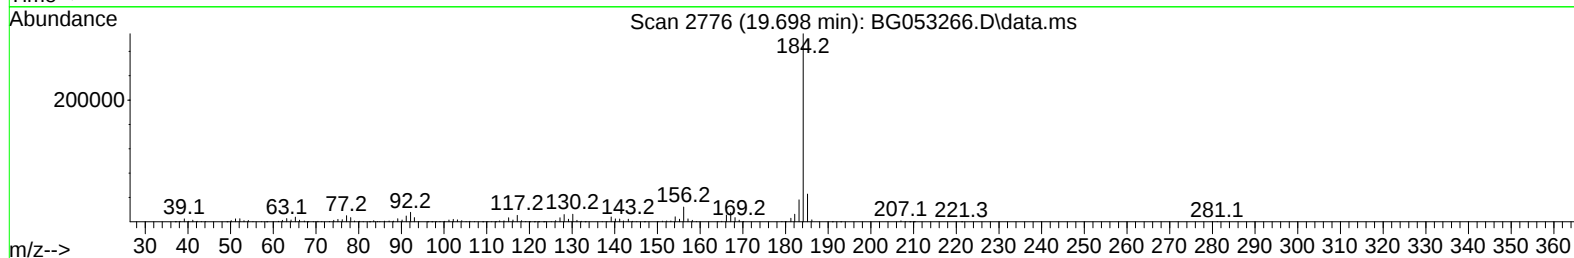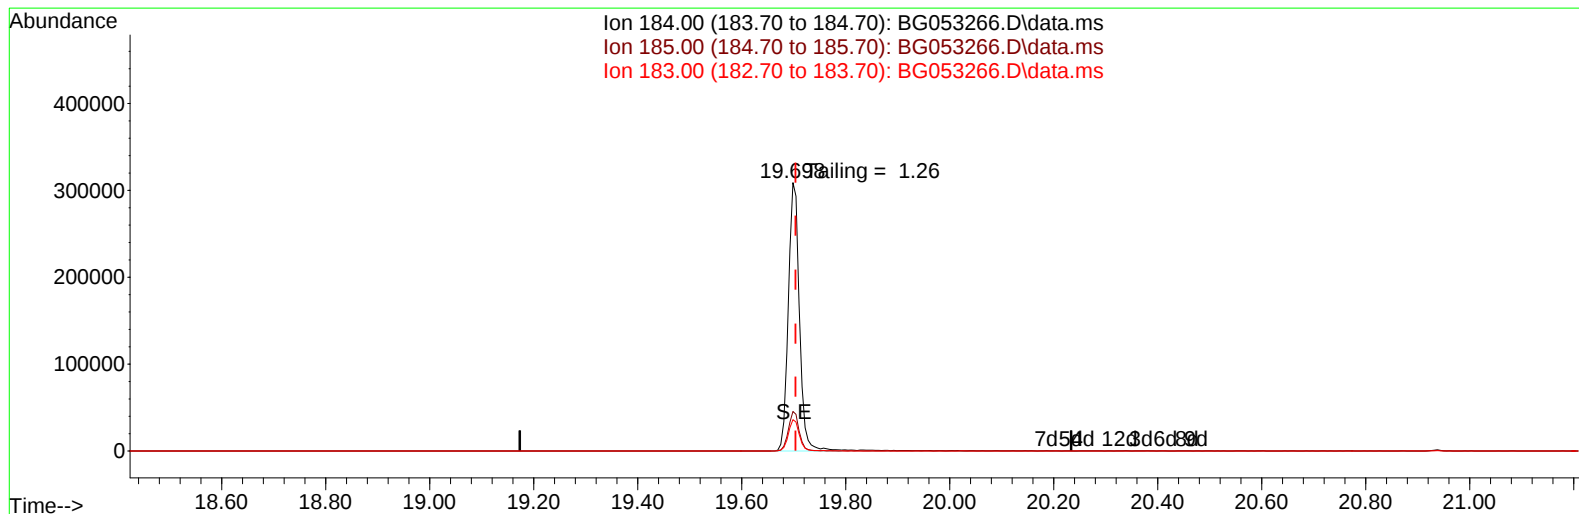

TIC: BG053266.D\data.ms

(77) Benzidine

19.698min (-0.005) 306343.28 ng m

response **471985**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.75
183.00	11.80	11.69
0.00	0.00	0.00