

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
 Data File : BG053264.D
 Acq On : 22 Apr 2022 16:57
 Operator : CG/JU
 Sample : N2487-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 UST-1-PB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.675	382	389	398	rBV	465746	757073	32.91%	8.304%
2	7.273	653	661	674	rBV	476908	853857	37.12%	9.366%
3	8.107	796	803	813	rBV2	84593	148544	6.46%	1.629%
4	9.270	993	1001	1013	rBV	306246	550626	23.94%	6.040%
5	10.921	1275	1282	1293	rVB	117876	207967	9.04%	2.281%
6	13.359	1689	1697	1706	rBV	778091	1233299	53.62%	13.528%
7	14.733	1923	1931	1939	rVB2	203886	315673	13.72%	3.463%
8	16.219	2177	2184	2200	rBV	786601	1207812	52.51%	13.249%
9	17.477	2391	2398	2405	rBV	293817	446531	19.41%	4.898%
10	20.079	2835	2841	2847	rBV	1784103	2300153	100.00%	25.231%
11	21.383	3059	3063	3070	rBV6	28810	45716	1.99%	0.501%
12	21.759	3120	3127	3135	rVB	313060	524305	22.79%	5.751%
13	25.055	3678	3688	3699	rVB2	177529	524915	22.82%	5.758%




Sum of corrected areas: 9116471

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053264.D
Acq On : 22 Apr 2022 16:57
Operator : CG/JU
Sample : N2487-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-1-PB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

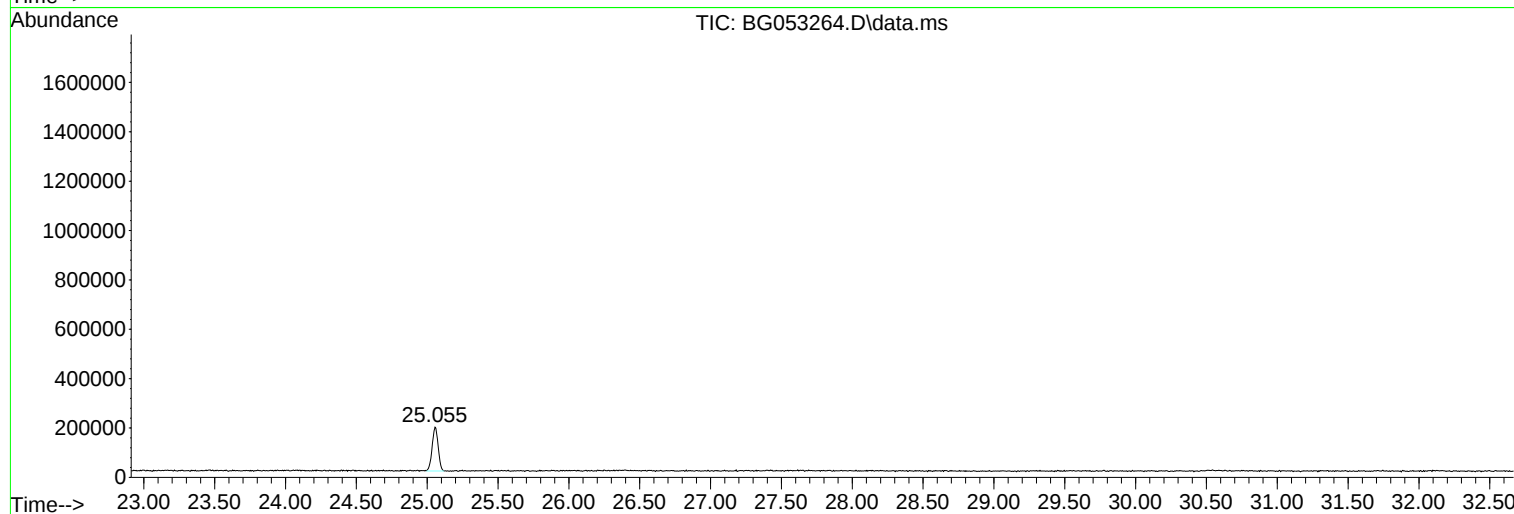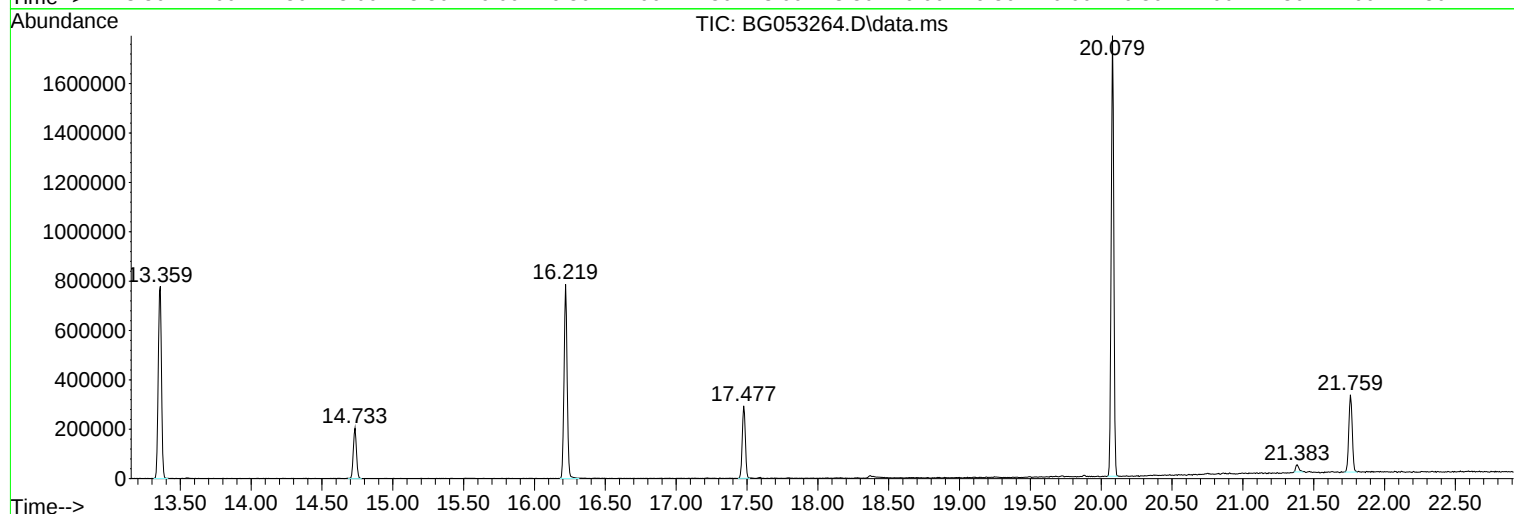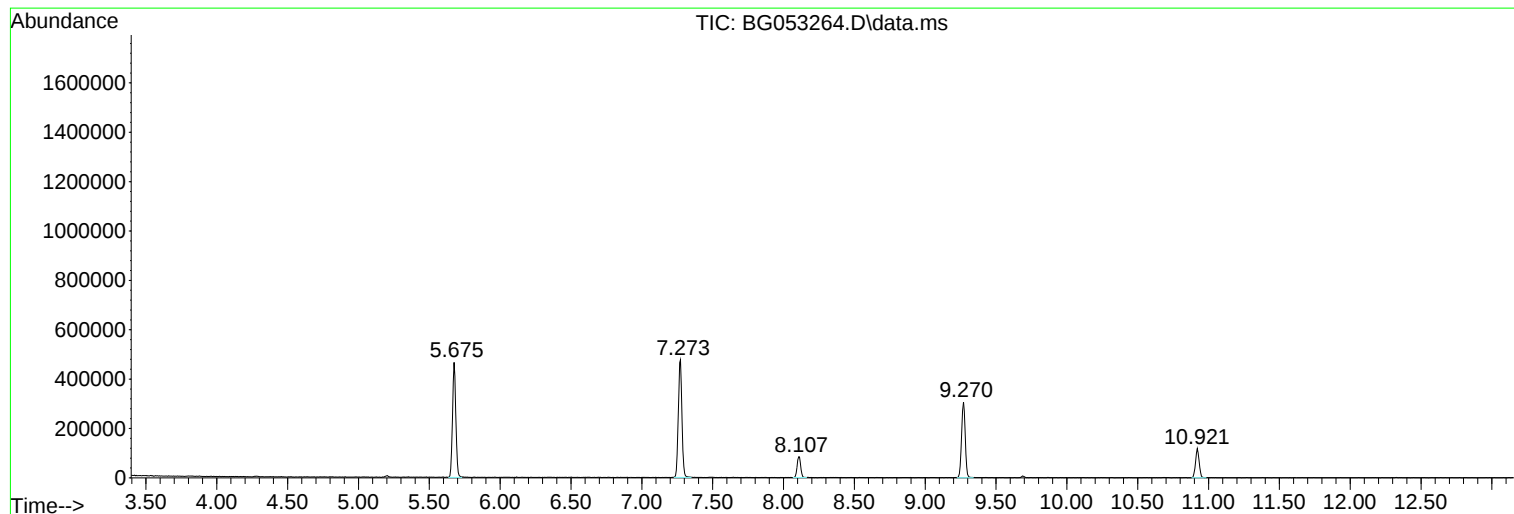

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053264.D
Acq On : 22 Apr 2022 16:57
Operator : CG/JU
Sample : N2487-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-1-PB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053264.D
Acq On : 22 Apr 2022 16:57
Operator : CG/JU
Sample : N2487-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-1-PB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------