

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
 Data File : BG053265.D
 Acq On : 22 Apr 2022 17:35
 Operator : CG/JU
 Sample : N2487-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 UST-1-N

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.673	381	389	402	rBV	510710	853001	33.25%	8.494%
2	7.271	654	661	675	rBV	547827	972682	37.91%	9.686%
3	8.111	796	804	810	rBV	85222	145270	5.66%	1.447%
4	9.268	993	1001	1013	rBV	338839	622107	24.25%	6.195%
5	10.919	1276	1282	1292	rBV	114318	204435	7.97%	2.036%
6	13.357	1690	1697	1707	rBV	909695	1393796	54.33%	13.880%
7	14.731	1923	1931	1940	rVB	206208	322701	12.58%	3.214%
8	16.217	2177	2184	2196	rBV	868829	1394235	54.35%	13.884%
9	17.475	2391	2398	2404	rBV	298241	456129	17.78%	4.542%
10	20.083	2835	2842	2848	rBV	1907949	2565437	100.00%	25.548%
11	21.381	3059	3063	3066	rBV3	25458	38954	1.52%	0.388%
12	21.763	3120	3128	3134	rBV	311019	537032	20.93%	5.348%
13	25.053	3679	3688	3700	rVB2	183564	536051	20.90%	5.338%




Sum of corrected areas: 10041830

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053265.D
Acq On : 22 Apr 2022 17:35
Operator : CG/JU
Sample : N2487-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-1-N

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

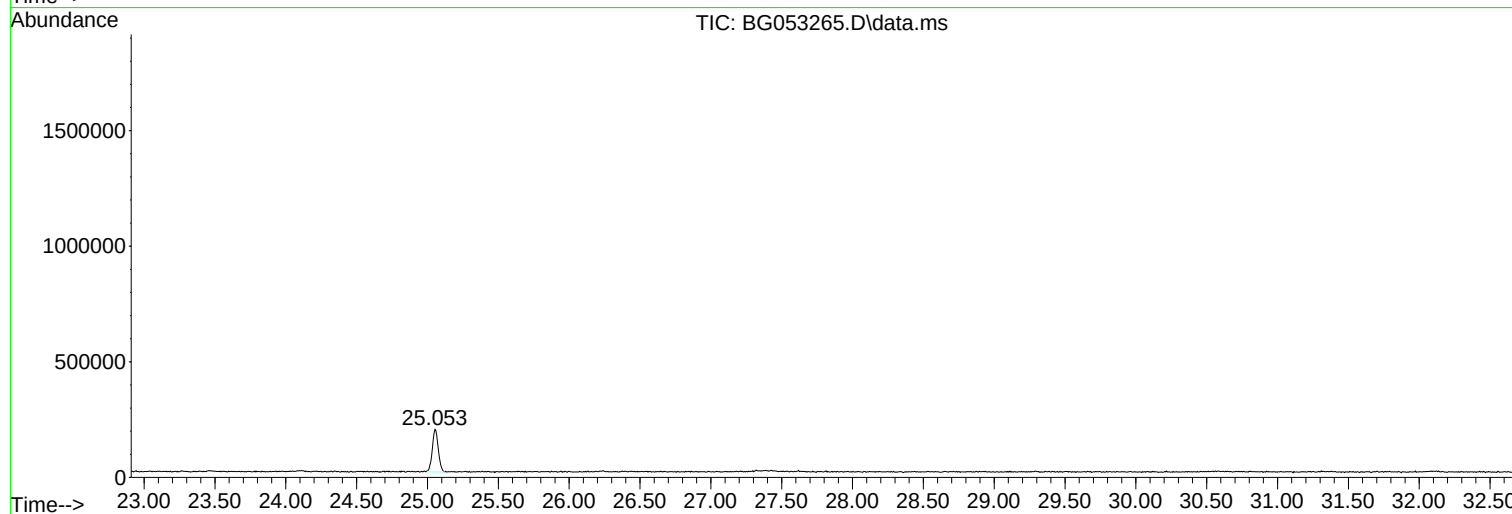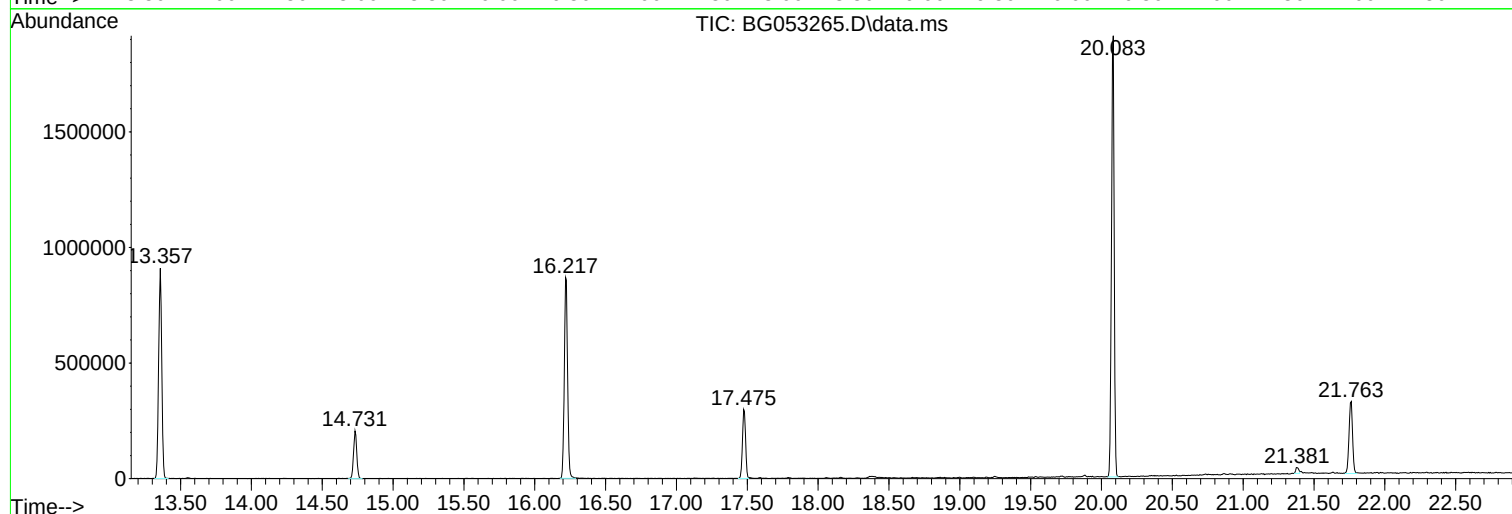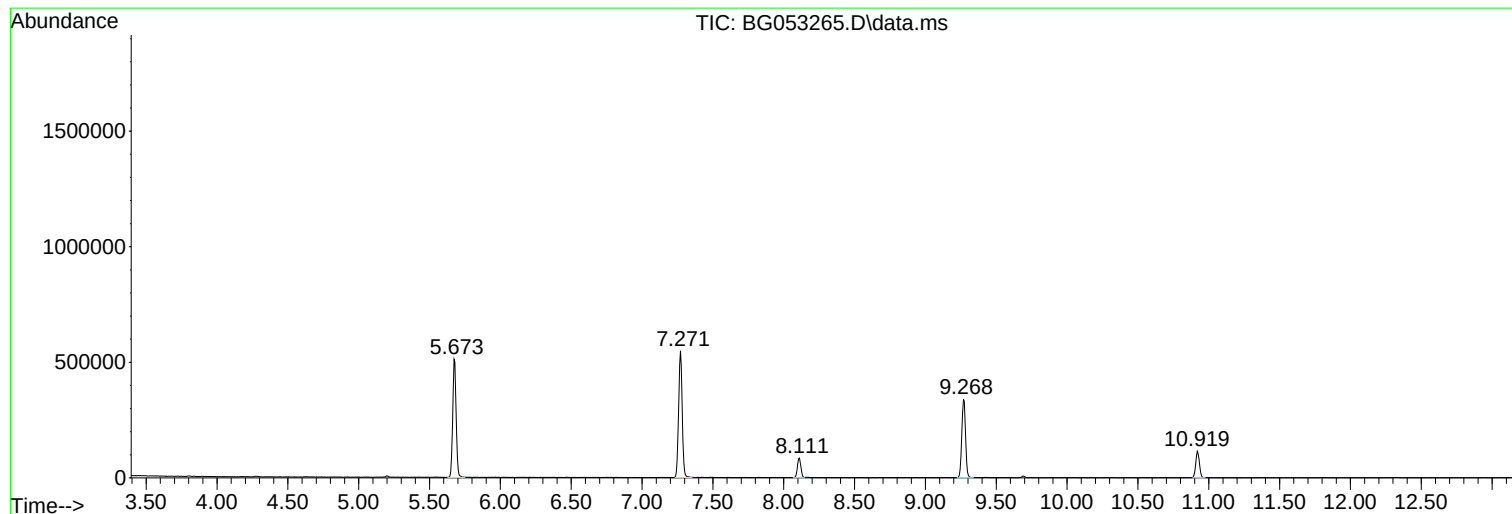

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053265.D
Acq On : 22 Apr 2022 17:35
Operator : CG/JU
Sample : N2487-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-1-N

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053265.D
Acq On : 22 Apr 2022 17:35
Operator : CG/JU
Sample : N2487-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
UST-1-N

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------